


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110422\
 Data File : BN022510.D
 Acq On : 04 Nov 2022 15:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 04 03:28:17 2022

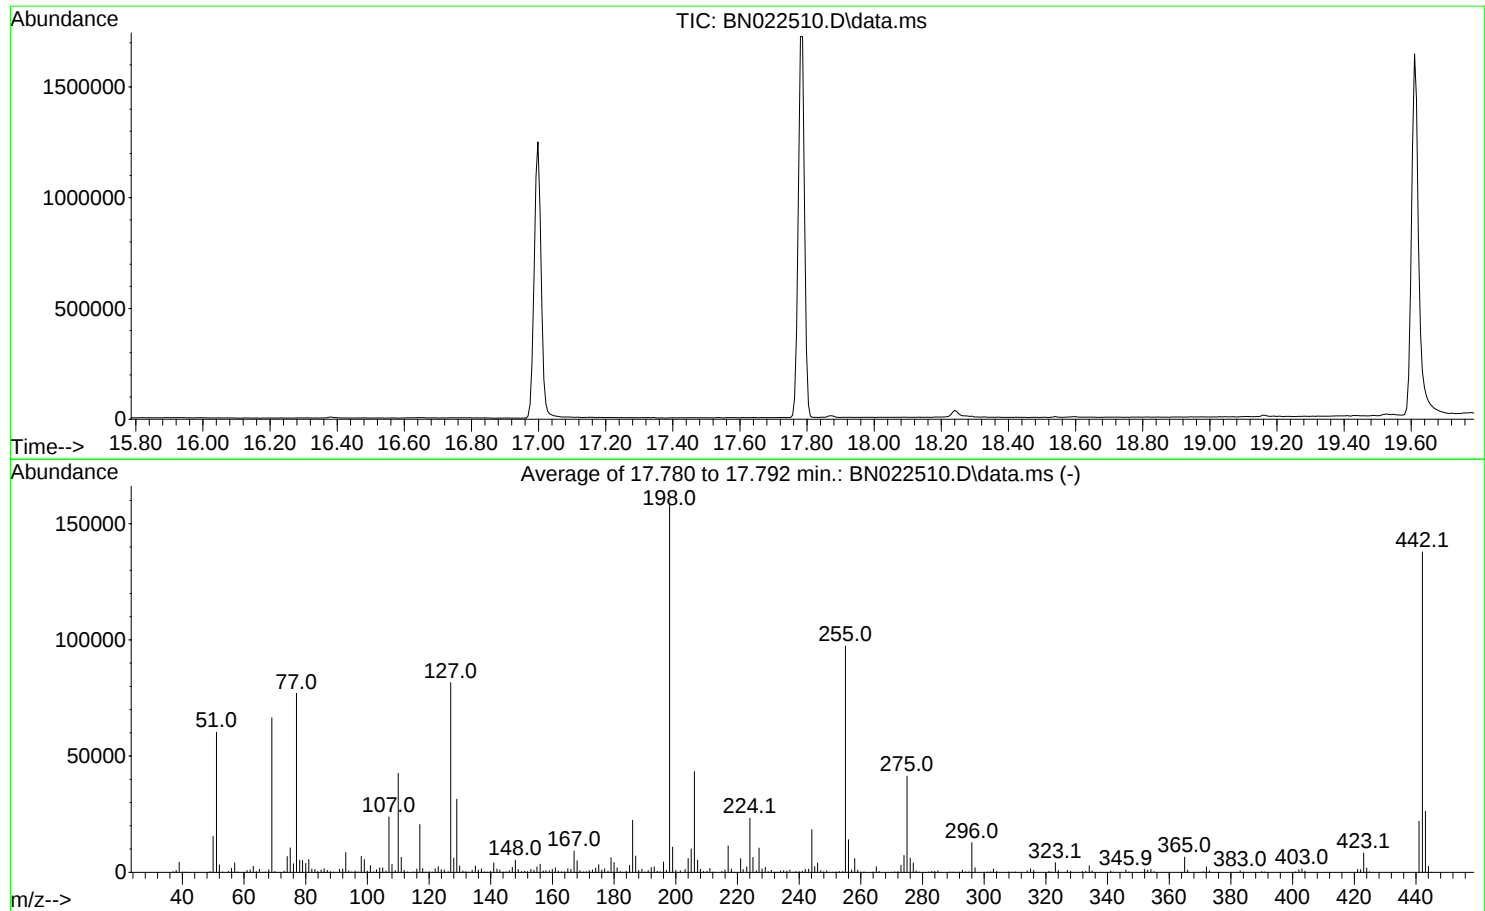




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	60296	PASS
68	69	0.00	2	1.7	1119	PASS
69	198	0.00	100	42.0	66501	PASS
70	69	0.00	2	0.6	389	PASS
127	198	10	80	51.6	81627	PASS
197	198	0.00	2	0.6	890	PASS
198	198	100	100	100.0	158307	PASS
199	198	5	9	6.9	10882	PASS
275	198	10	60	26.1	41344	PASS
365	198	1	100	4.1	6494	PASS
441	198	0.01	100	13.9	22011	PASS
442	442	50	100	100.0	137859	PASS
443	442	15	24	19.0	26205	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110422\
Data File : BN022510.D
Acq On : 04 Nov 2022 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 05 04:35:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 05 04:35:21 2022
Response via : Initial Calibration

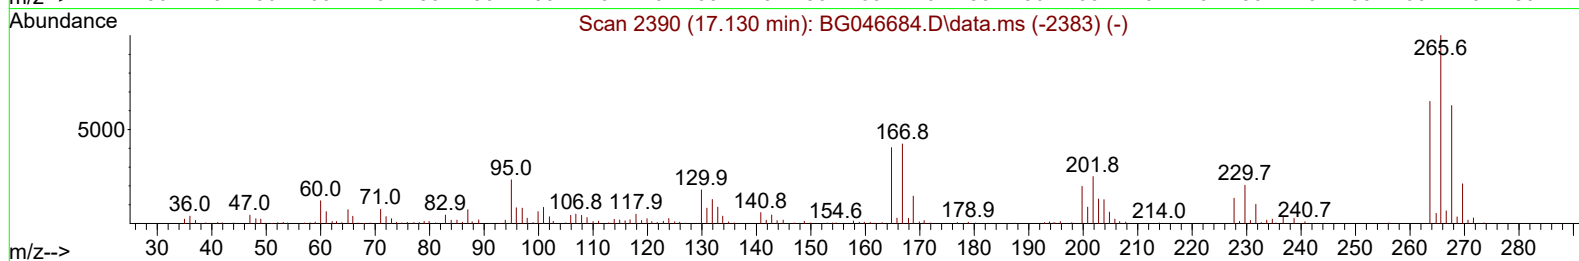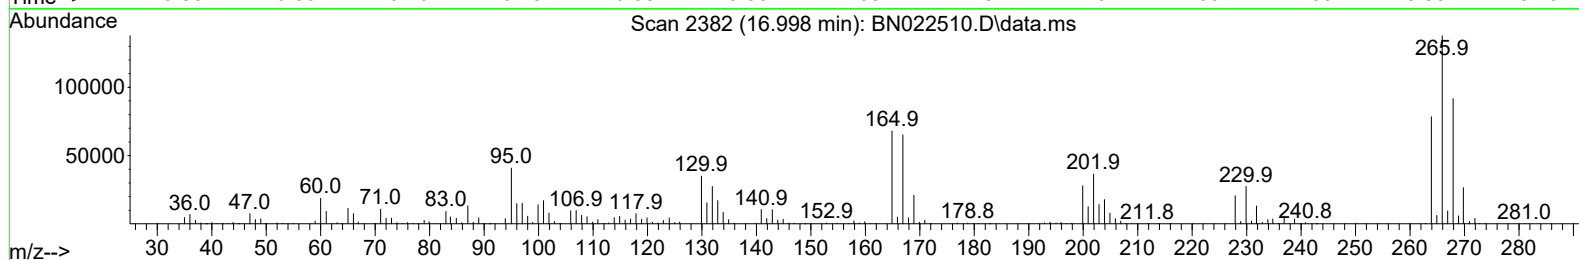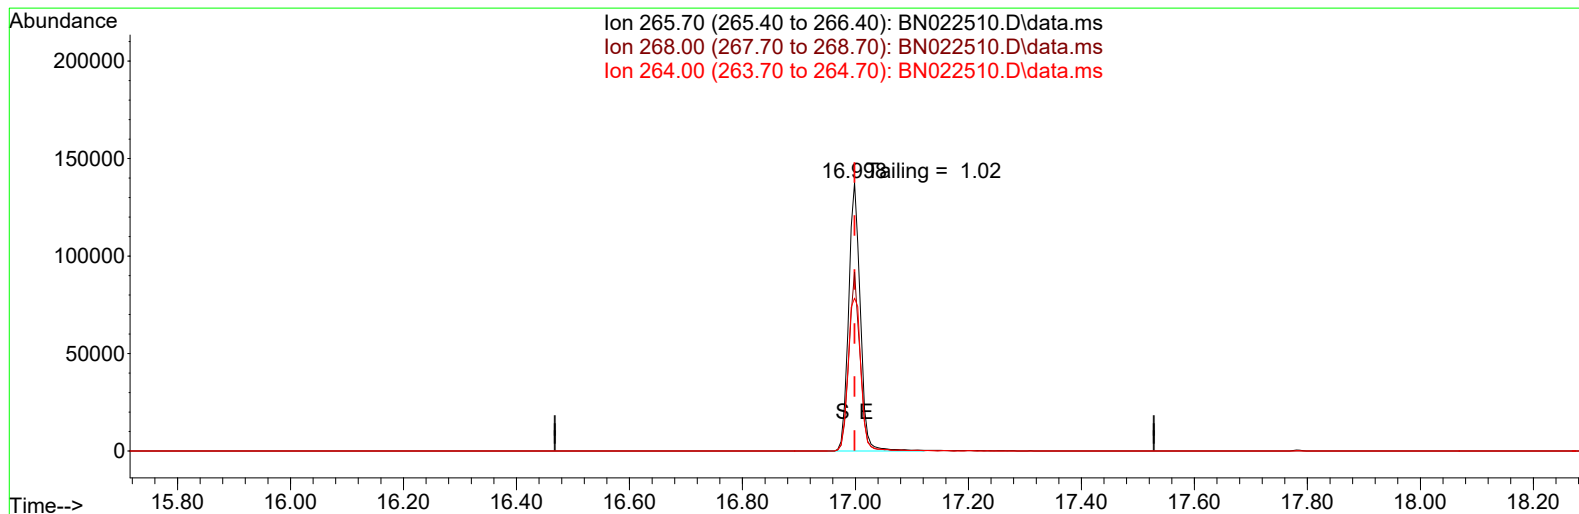

TIC: BN022510.D\data.ms

(70) Pentachlorophenol (C)

16.998min (0.000) 20796.05 ng




response 196985

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.59
264.00	61.60	56.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110422\
Data File : BN022510.D
Acq On : 04 Nov 2022 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 05 04:35:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 05 04:35:21 2022
Response via : Initial Calibration

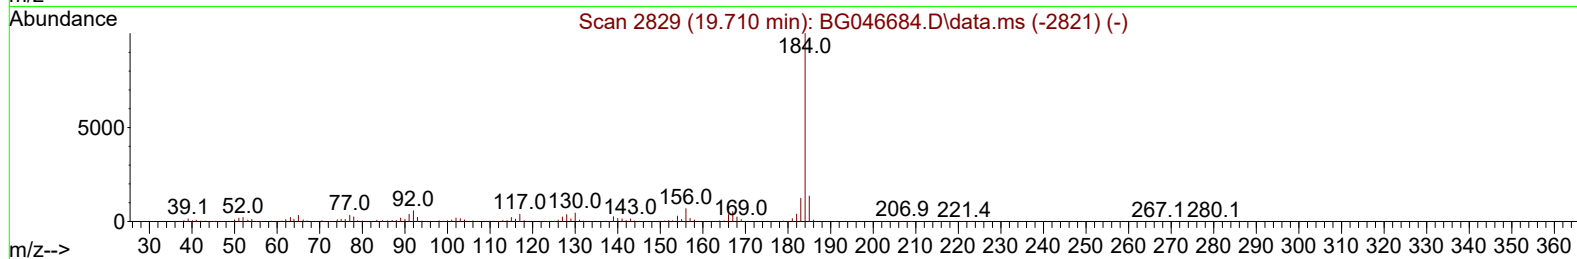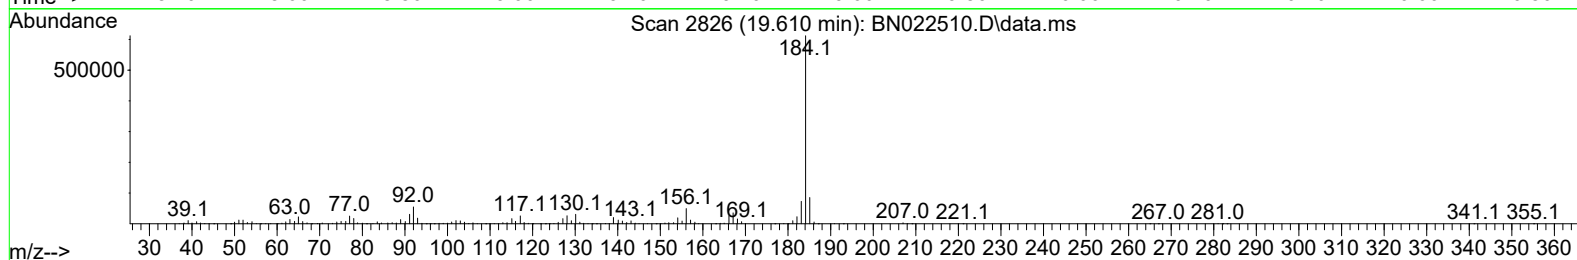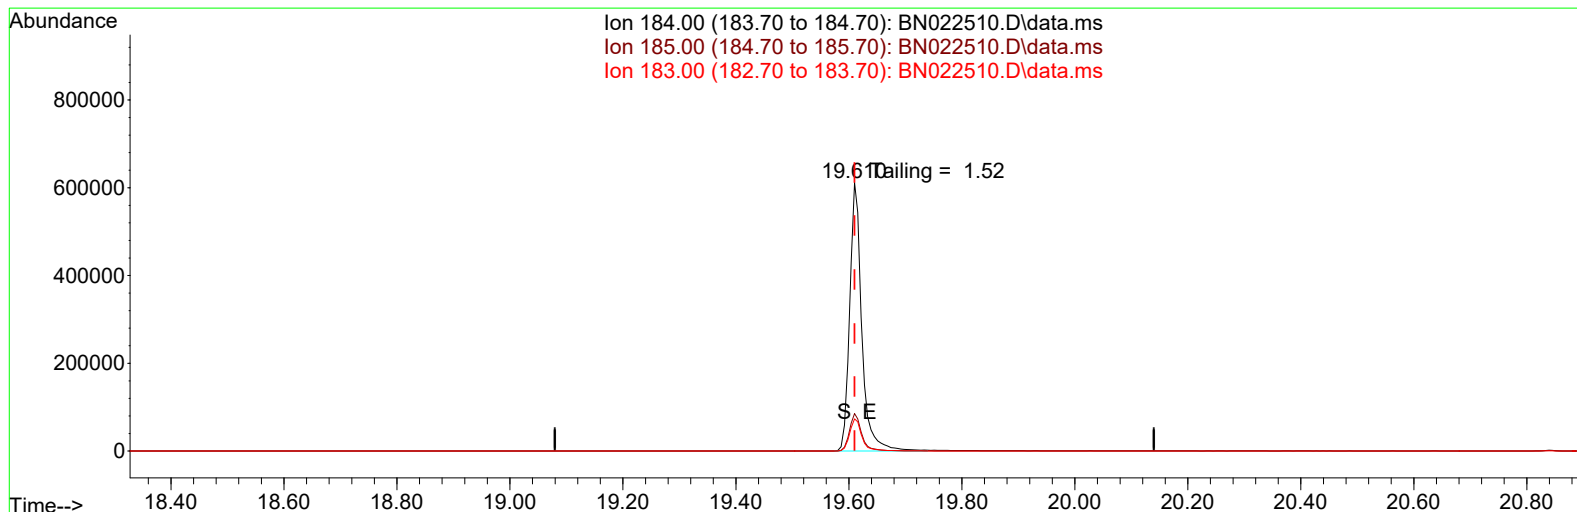

TIC: BN022510.D\data.ms

(77) Benzidine

19.610min (0.000) 0.00 ng

response 916998

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2022	BNA_N	<u>BN022510.D</u>
Compound Name	Response	Retention Time
DDT	360065	20.839
DDD	102546	20.398
DDE	57	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
102603	462668	22.18

Instrument :
BNA_N
ClientSampleId :
DFTPP