
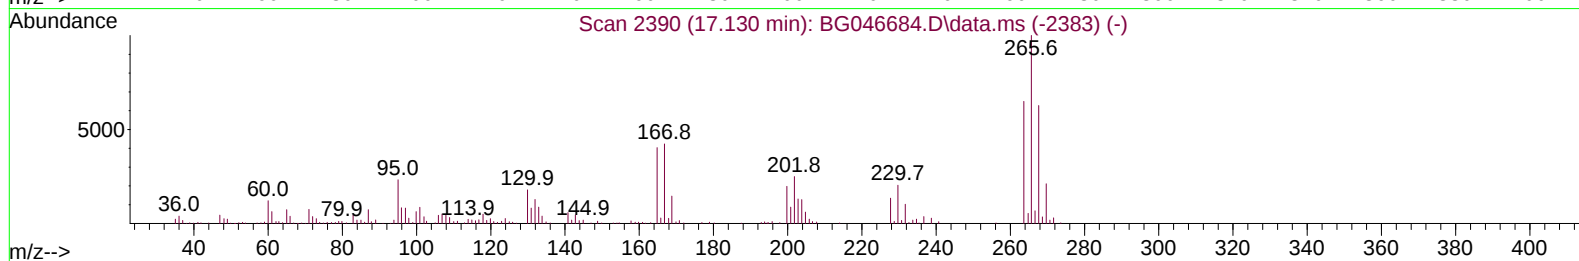
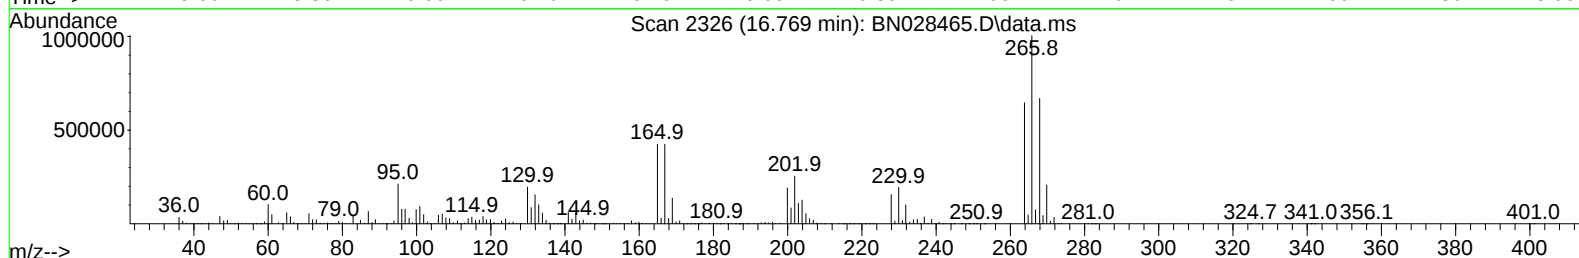


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110423\
Data File : BN028465.D
Acq On : 04 Nov 2023 09:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 05:19:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 05:19:43 2023
Response via : Initial Calibration

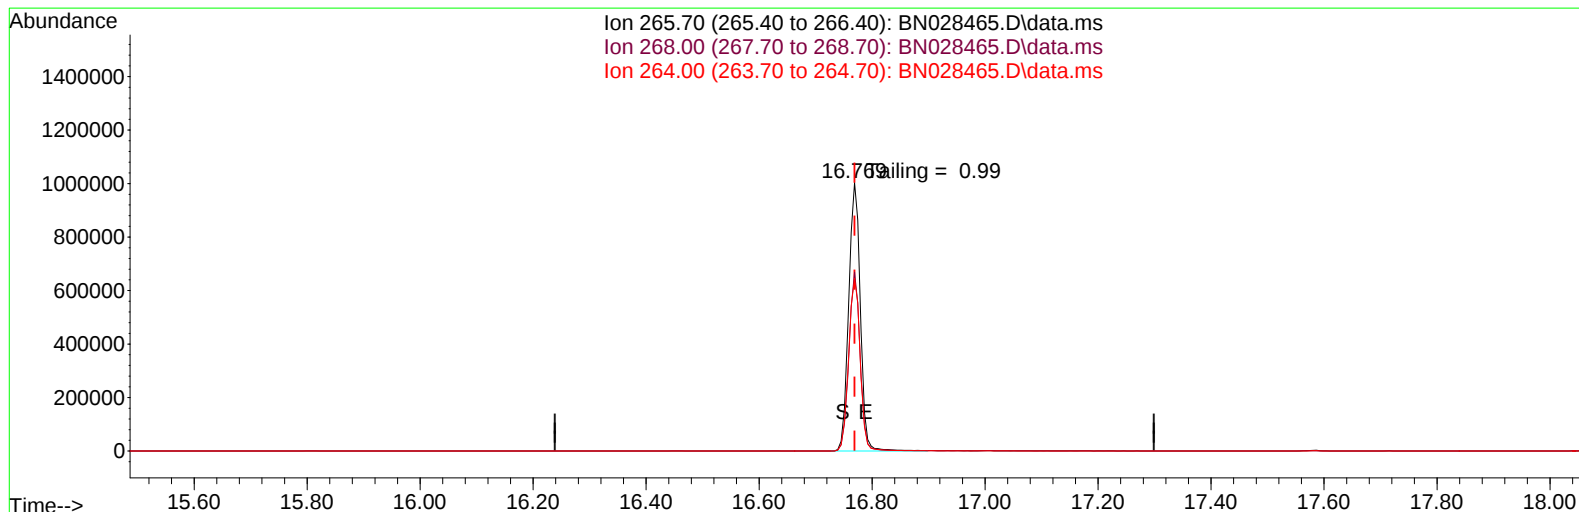

TIC: BN028465.D\data.ms

(70) Pentachlorophenol (C)




16.769min (0.000) 24822.81 ng

response 1438816

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.67
264.00	61.60	64.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110423\
Data File : BN028465.D
Acq On : 04 Nov 2023 09:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 05:19:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 05:19:43 2023
Response via : Initial Calibration

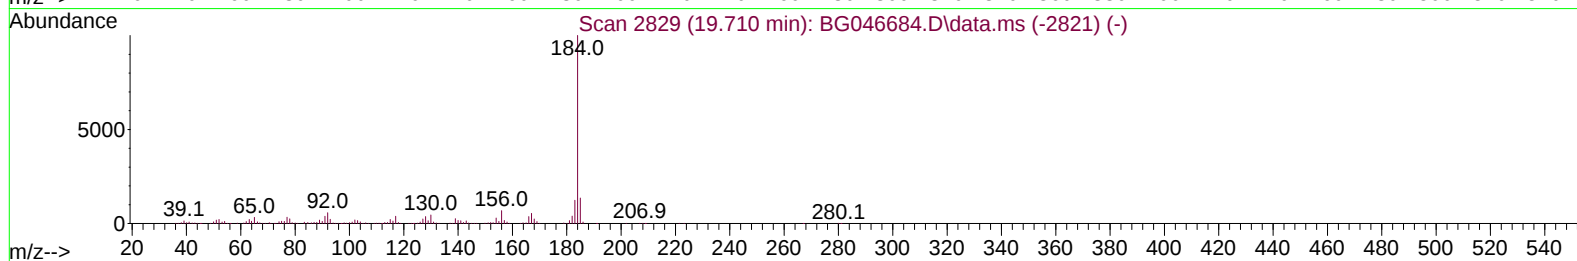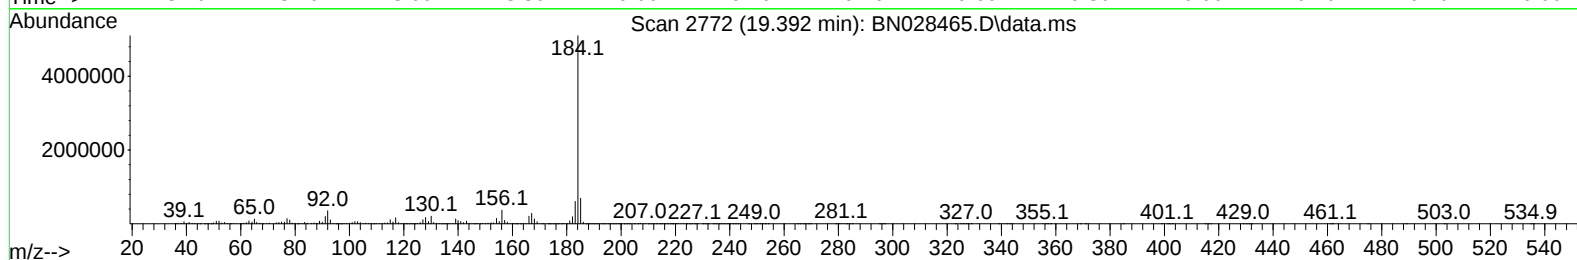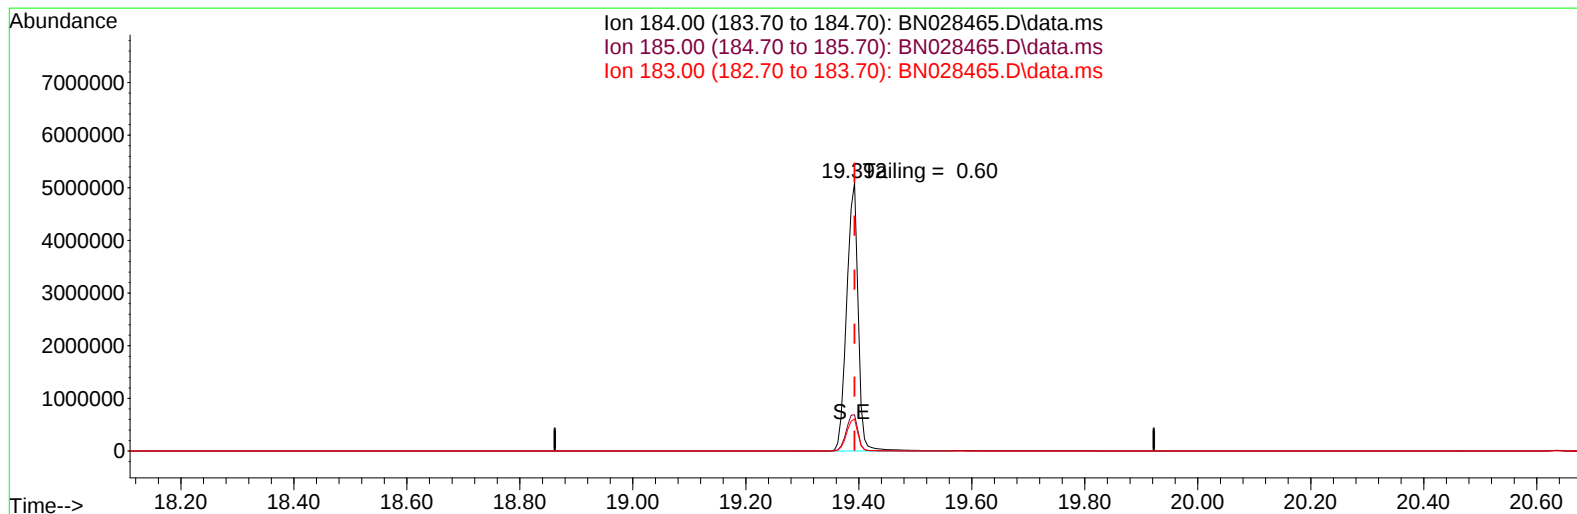

TIC: BN028465.D\data.ms

(77) Benzidine**19.392min (0.000) 3161262.59 ng****response 7211085**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.50
183.00	13.20	11.94
0.00	0.00	0.00