


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110423\
Data File : BN028465.D
Acq On : 04 Nov 2023 09:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 02 06:26:50 2023

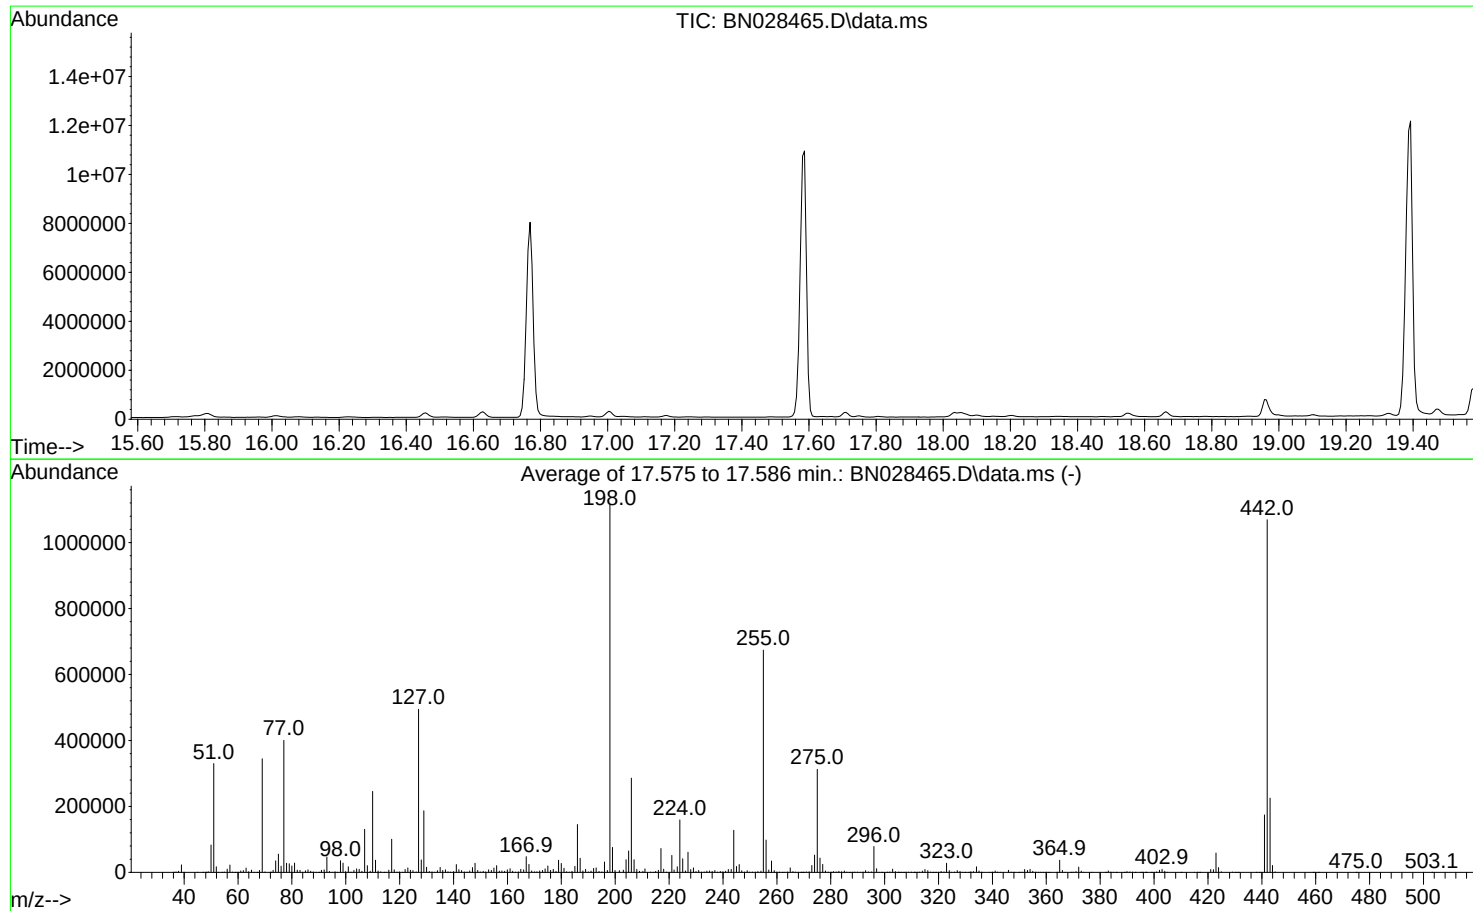




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2454

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	29.6	329755	PASS
68	69	0.00	2	1.7	5698	PASS
69	198	0.00	100	30.9	344519	PASS
70	69	0.00	2	0.4	1468	PASS
127	198	10	80	44.3	494615	PASS
197	198	0.00	2	0.5	5968	PASS
198	198	100	100	100.0	1115392	PASS
199	198	5	9	6.8	75642	PASS
275	198	10	60	28.0	312448	PASS
365	198	1	100	3.3	36717	PASS
441	198	0.01	100	15.6	174448	PASS
442	442	50	100	100.0	1069141	PASS
443	442	15	24	21.0	225024	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110423\
Data File : BN028465.D
Acq On : 04 Nov 2023 09:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 06 05:19:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 05:19:43 2023
Response via : Initial Calibration

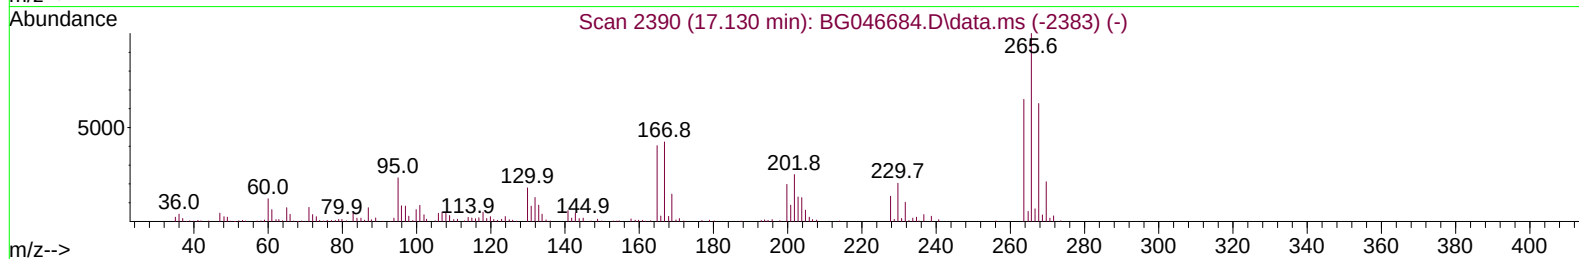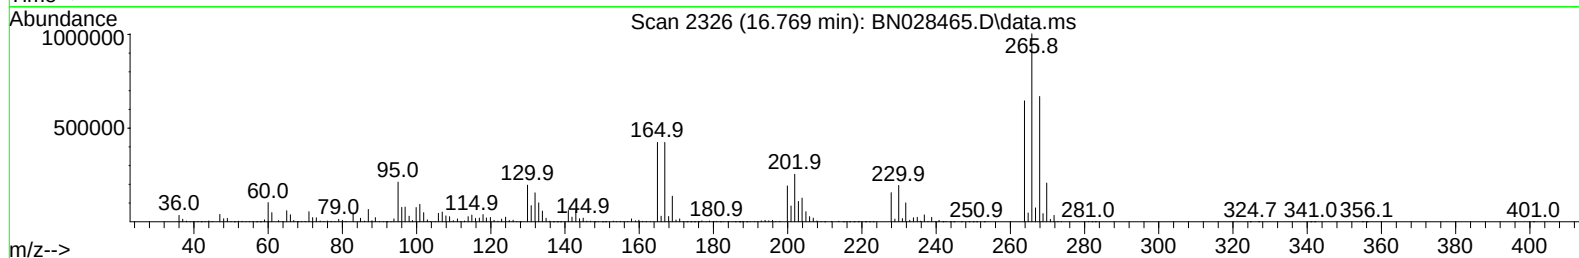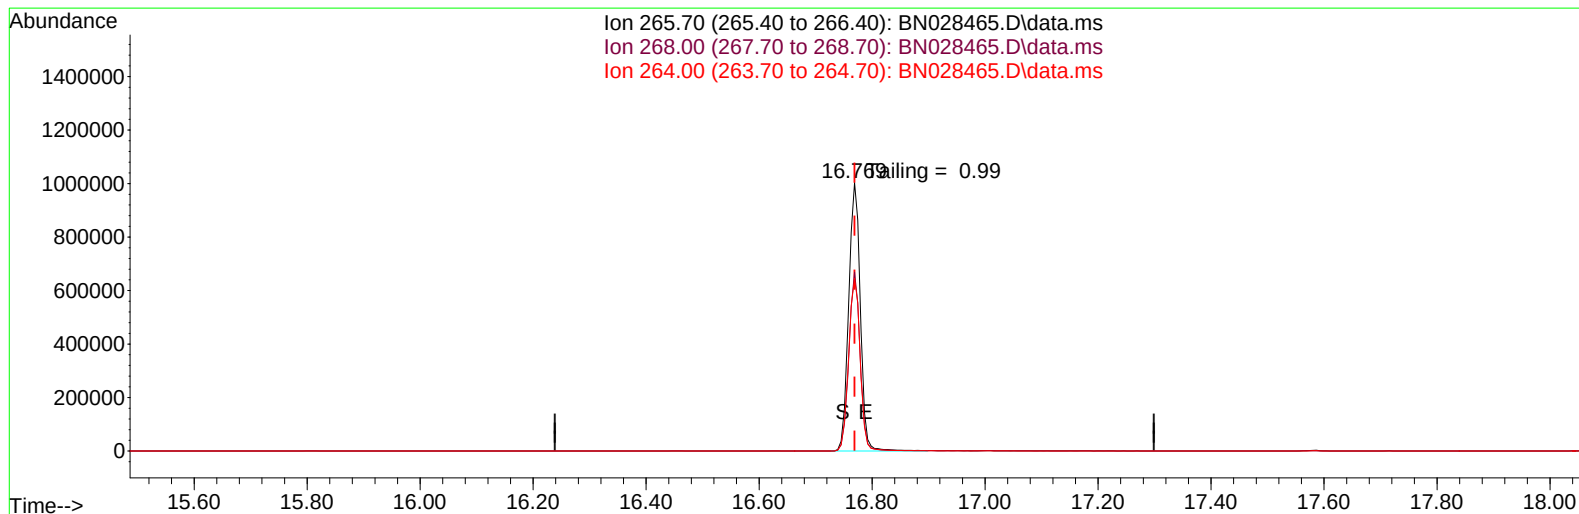

TIC: BN028465.D\data.ms

(70) Pentachlorophenol (C)

16.769min (0.000) 24822.81 ng




response 1438816

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.67
264.00	61.60	64.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110423\
 Data File : BN028465.D
 Acq On : 04 Nov 2023 09:22
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 06 05:19:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 06 05:19:43 2023
 Response via : Initial Calibration

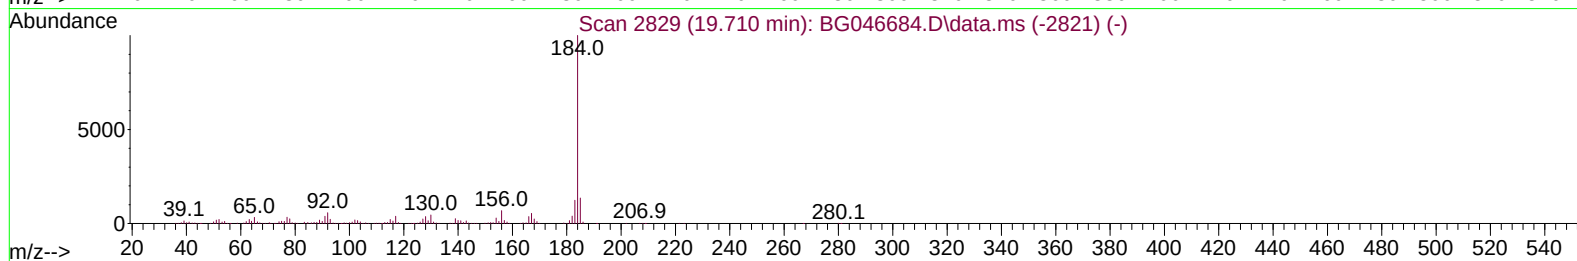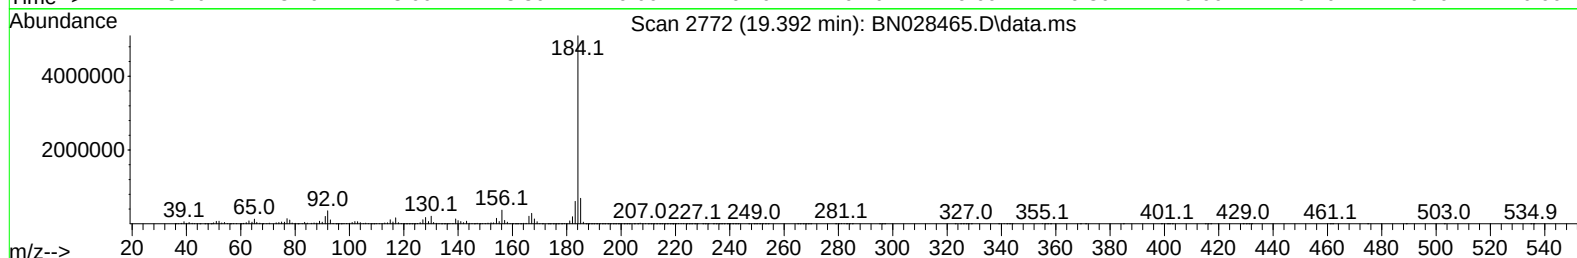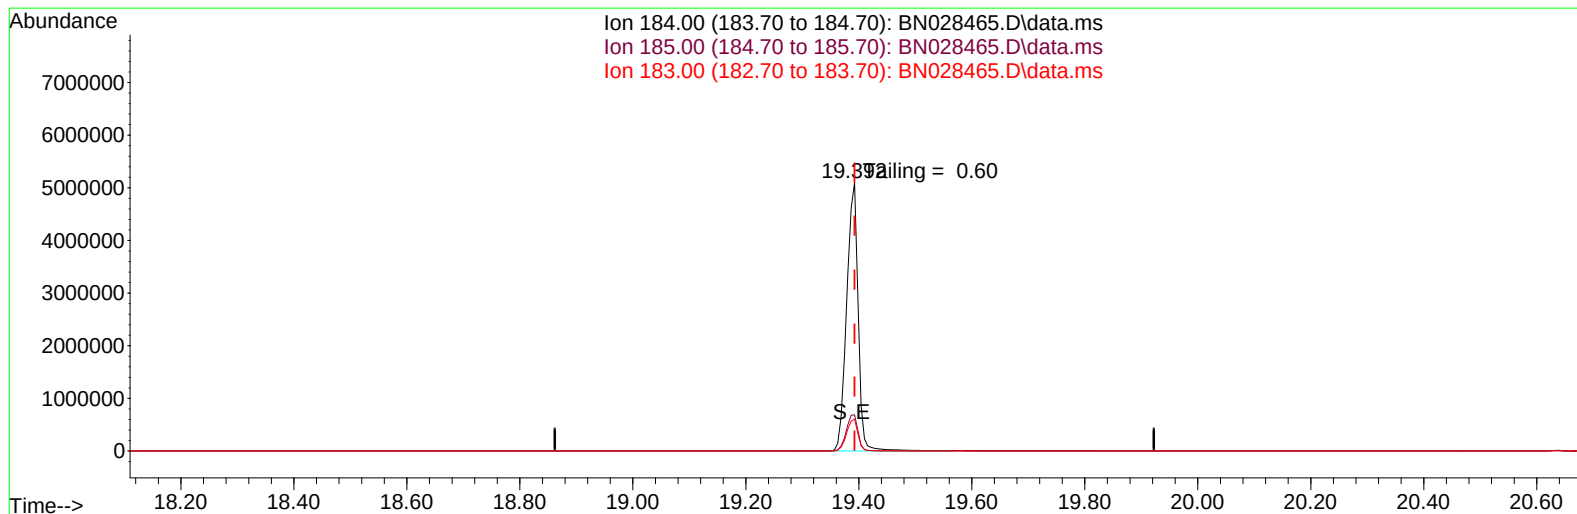

TIC: BN028465.D\data.ms

(77) Benzidine**19.392min (0.000) 3161262.59 ng****response 7211085**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.50
183.00	13.20	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2023	BNA_N	<u>BN028465.D</u>
Compound Name	Response	Retention Time
DDT	3813348	20.633
DDD	198775	20.186
DDE	4665	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
203440	4016788	5.06

Instrument :
BNA_N
ClientSampleId :
DFTPP