
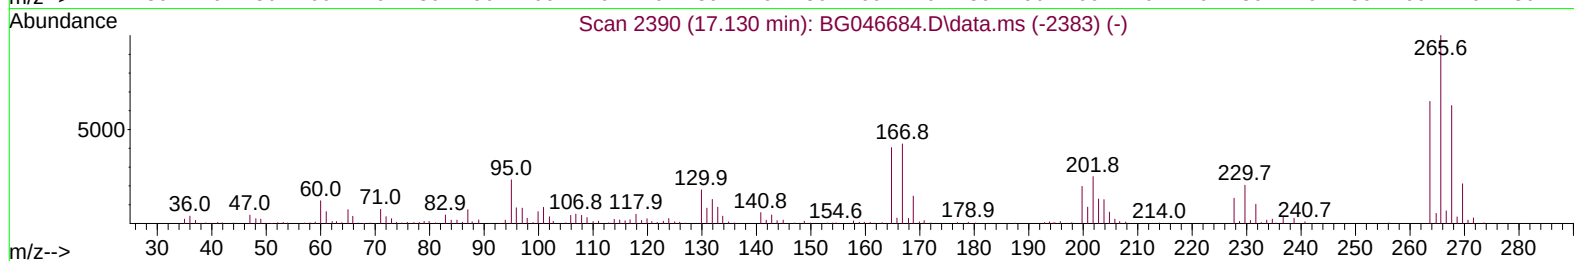
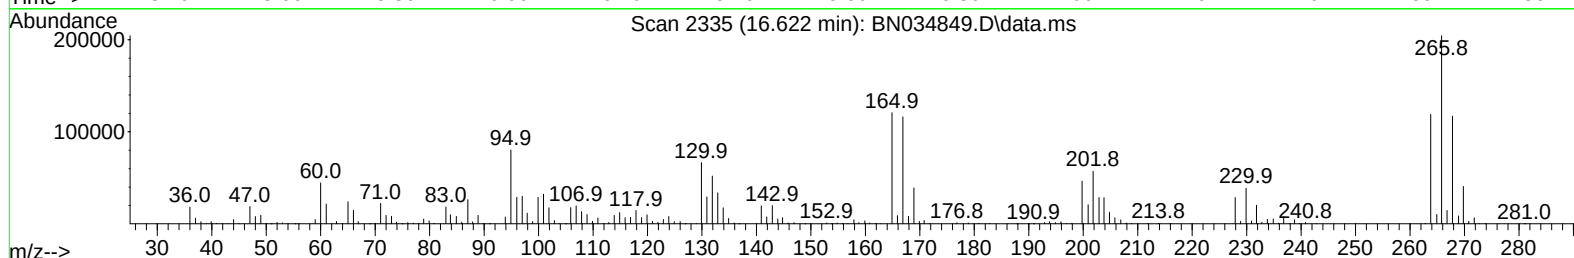


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110424\
Data File : BN034849.D
Acq On : 04 Nov 2024 20:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 23:56:03 2024
Response via : Initial Calibration

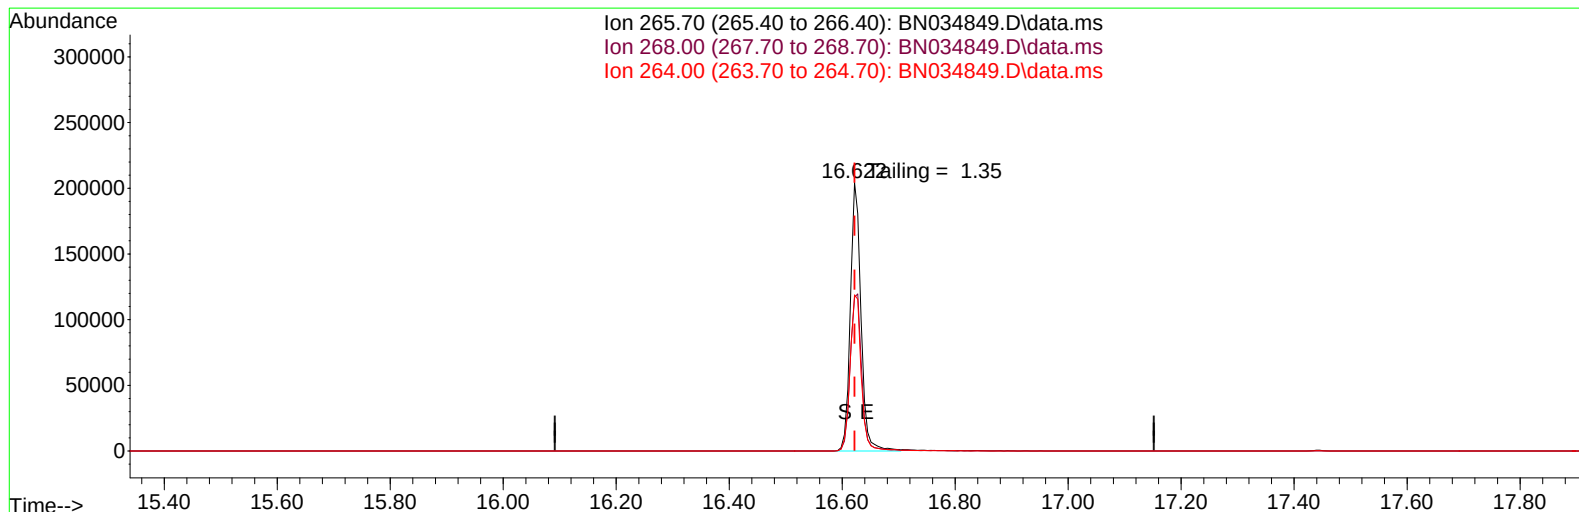

TIC: BN034849.D\data.ms

(70) Pentachlorophenol (C)




16.622min (0.000) 21272.94 ng

response 271619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.32
264.00	61.60	58.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110424\
Data File : BN034849.D
Acq On : 04 Nov 2024 20:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 23:56:03 2024
Response via : Initial Calibration

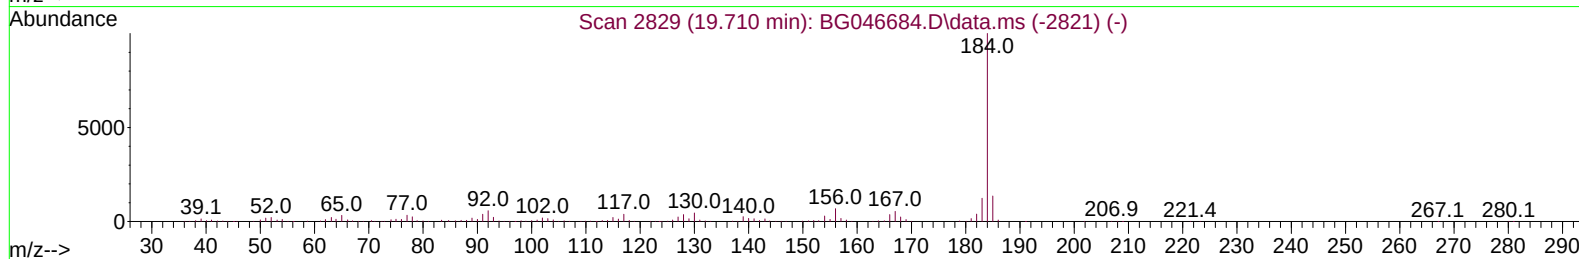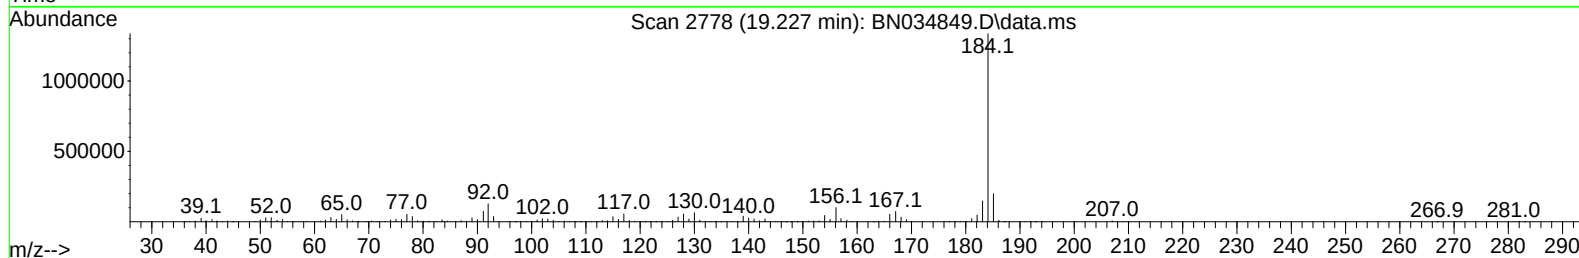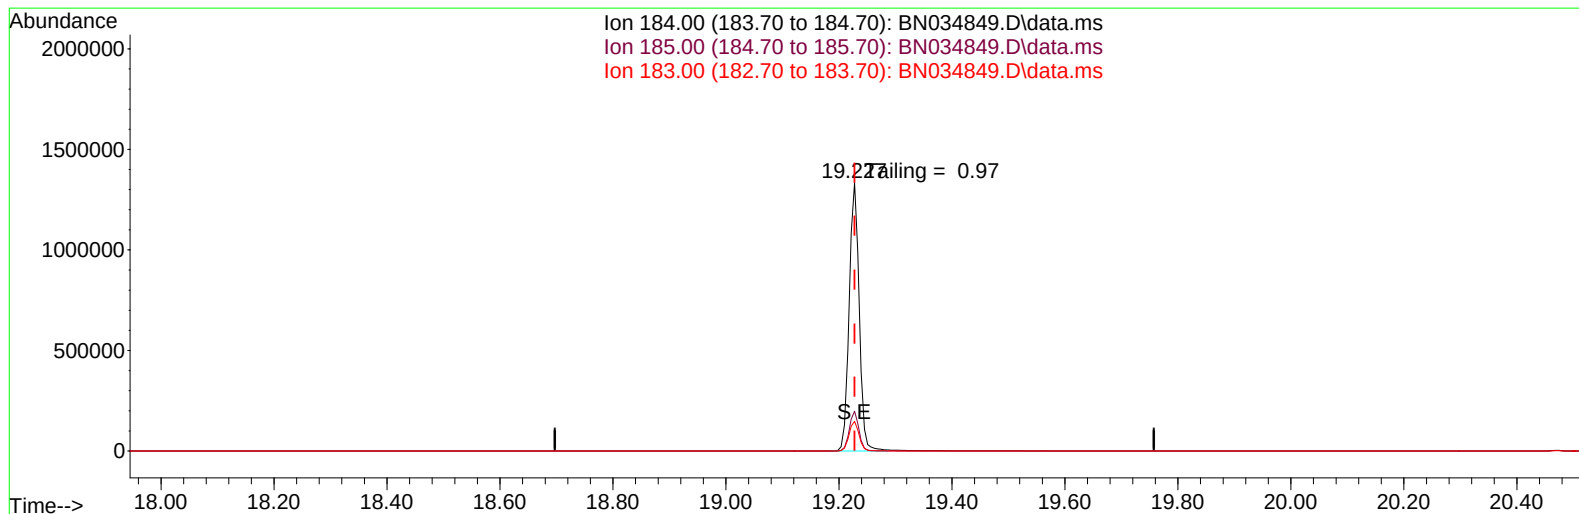

TIC: BN034849.D\data.ms

(77) Benzidine

19.227min (0.000) 0.00 ng

response 1662756

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.88
183.00	13.20	11.04
0.00	0.00	0.00