
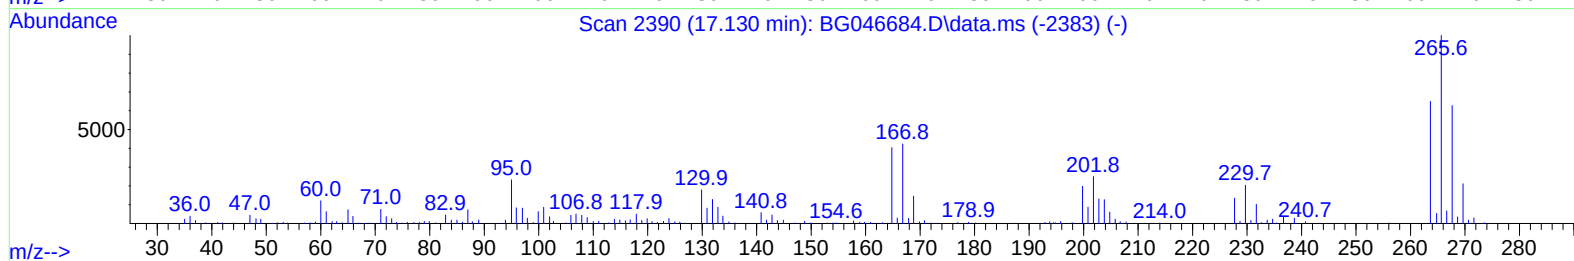
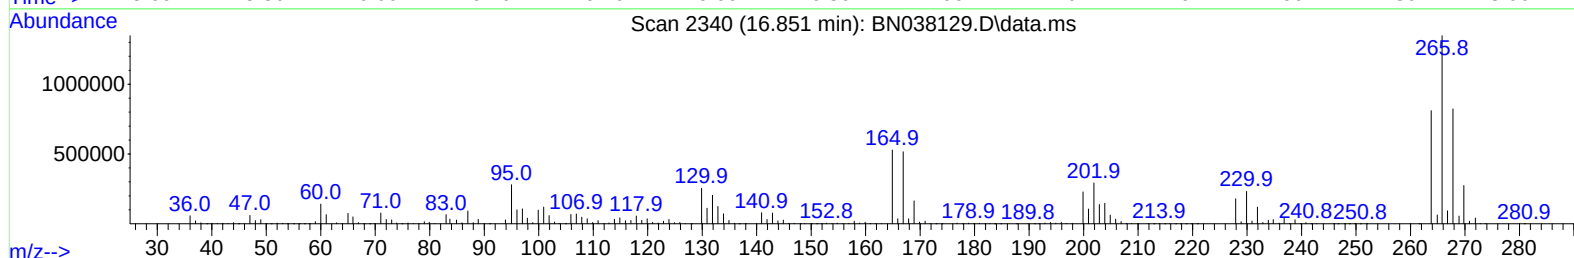


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110425\
Data File : BN038129.D
Acq On : 04 Nov 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 14:05:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 04 14:05:21 2025
Response via : Initial Calibration

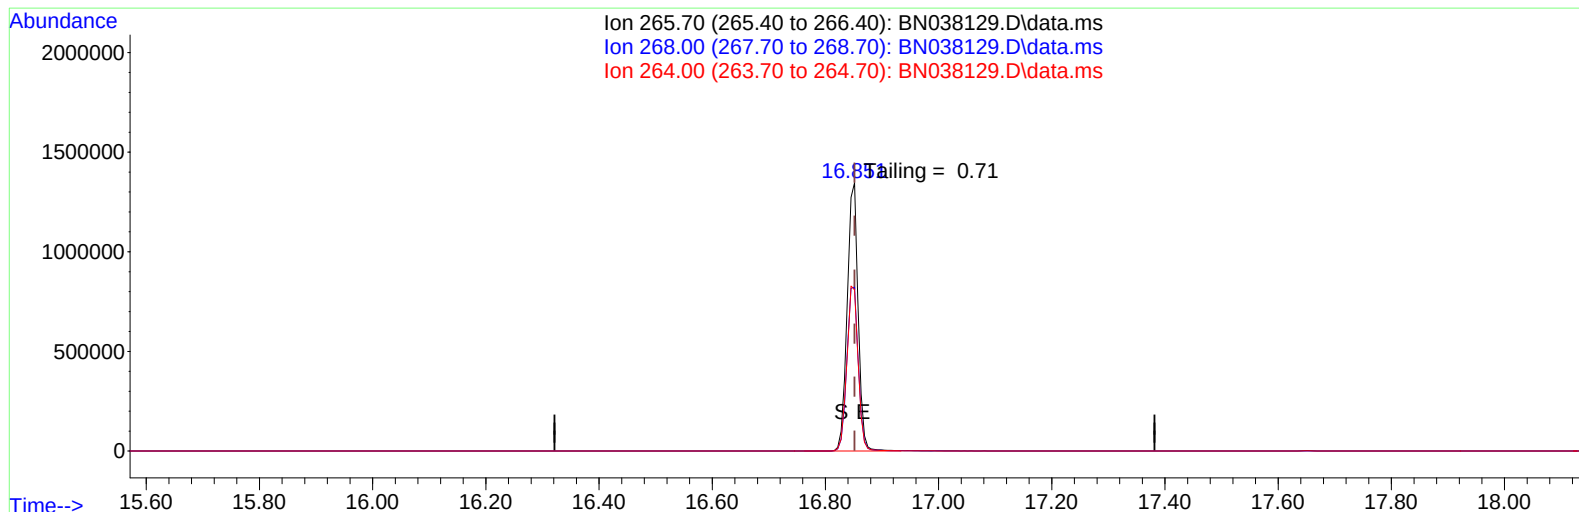

TIC: BN038129.D\data.ms

(70) Pentachlorophenol (C)




16.851min (0.000) 277.93 ng

response 1813451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.08
264.00	61.60	60.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110425\
Data File : BN038129.D
Acq On : 04 Nov 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 14:05:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 04 14:05:21 2025
Response via : Initial Calibration

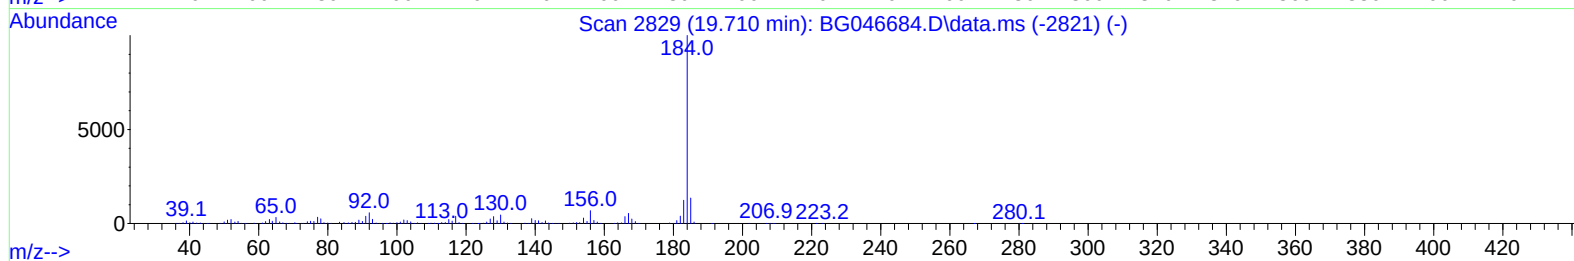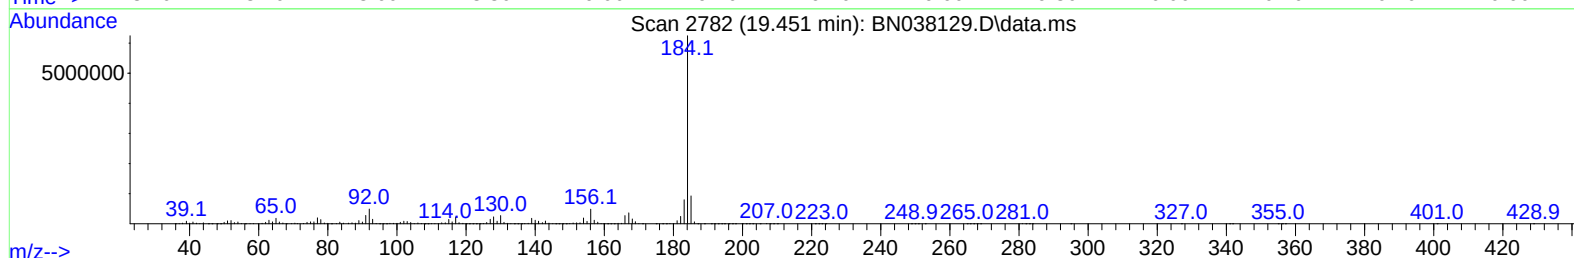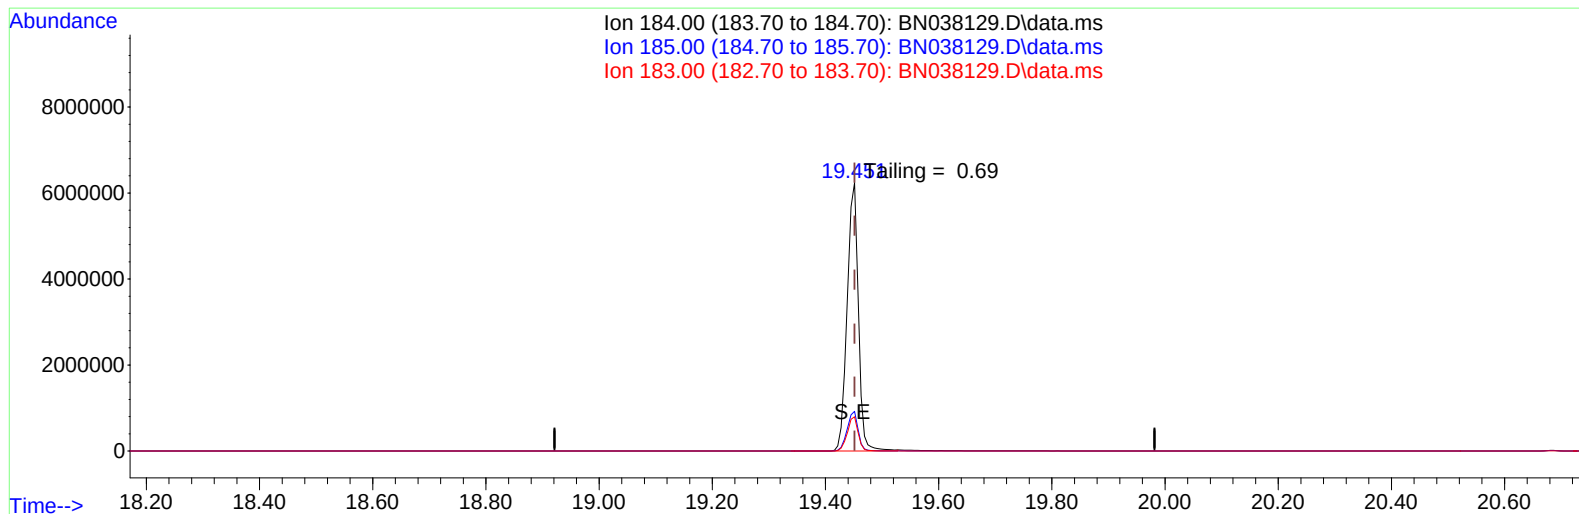

TIC: BN038129.D\data.ms

(77) Benzidine

19.451min (0.000) 0.00 ng

response 8673581

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.80
183.00	13.20	12.79
0.00	0.00	0.00