
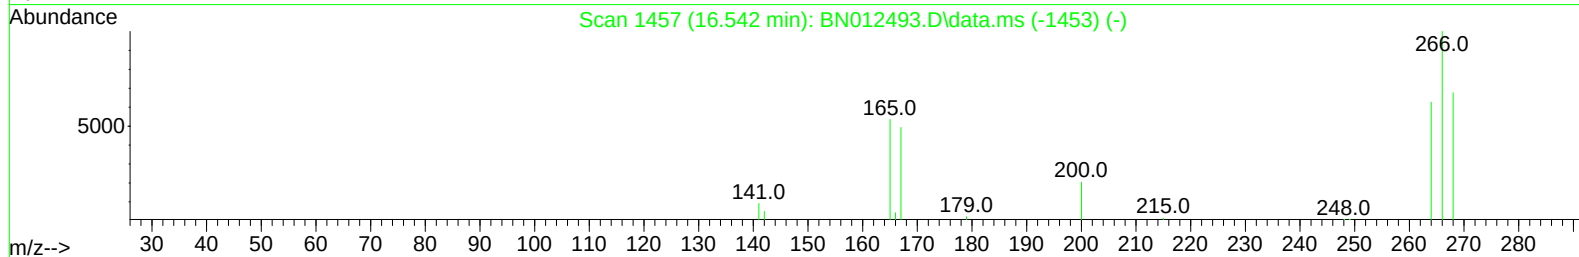
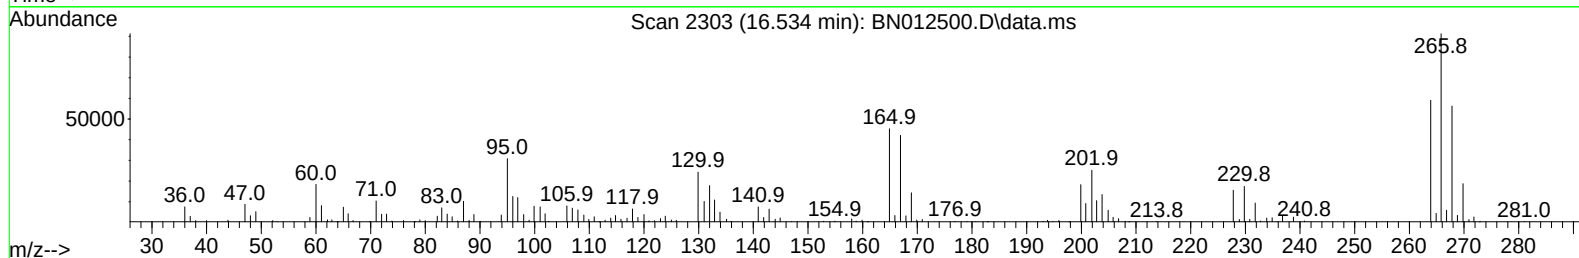


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110520\
Data File : BN012500.D
Acq On : 05 Nov 2020 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 03:44:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 05 05:46:47 2020
Response via : Initial Calibration

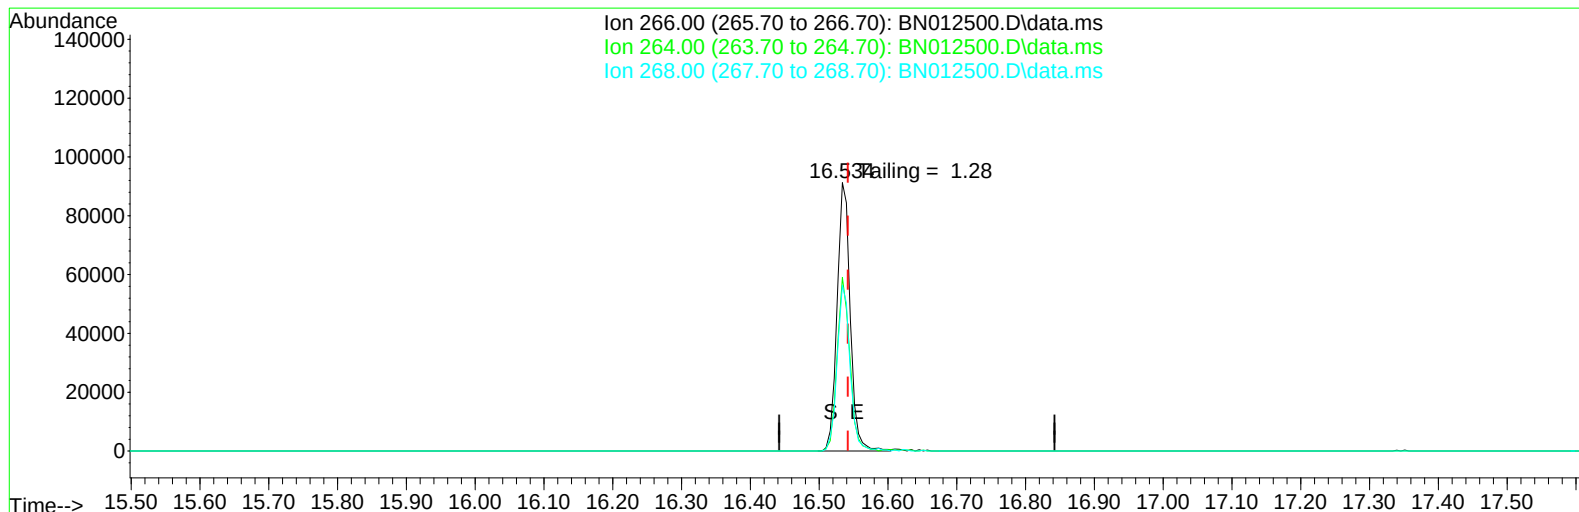

TIC: BN012500.D\data.ms

(24) Pentachlorophenol

16.534min (-0.008) 0.00 ng

response 121193

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.61
268.00	64.40	60.94
0.00	0.00	0.00