
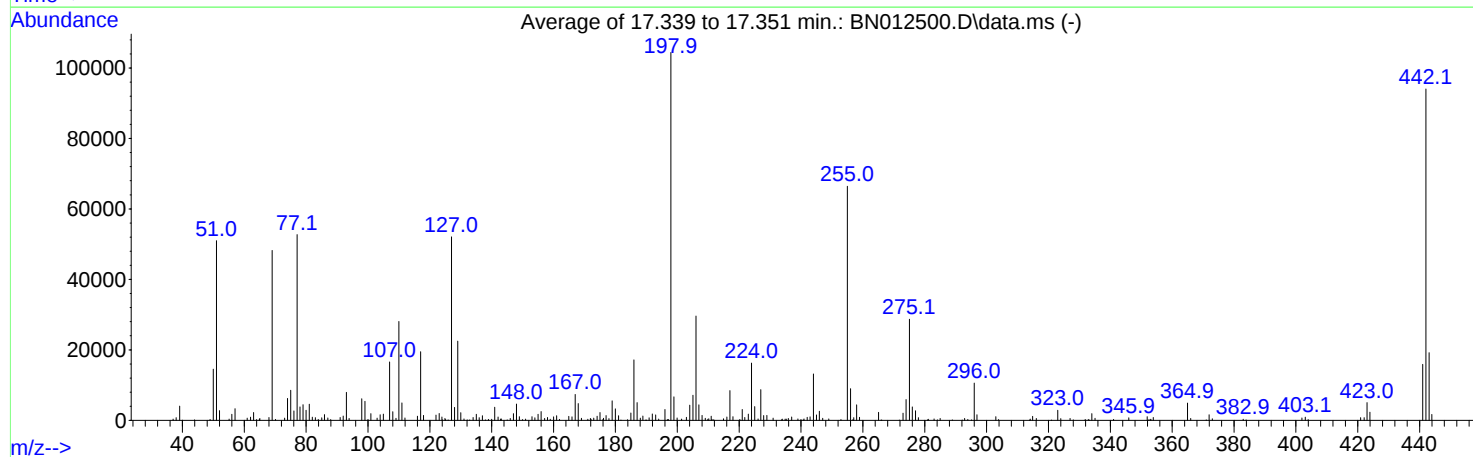


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110520\
 Data File : BN012500.D
 Acq On : 05 Nov 2020 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 05 05:46:47 2020

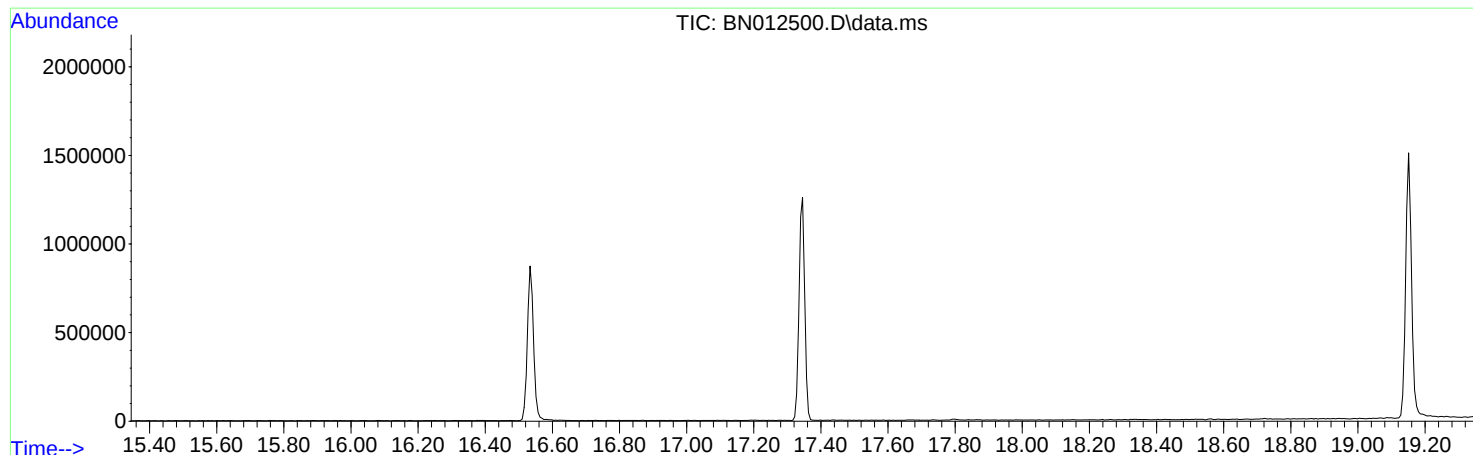

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	50989	PASS
68	69	0.00	2	1.7	820	PASS
69	198	0.00	100	46.2	48211	PASS
70	69	0.00	2	0.6	277	PASS
127	198	10	80	49.9	52107	PASS
197	198	0.00	2	0.3	272	PASS
198	198	100	100	100.0	104392	PASS
199	198	5	9	6.4	6685	PASS
275	198	10	60	27.5	28717	PASS
365	198	1	100	4.7	4884	PASS
441	198	0.01	100	15.2	15917	PASS
442	198	50	100	90.1	94056	PASS
443	442	15	24	20.4	19216	PASS