
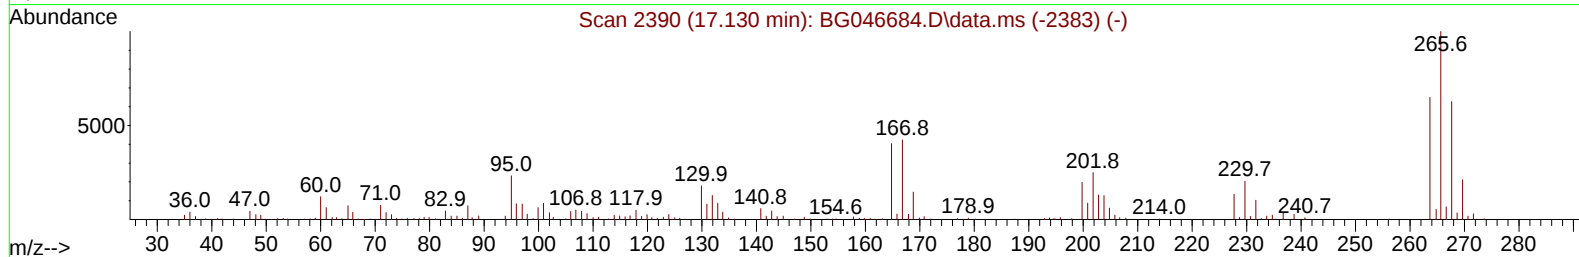
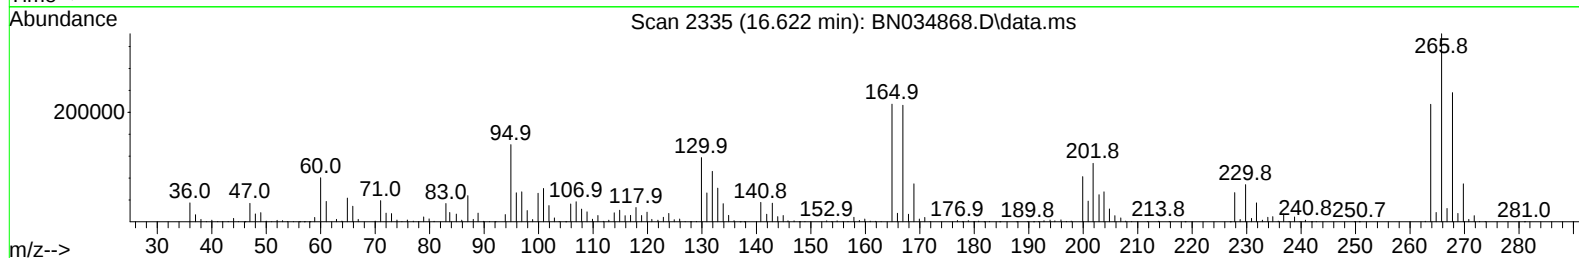


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110624\
Data File : BN034868.D
Acq On : 06 Nov 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 14:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 23:56:03 2024
Response via : Initial Calibration

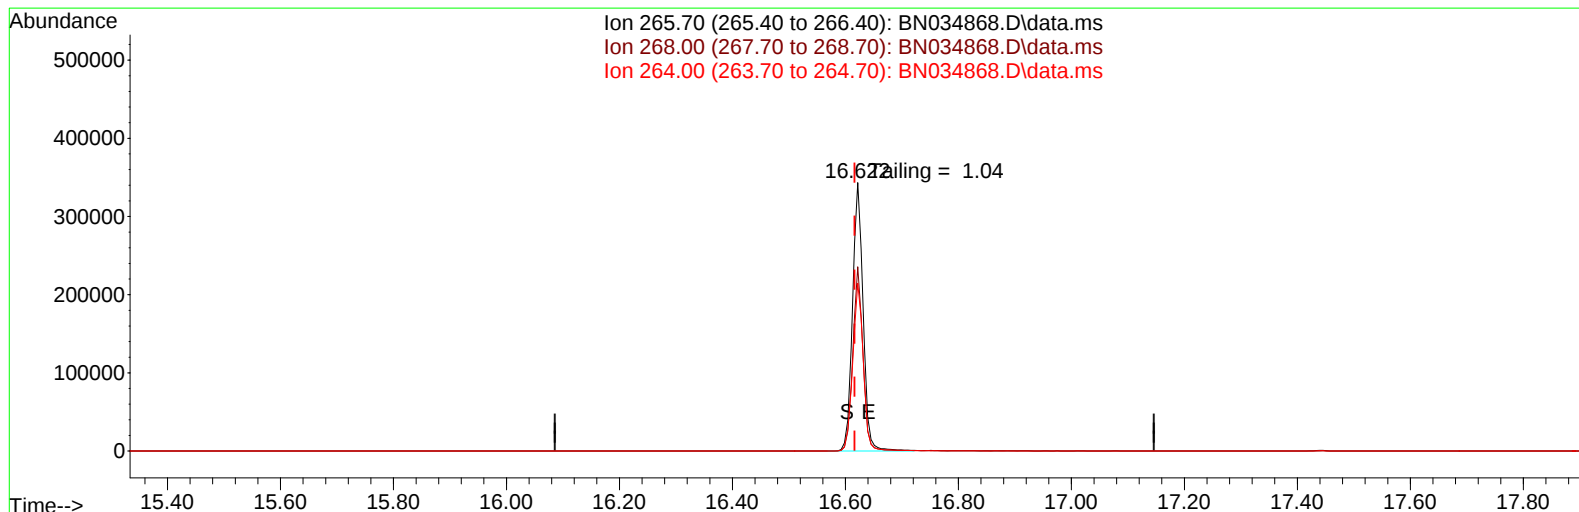

TIC: BN034868.D\data.ms

(70) Pentachlorophenol (C)




16.622min (+ 0.006) 17734.46 ng

response 450233

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.66
264.00	61.60	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110624\
Data File : BN034868.D
Acq On : 06 Nov 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 14:42:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 23:56:03 2024
Response via : Initial Calibration

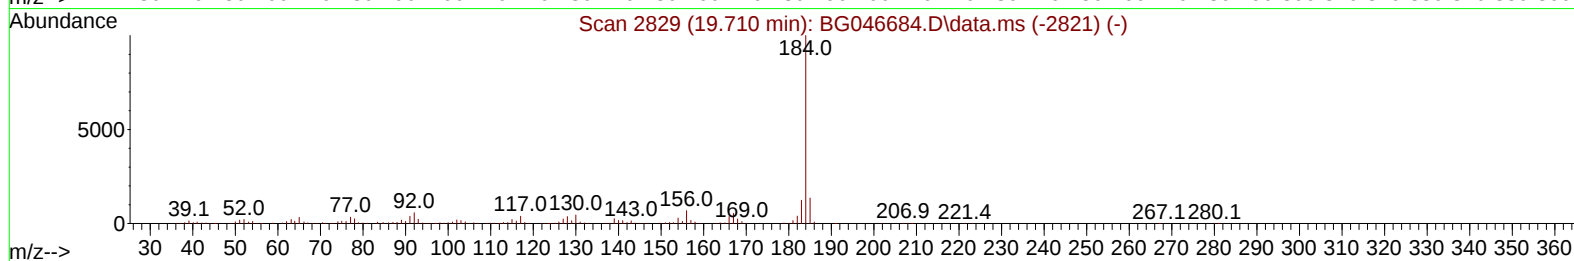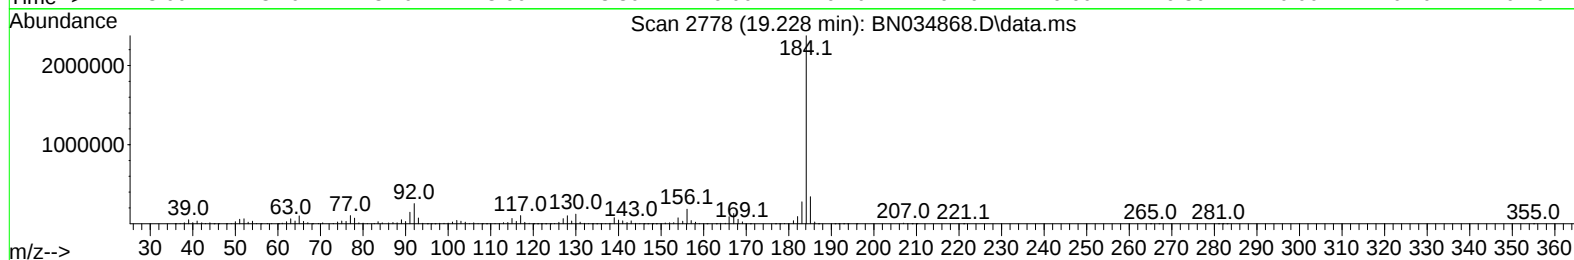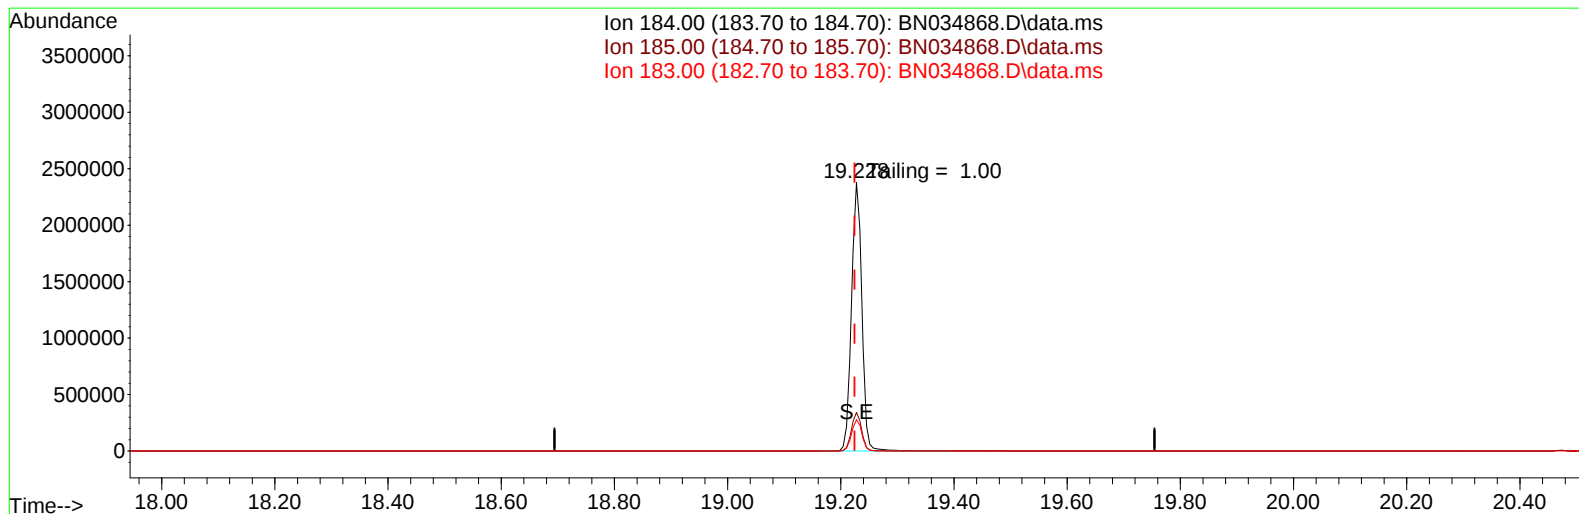

TIC: BN034868.D\data.ms

(77) Benizidine

19.228min (+ 0.004) 0.00 ng

response 3023707

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.40
183.00	13.20	11.71
0.00	0.00	0.00