


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110624\
Data File : BN034868.D
Acq On : 06 Nov 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN103024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 05 00:03:28 2024

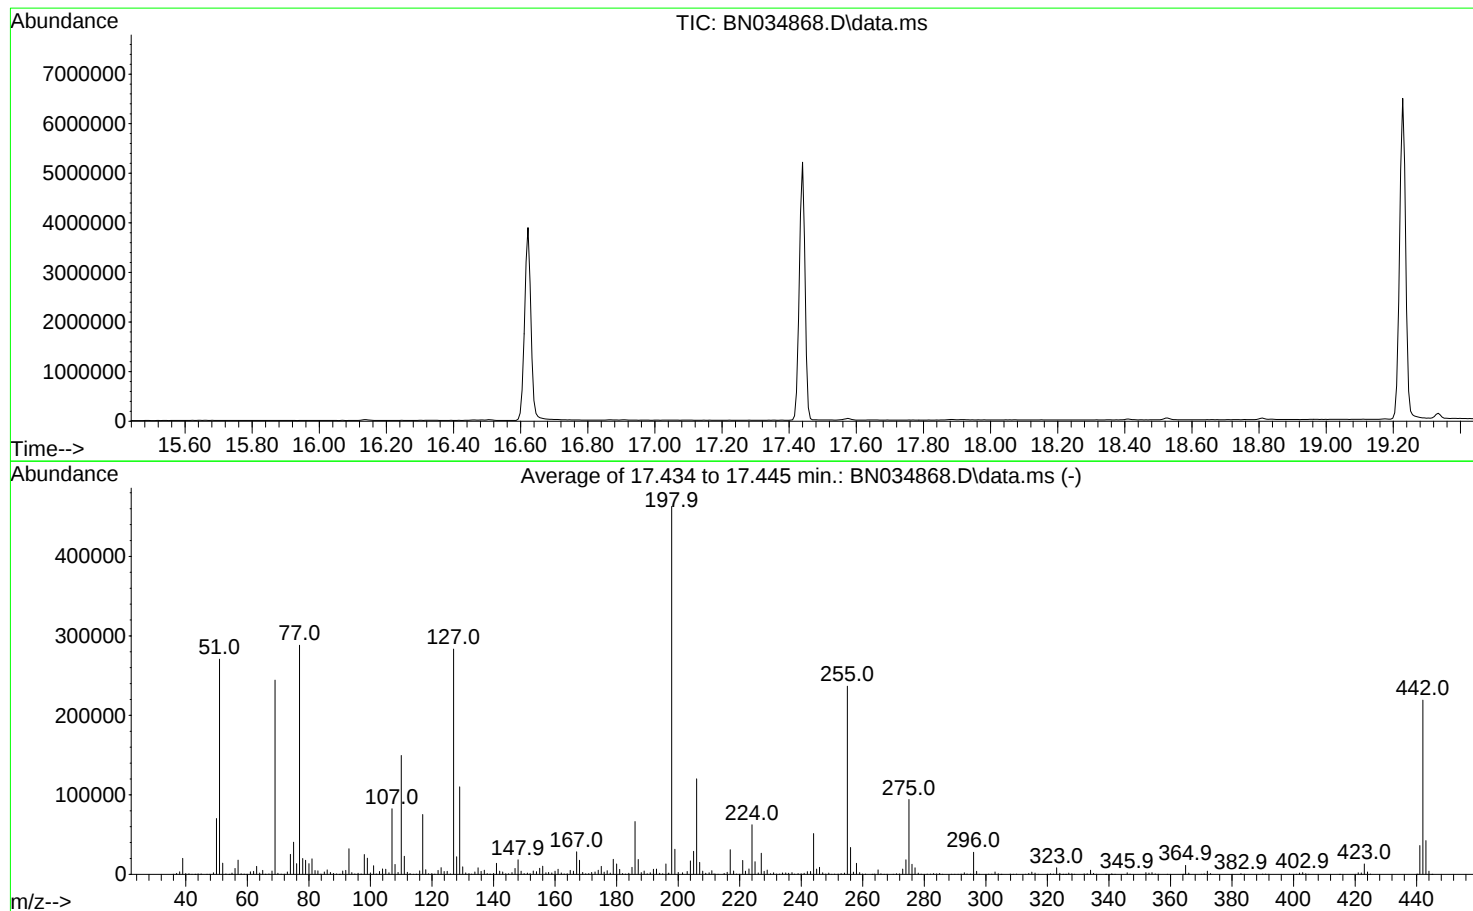




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.5	270745	PASS
68	69	0.00	2	1.7	4169	PASS
69	198	0.00	100	52.8	244288	PASS
70	69	0.00	2	0.6	1402	PASS
127	198	10	80	61.2	283349	PASS
197	198	0.00	2	0.4	1659	PASS
198	198	100	100	100.0	462784	PASS
199	198	5	9	6.8	31541	PASS
275	198	10	60	20.3	94171	PASS
365	198	1	100	2.4	11327	PASS
441	198	0.01	100	7.8	36168	PASS
442	442	50	100	100.0	219221	PASS
443	442	15	24	19.4	42464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110624\
Data File : BN034868.D
Acq On : 06 Nov 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 06 14:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 23:56:03 2024
Response via : Initial Calibration

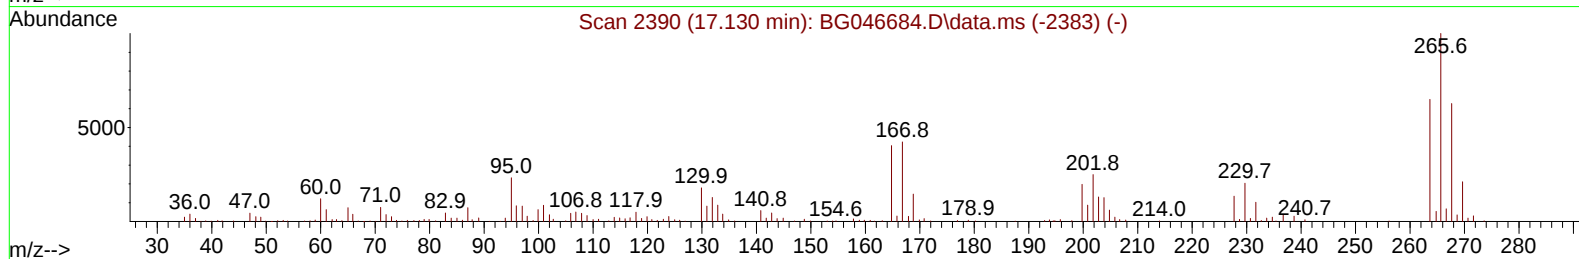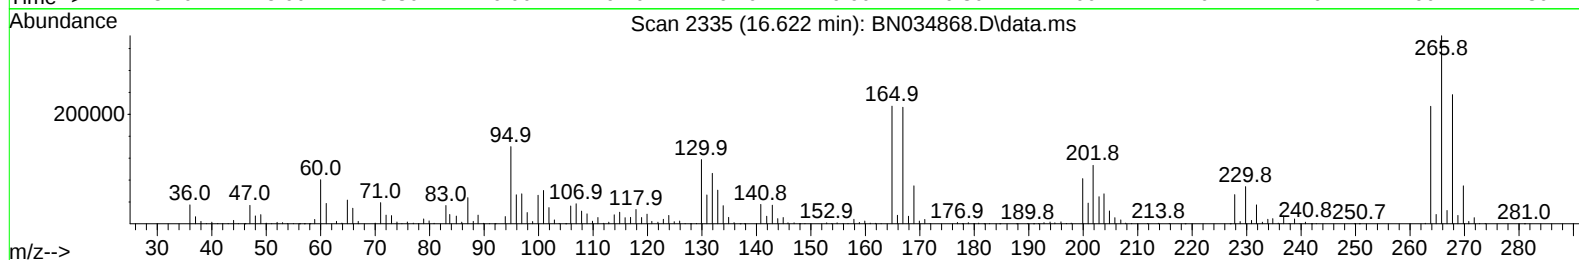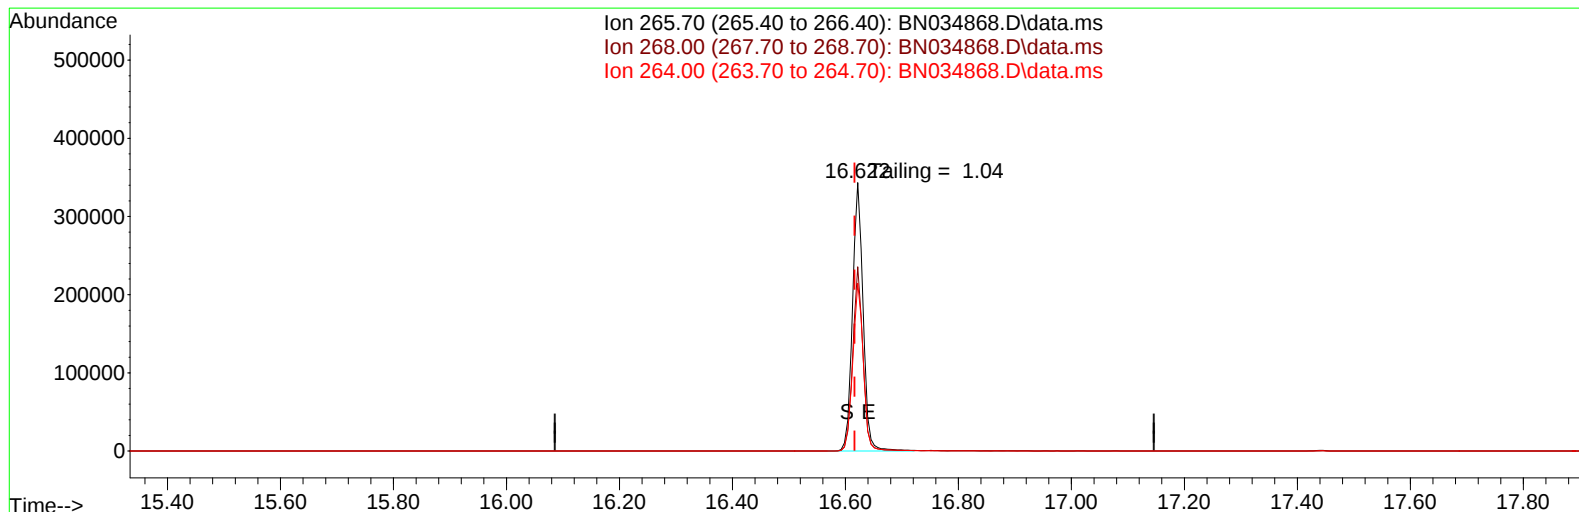

TIC: BN034868.D\data.ms

(70) Pentachlorophenol (C)

16.622min (+ 0.006) 17734.46 ng




response 450233

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.66
264.00	61.60	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110624\
Data File : BN034868.D
Acq On : 06 Nov 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 06 14:42:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 23:56:03 2024
Response via : Initial Calibration

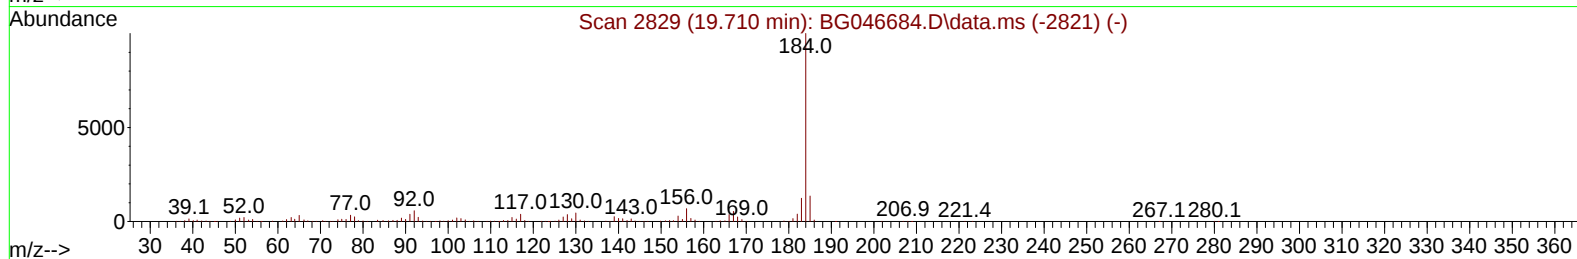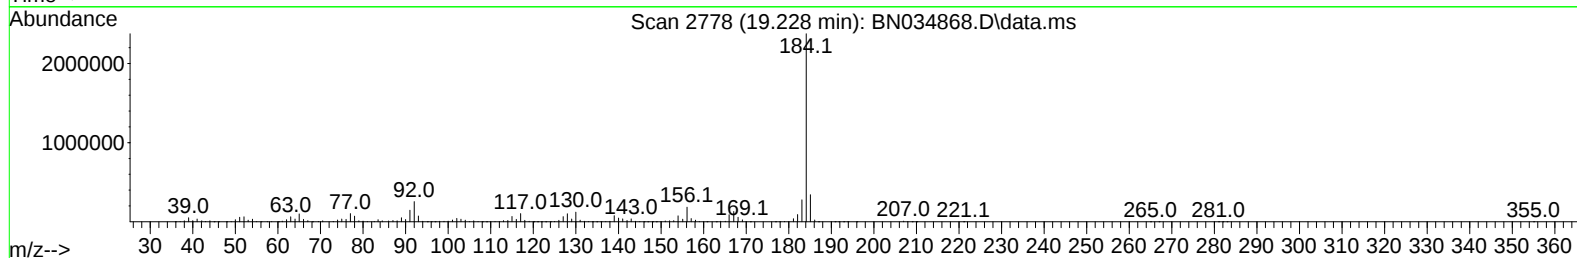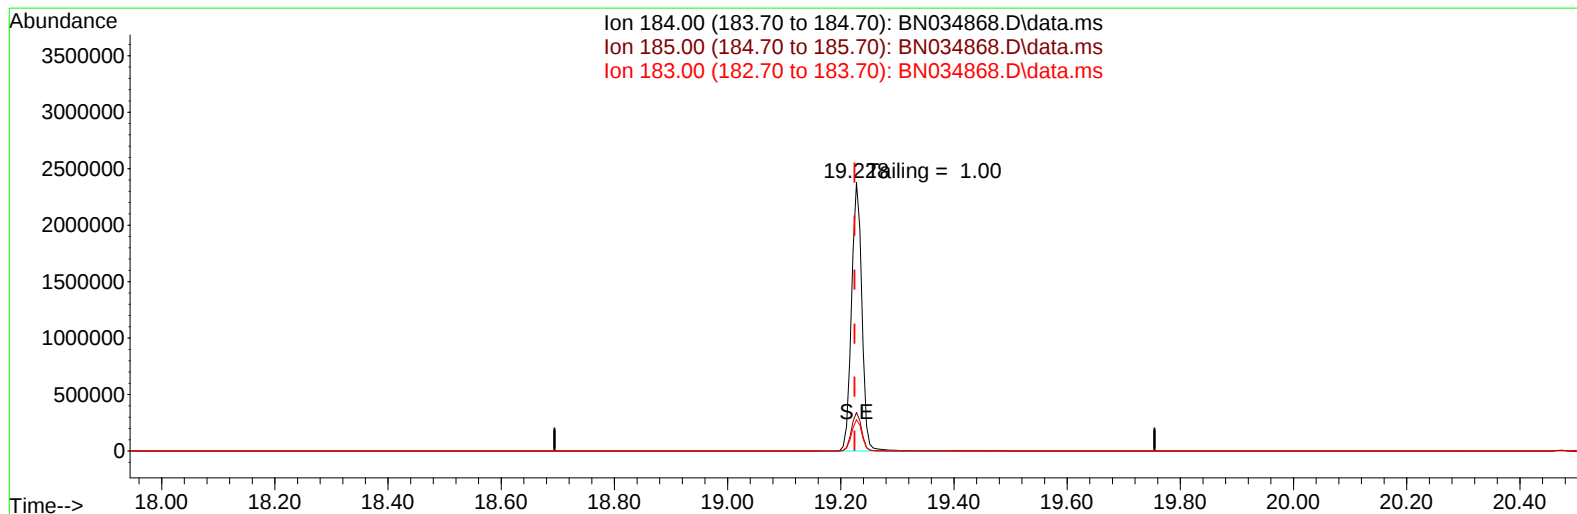

TIC: BN034868.D\data.ms

(77) Benizidine

19.228min (+ 0.004) 0.00 ng

response 3023707

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.40
183.00	13.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/6/2024	BNA_N	<u>BN034868.D</u>
Compound Name	Response	Retention Time
DDT	1490683	20.475
DDD	32606	20.033
DDE	1778	19.522
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34384	1525067	2.25

Instrument :
BNA_N
ClientSampleId :
DFTPP