

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022522.D
 Acq On : 07 Nov 2022 11:48
 Operator : CG/JU
 Sample : PB148655BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK655

Quant Time: Nov 07 23:33:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:30:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	2598	0.400	ng/ul	0.00
4) Naphthalene-d8	10.745	136	8889	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.595	164	5505	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	8445	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	10009	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264	9949	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	22880	6.776	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.345	152	4915	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	11546	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.783	128	597	0.023	ng/ul#	32
20) Pyrene	19.756	202	1527	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	3143	0.079	ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022522.D
Acq On : 07 Nov 2022 11:48
Operator : CG/JU
Sample : PB148655BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK655

Quant Time: Nov 07 23:33:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:30:37 2022
Response via : Initial Calibration




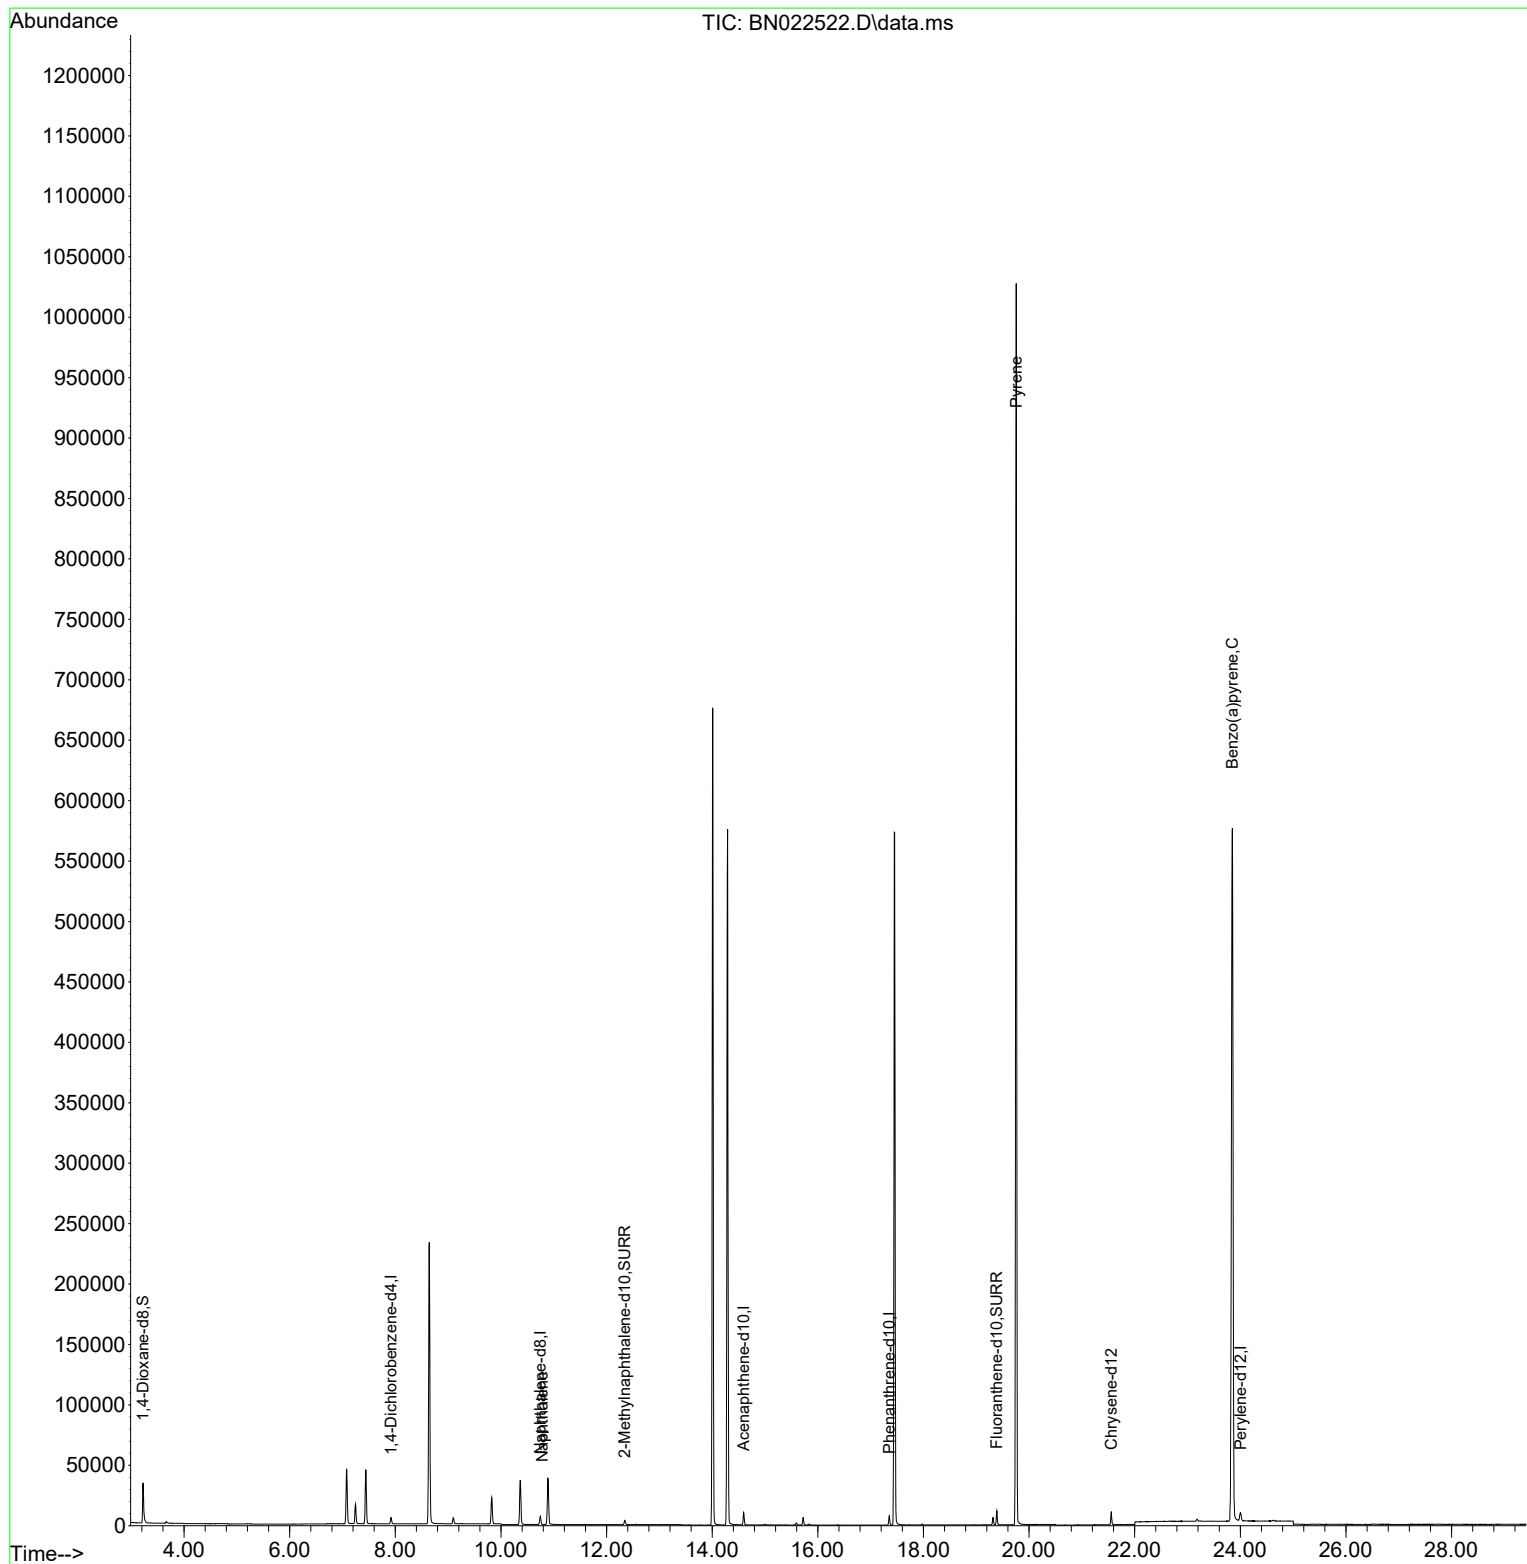


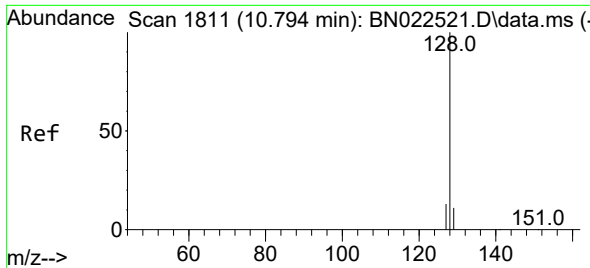

#5
Naphthalene
Concen: 0.023 ng/ul
RT: 10.783 min Scan# 1809
Delta R.T. -0.011 min
Lab File: BN022522.D
Acq: 07 Nov 2022 11:48




Instrument :
BNA_N
ClientSampleId :
SBLK655


Tgt Ion:128 Resp: 597
Ion Ratio Lower Upper
128 100
129 43.5 9.3 13.9#
127 35.2 10.7 16.1#

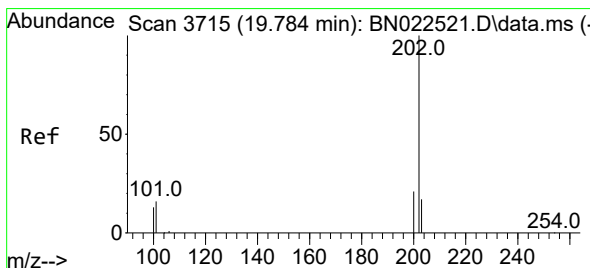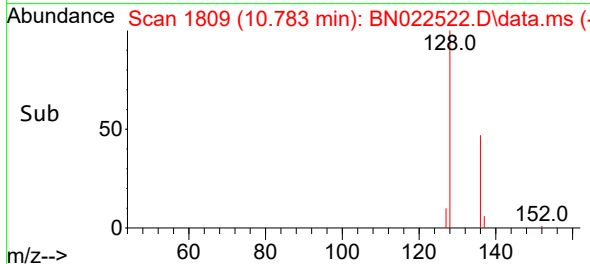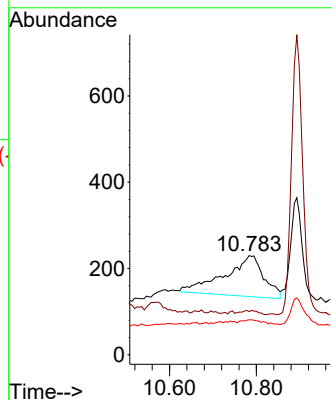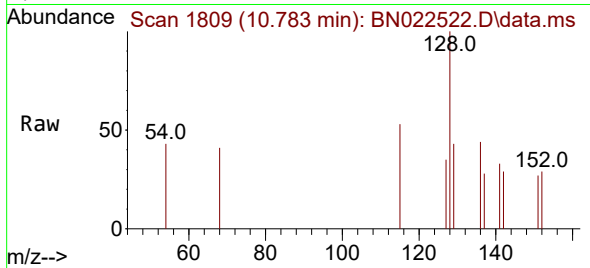

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.756 min Scan# 3709
Delta R.T. -0.028 min
Lab File: BN022522.D
Acq: 07 Nov 2022 11:48


Tgt Ion:202 Resp: 1527
Ion Ratio Lower Upper
202 100
101 177.4 13.1 19.7#
100 1286.8 10.6 16.0#

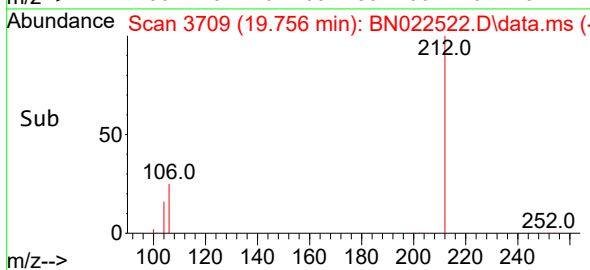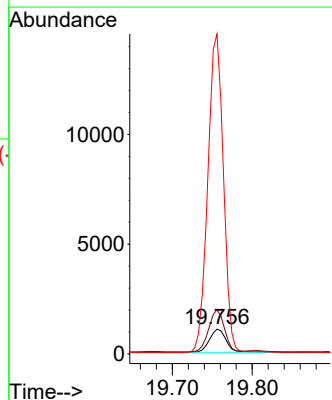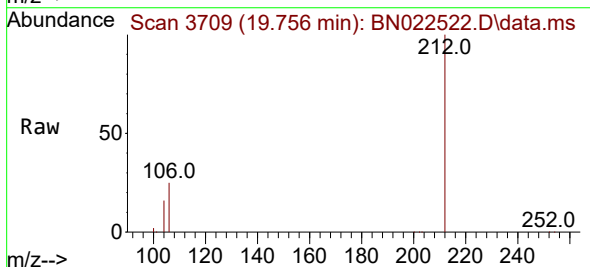

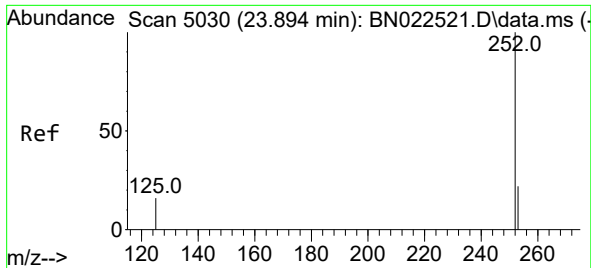

#26
 Benzo(a)pyrene
 Concen: 0.079 ng/ul
 RT: 23.847 min Scan# 5014
 Delta R.T. -0.047 min
 Lab File: BN022522.D
 Acq: 07 Nov 2022 11:48

Instrument :
 BNA_N
 ClientSampleId :
 SBLK655

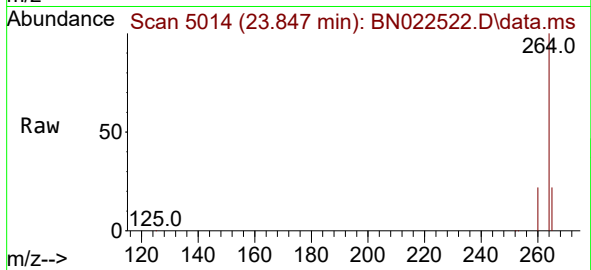

Tgt Ion:252 Resp: 3143
 Ion Ratio Lower Upper
 252 100
 253 50.6 21.0 31.6#
 125 58.1 17.9 26.9#

