

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022523.D
 Acq On : 07 Nov 2022 12:27
 Operator : CG/JU
 Sample : PB148656BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK656

Quant Time: Nov 07 23:33:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:30:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	3004	0.400	ng/ul	0.00
4) Naphthalene-d8	10.745	136	10054	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.595	164	4437	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	13566	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	11306	0.400	ng/ul	0.00
23) Perylene-d12	24.005	264	10989	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	22608	5.791	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.345	152	3477	0.229	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	11308	0.298	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.756	202	1521	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	3233	0.073	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022523.D
Acq On : 07 Nov 2022 12:27
Operator : CG/JU
Sample : PB148656BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK656

Quant Time: Nov 07 23:33:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:30:37 2022
Response via : Initial Calibration

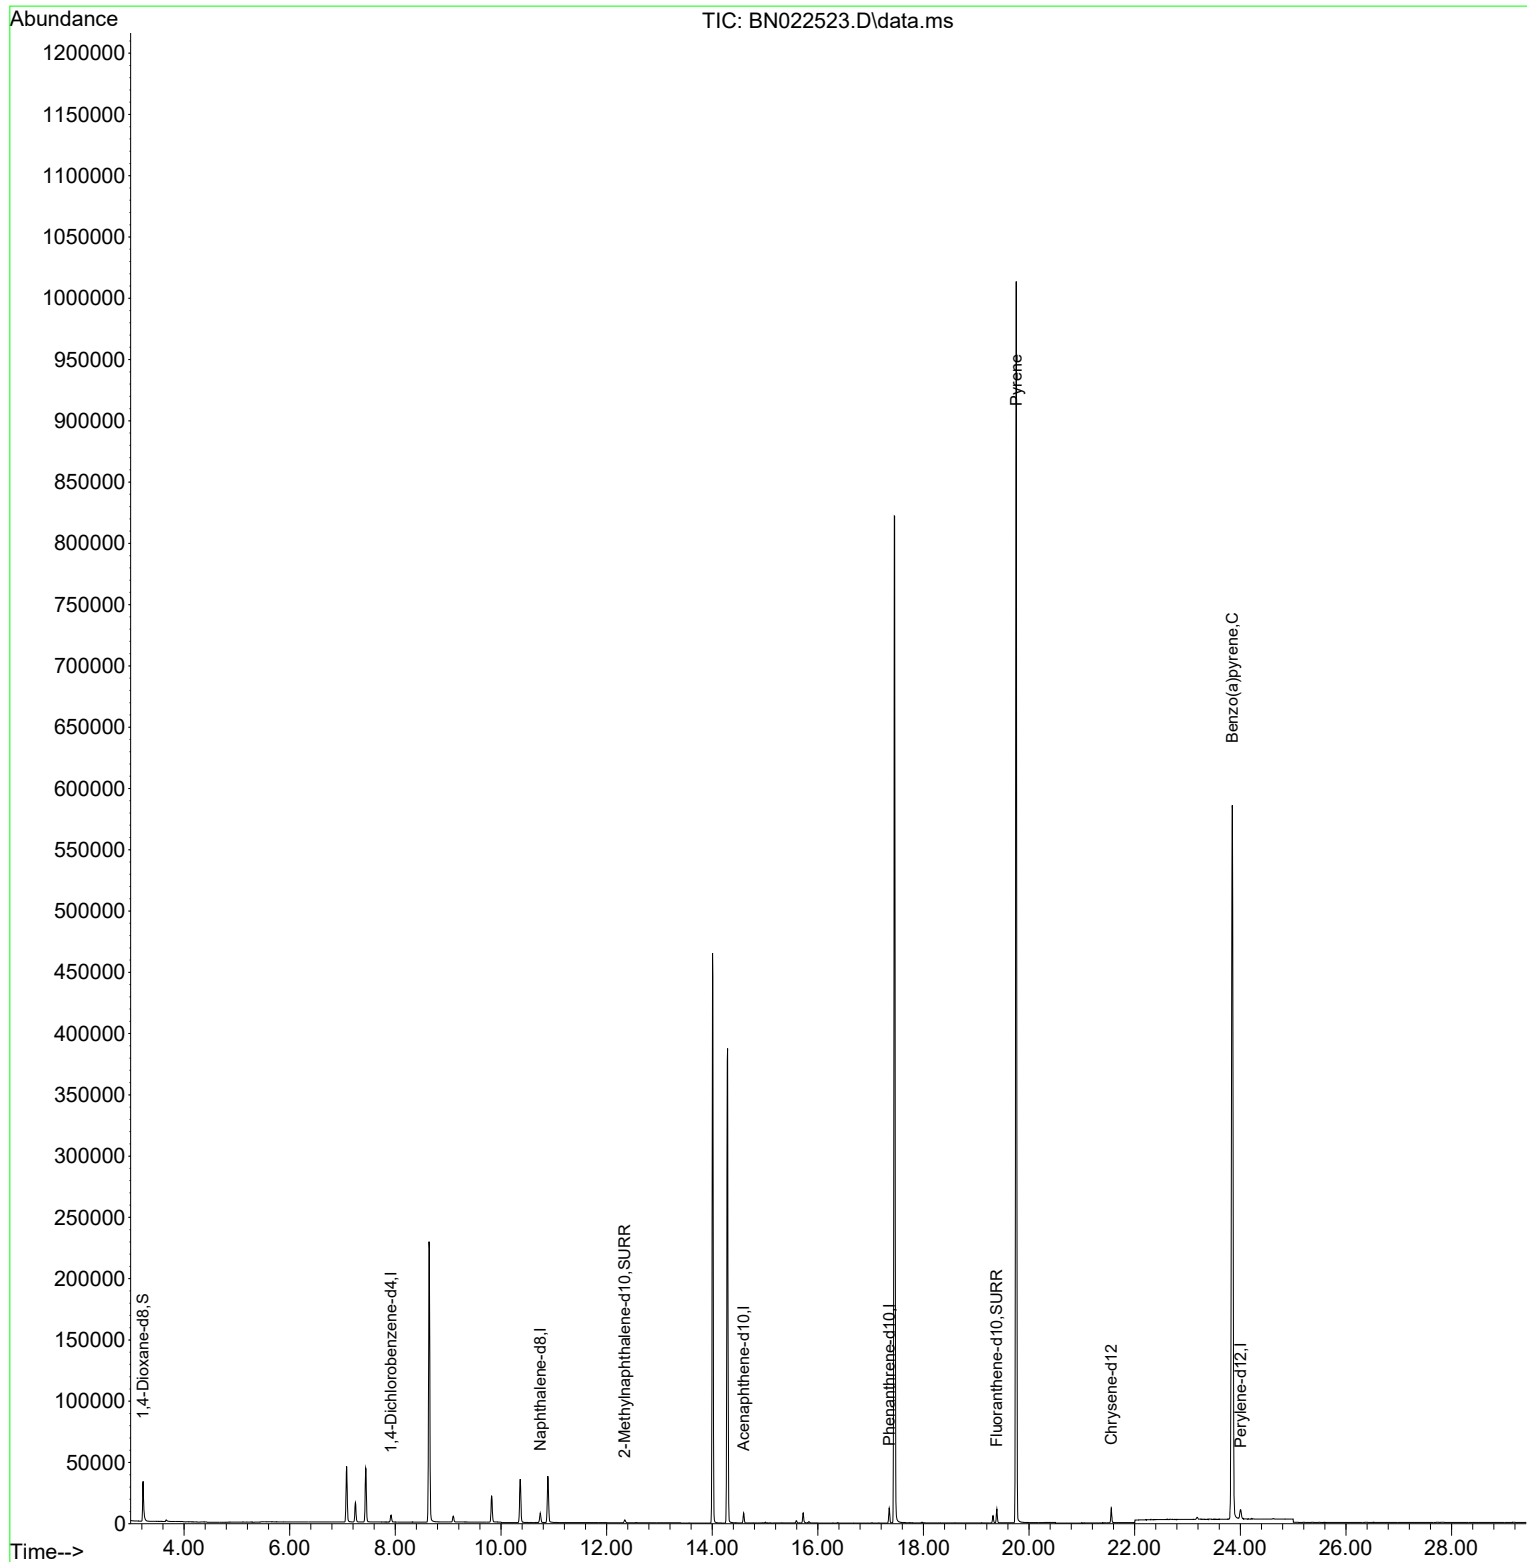

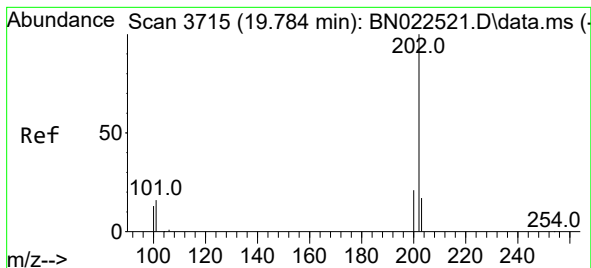

#20

Pyrene

Concen: 0.029 ng/ul

RT: 19.756 min Scan# 31

Delta R.T. -0.028 min

Lab File: BN022523.D

Acq: 07 Nov 2022 12:27

Instrument :

BNA_N

ClientSampleId :

SBLK656





Tgt Ion:202 Resp: 1521

Ion Ratio Lower Upper

202 100

101 179.2 13.1 19.7#

100 1310.4 10.6 16.0#

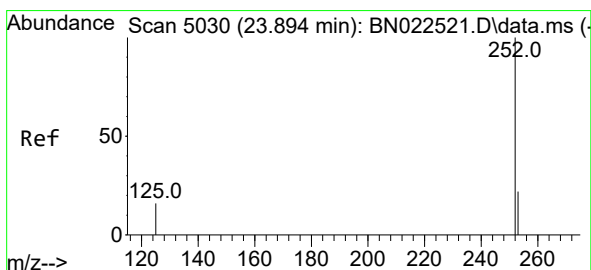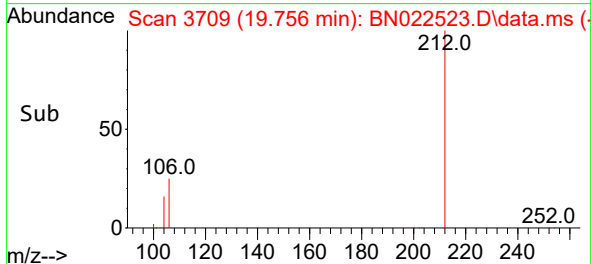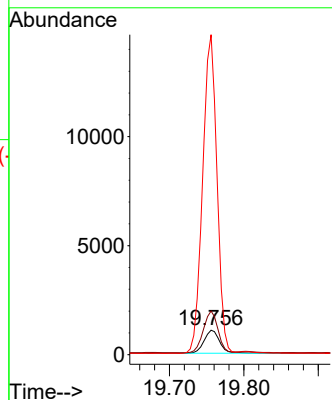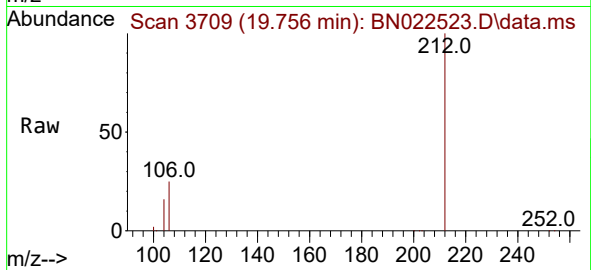

#26

Benzo(a)pyrene

Concen: 0.073 ng/ul

RT: 23.847 min Scan# 5014

Delta R.T. -0.047 min

Lab File: BN022523.D

Acq: 07 Nov 2022 12:27

Tgt Ion:252 Resp: 3233

Ion Ratio Lower Upper

252 100

253 49.3 21.0 31.6#

125 56.2 17.9 26.9#

