

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022528.D
 Acq On : 07 Nov 2022 15:43
 Operator : CG/JU
 Sample : PB148825BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK825

Quant Time: Nov 07 23:34:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:30:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	2265	0.400	ng/ul	0.00
4) Naphthalene-d8	10.745	136	7783	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.596	164	4723	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	9434	0.400	ng/ul	0.00
17) Chrysene-d12	21.559	240	8227	0.400	ng/ul	0.00
23) Perylene-d12	24.005	264	7846	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.224	96	20290	6.893	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.345	152	4414	0.375	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	8258	0.299	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.595	166	1577	0.076	ng/ul#	15
20) Pyrene	19.761	202	1612	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	2922	0.093	ng/ul#	20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022528.D
Acq On : 07 Nov 2022 15:43
Operator : CG/JU
Sample : PB148825BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK825

Quant Time: Nov 07 23:34:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:30:37 2022
Response via : Initial Calibration




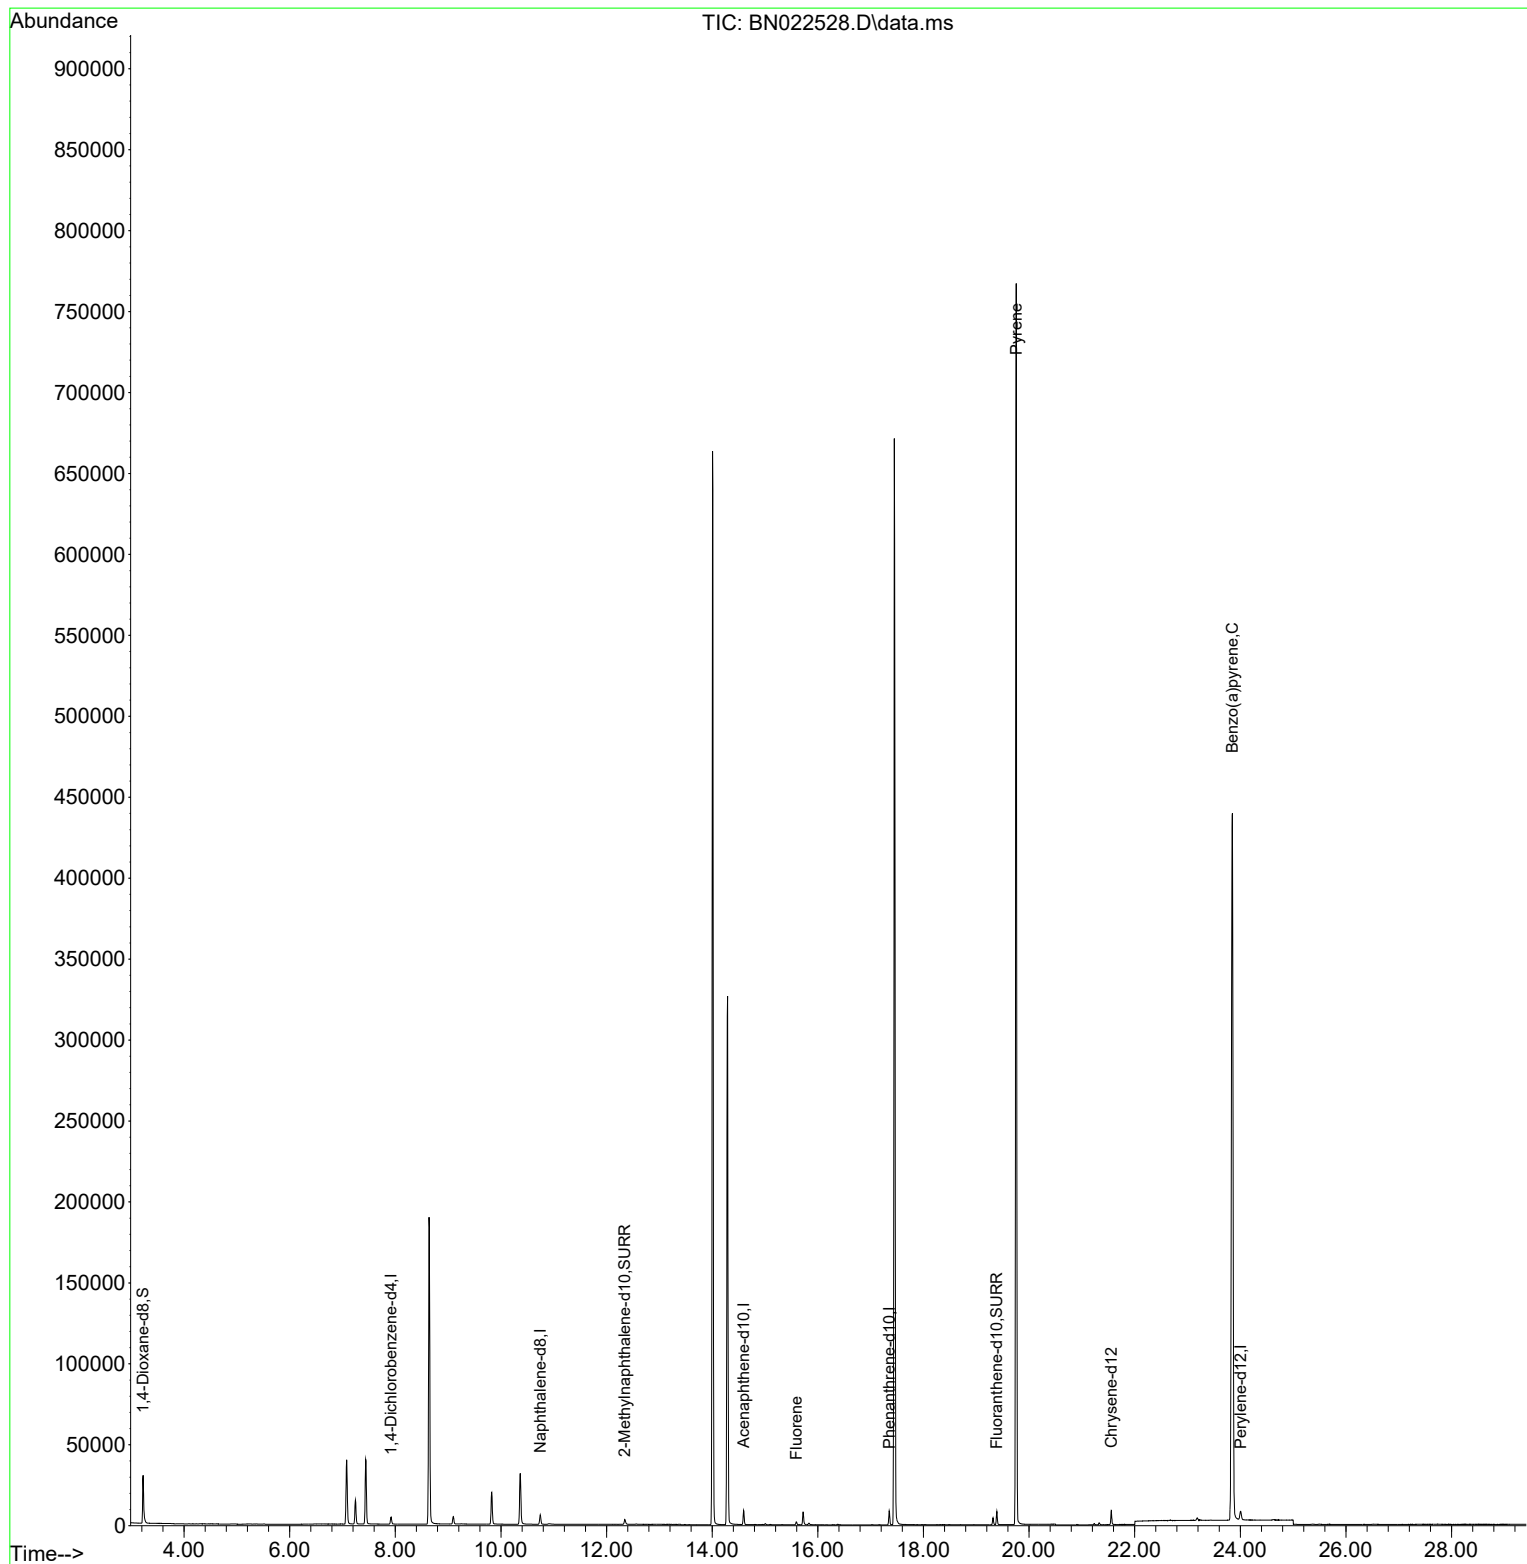


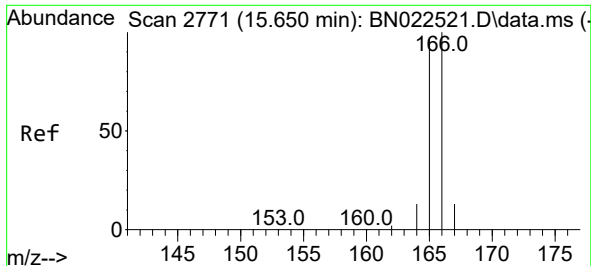

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.595 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN022528.D
Acq: 07 Nov 2022 15:43




Instrument :
BNA_N
ClientSampleId :
SBLK825


Tgt Ion:166 Resp: 1577
Ion Ratio Lower Upper
166 100
165 10.1 78.2 117.2#
167 37.8 11.0 16.4#

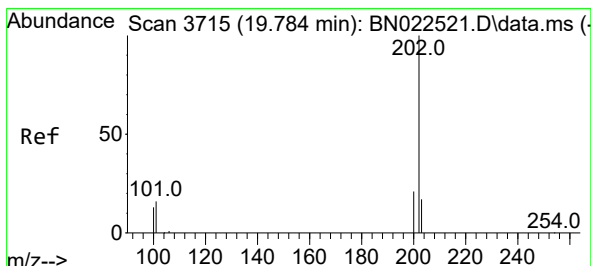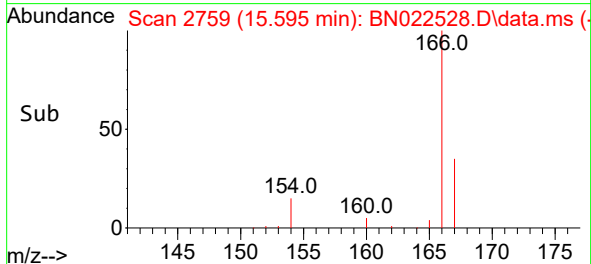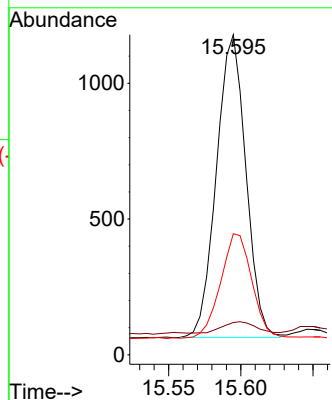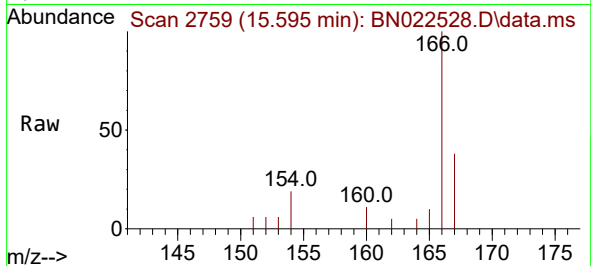

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.761 min Scan# 3710
Delta R.T. -0.023 min
Lab File: BN022528.D
Acq: 07 Nov 2022 15:43

Tgt Ion:202 Resp: 1612
Ion Ratio Lower Upper
202 100
101 164.6 13.1 19.7#
100 822.0 10.6 16.0#

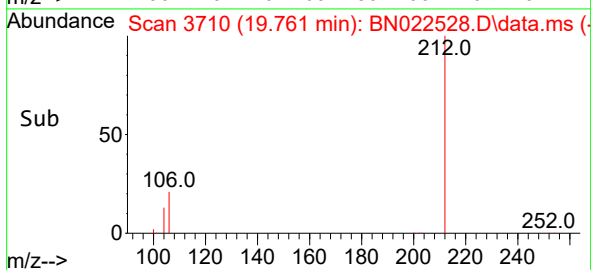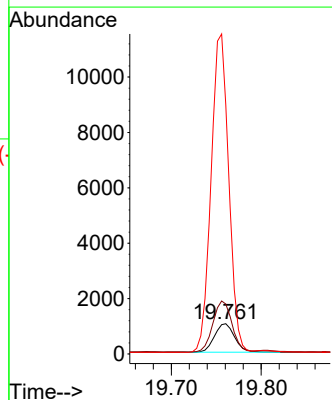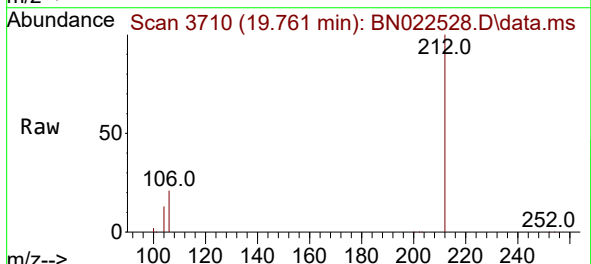

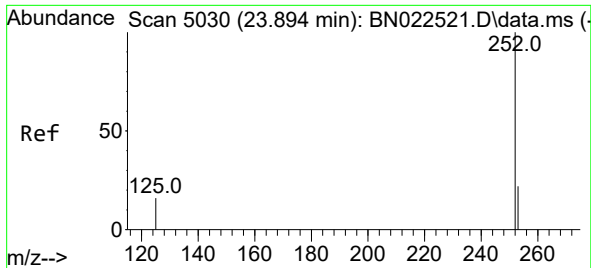

#26

Benzo(a)pyrene

Concen: 0.093 ng/ul

RT: 23.847 min Scan# 50

Delta R.T. -0.047 min

Lab File: BN022528.D


Acq: 07 Nov 2022 15:43

Instrument :

BNA_N

ClientSampleId :

SBLK825

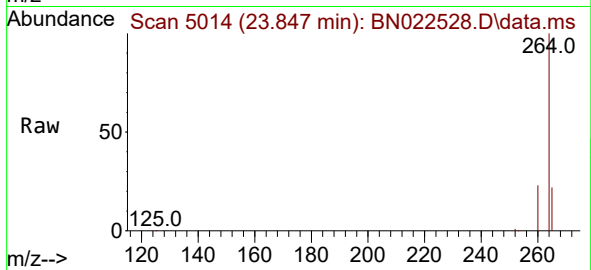

Tgt Ion:252 Resp: 2922

Ion Ratio Lower Upper

252 100

253 64.5 21.0 31.6#

125 64.2 17.9 26.9#

