

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022536.D
 Acq On : 07 Nov 2022 20:59
 Operator : CG/JU
 Sample : N5407-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y4

Quant Time: Nov 07 23:35:19 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:30:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.915	152	2167	0.400	ng/ul	0.00
4) Naphthalene-d8	10.745	136	10339	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.595	164	6542	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	15188	0.400	ng/ul	0.00
17) Chrysene-d12	21.558	240	11922	0.400	ng/ul	0.00
23) Perylene-d12	24.008	264	8710	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	15763	5.597	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.345	152	5270	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.393	212	16108	0.402	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.261	88	805	0.278	ng/ul#	67
20) Pyrene	19.760	202	2028	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.853	252	3021	0.087	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022536.D
Acq On : 07 Nov 2022 20:59
Operator : CG/JU
Sample : N5407-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Y4

Quant Time: Nov 07 23:35:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:30:37 2022
Response via : Initial Calibration




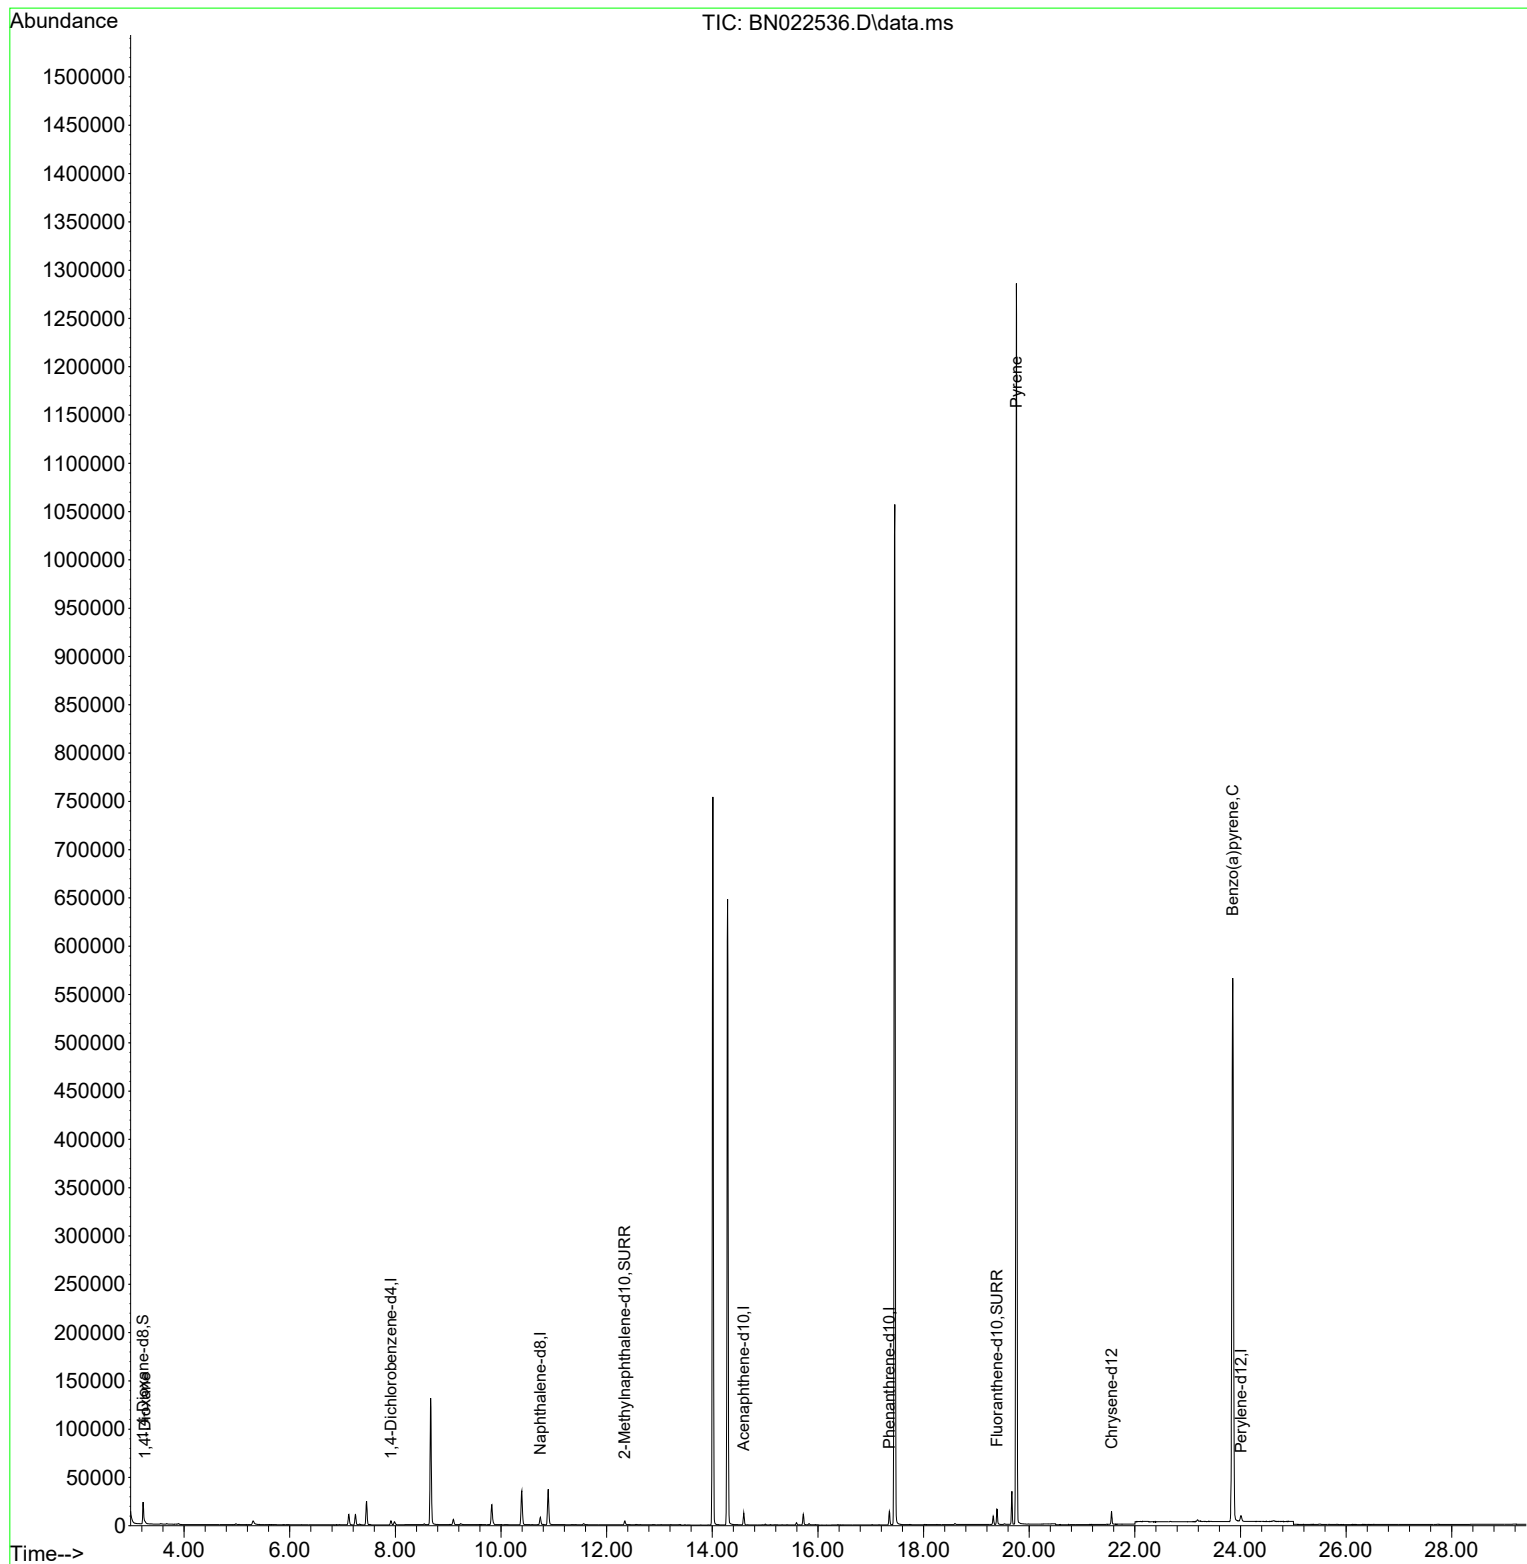


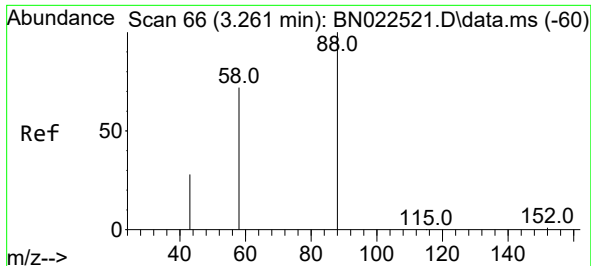

#2
 1,4-Dioxane
 Concen: 0.278 ng/ul
 RT: 3.261 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BN022536.D
 Acq: 07 Nov 2022 20:59




Instrument :
 BNA_N
 ClientSampleId :
 EW4Y4


Tgt Ion: 88 Resp: 805
 Ion Ratio Lower Upper
 88 100
 43 81.2 27.4 41.2#
 58 56.1 48.2 72.2

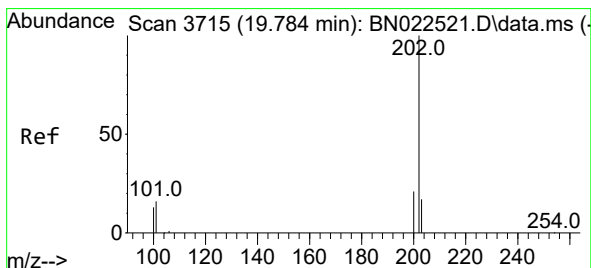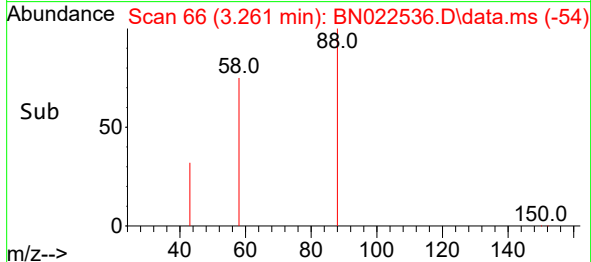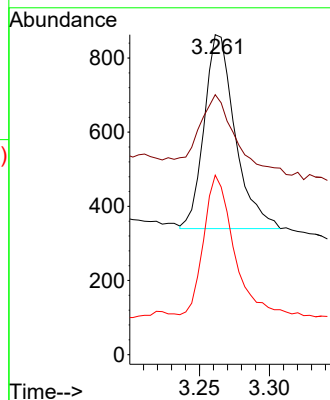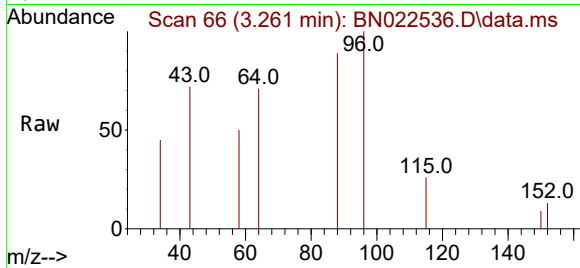

#20
 Pyrene
 Concen: 0.037 ng/ul
 RT: 19.760 min Scan# 3710
 Delta R.T. -0.023 min
 Lab File: BN022536.D
 Acq: 07 Nov 2022 20:59


Tgt Ion: 202 Resp: 2028
 Ion Ratio Lower Upper
 202 100
 101 164.7 13.1 19.7#
 100 1114.5 10.6 16.0#

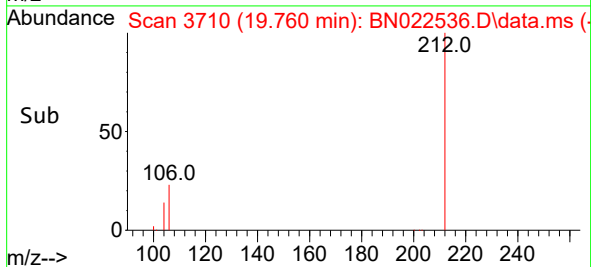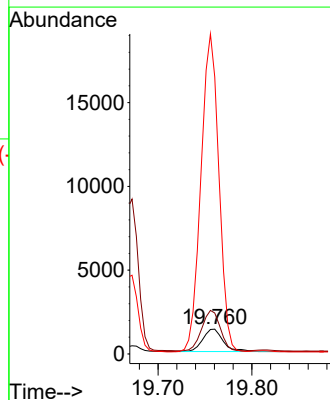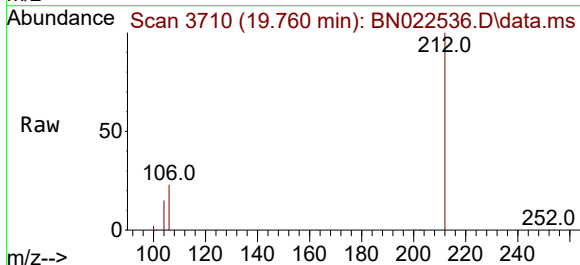

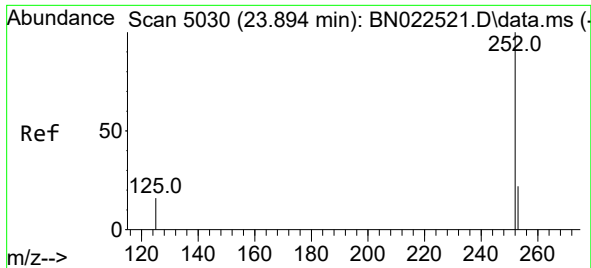

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.853 min Scan# 50
Delta R.T. -0.041 min
Lab File: BN022536.D
Acq: 07 Nov 2022 20:59

Instrument :
BNA_N
ClientSampleId :
EW4Y4

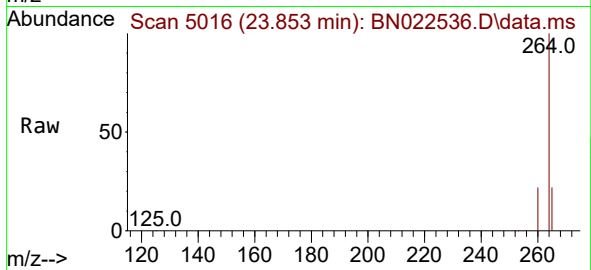

Tgt Ion:252 Resp: 3021
Ion Ratio Lower Upper
252 100
253 56.4 21.0 31.6#
125 56.9 17.9 26.9#

