

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022538.D
 Acq On : 07 Nov 2022 22:53
 Operator : CG/JU
 Sample : PB148827BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK827

Quant Time: Nov 07 23:35:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:30:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.915	152	2078	0.400	ng/ul	0.00
4) Naphthalene-d8	10.745	136	7210	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.595	164	4764	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.349	188	10909	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	8926	0.400	ng/ul	0.00
23) Perylene-d12	24.005	264	7355	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	14292	5.292	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.345	152	3412	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	8619	0.288	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.590	166	1225	0.058	ng/ul#	17
20) Pyrene	19.756	202	1118	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	1998	0.068	ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022538.D
Acq On : 07 Nov 2022 22:53
Operator : CG/JU
Sample : PB148827BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK827

Quant Time: Nov 07 23:35:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:30:37 2022
Response via : Initial Calibration




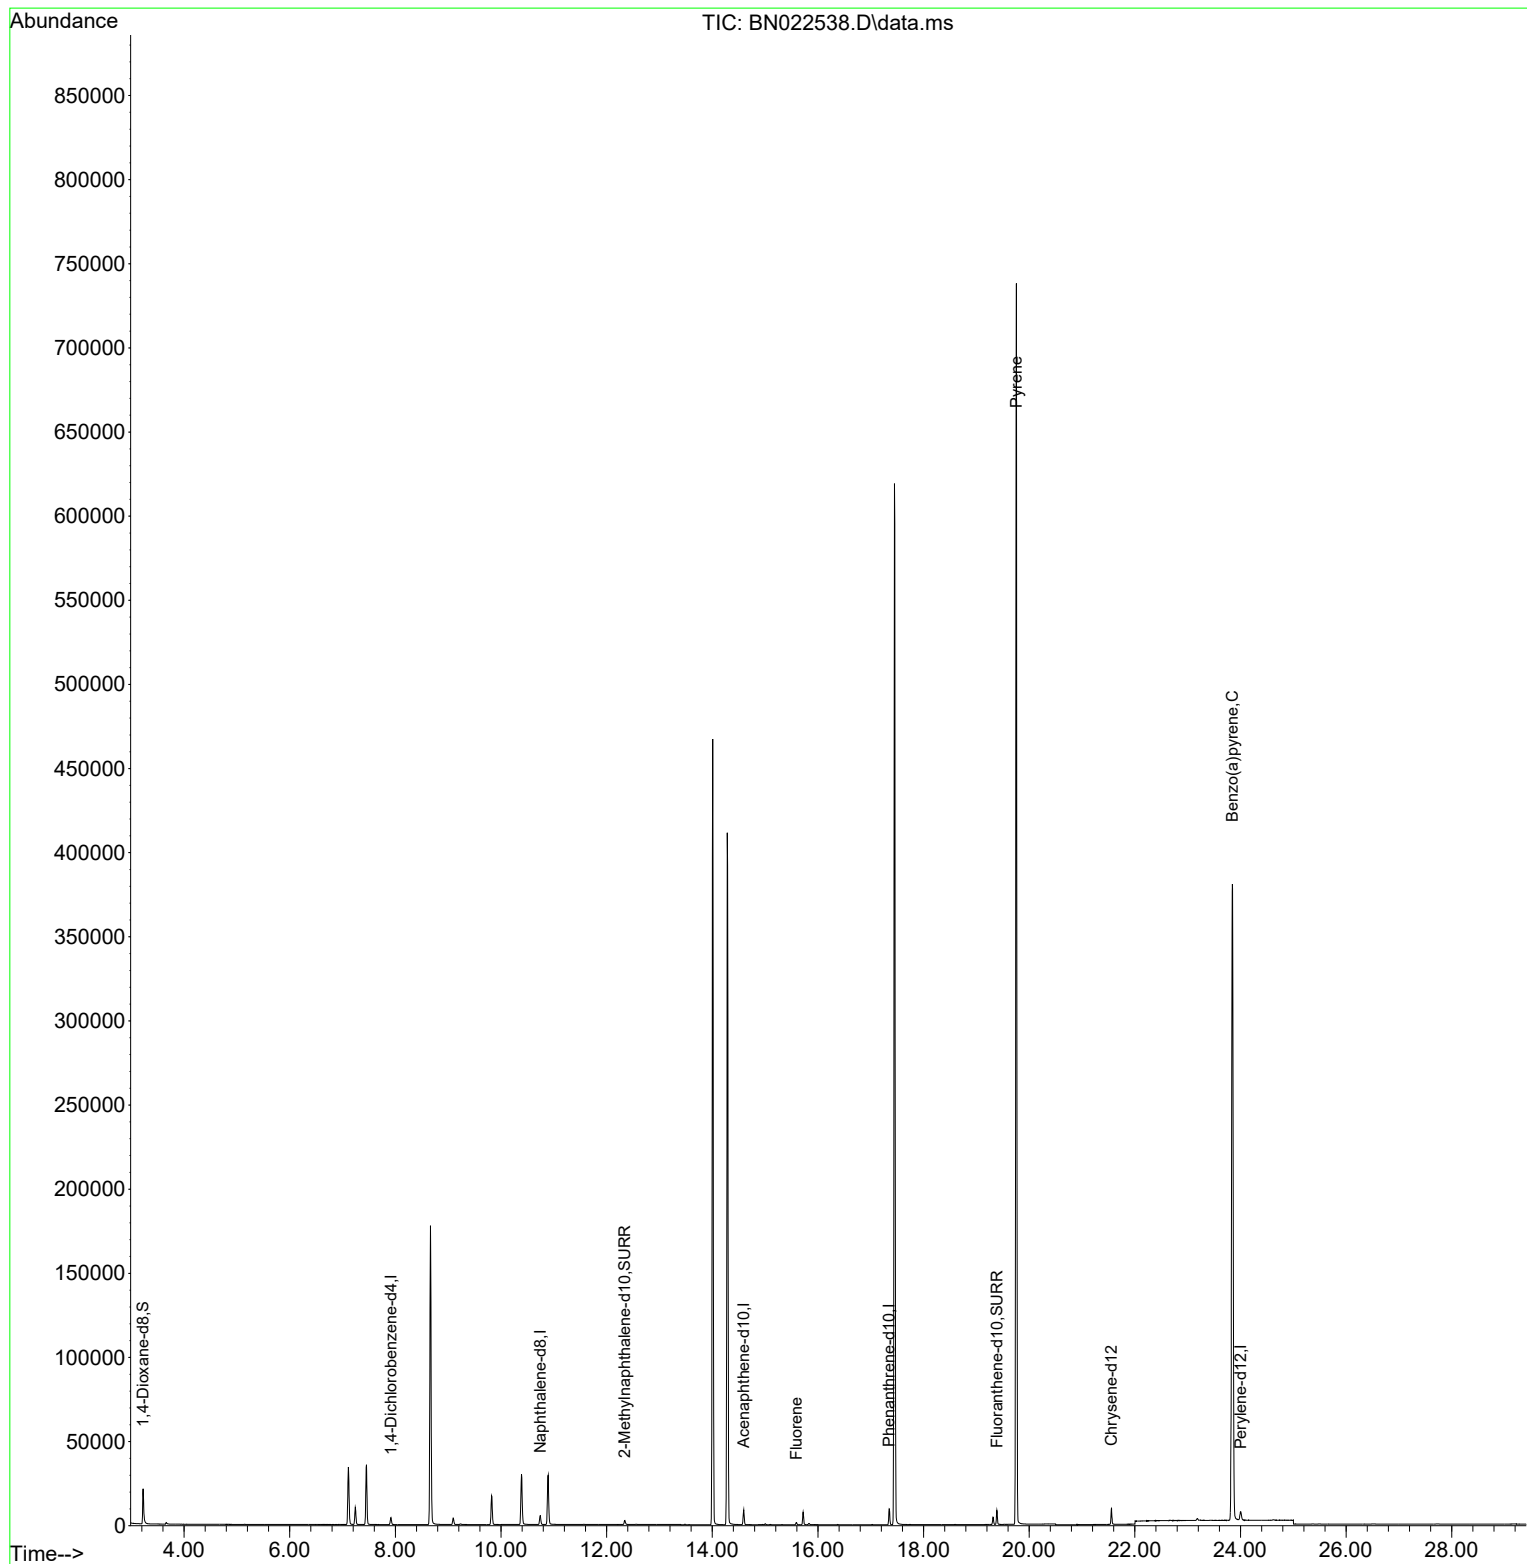


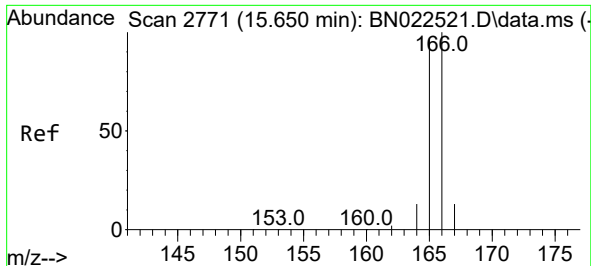

#12
Fluorene
Concen: 0.058 ng/ul
RT: 15.590 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN022538.D
Acq: 07 Nov 2022 22:53




Instrument :
BNA_N
ClientSampleId :
SBLK827


Tgt Ion:166 Resp: 1225
Ion Ratio Lower Upper
166 100
165 11.3 78.2 117.2#
167 34.2 11.0 16.4#

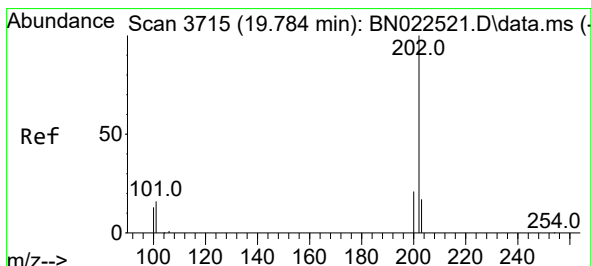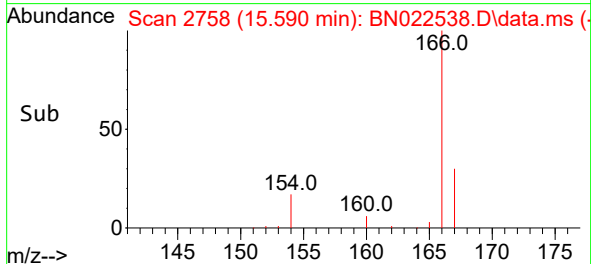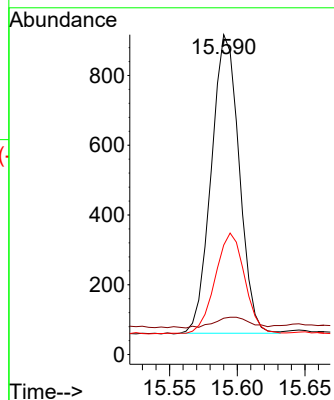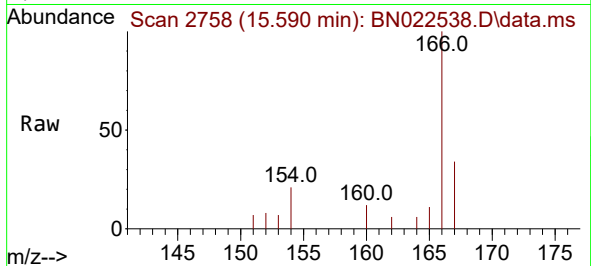

#20
Pyrene
Concen: 0.027 ng/ul
RT: 19.756 min Scan# 3709
Delta R.T. -0.028 min
Lab File: BN022538.D
Acq: 07 Nov 2022 22:53


Tgt Ion:202 Resp: 1118
Ion Ratio Lower Upper
202 100
101 182.4 13.1 19.7#
100 1315.8 10.6 16.0#

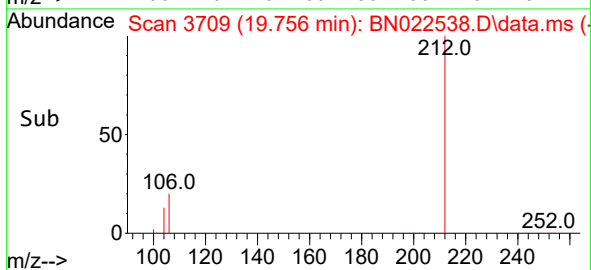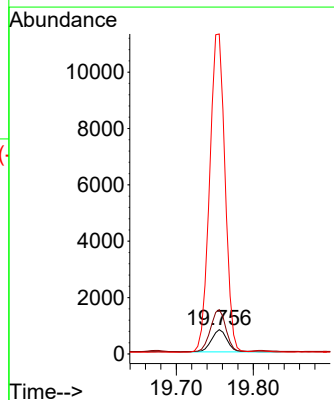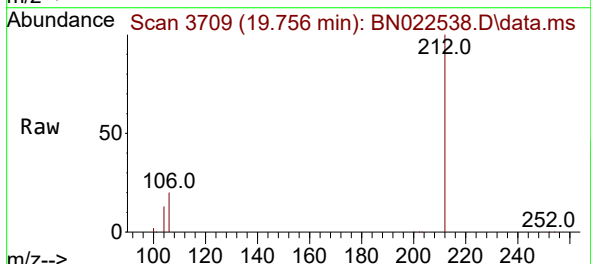

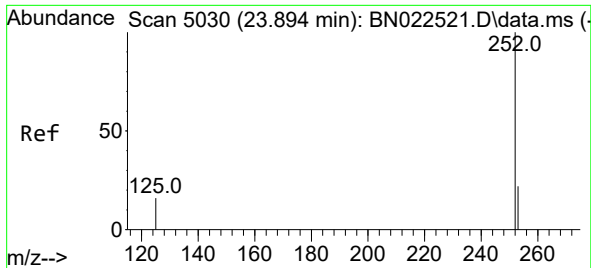

#26
Benzo(a)pyrene
Concen: 0.068 ng/ul
RT: 23.847 min Scan# 5014
Delta R.T. -0.047 min
Lab File: BN022538.D
Acq: 07 Nov 2022 22:53

Instrument :
BNA_N
ClientSampleId :
SBLK827

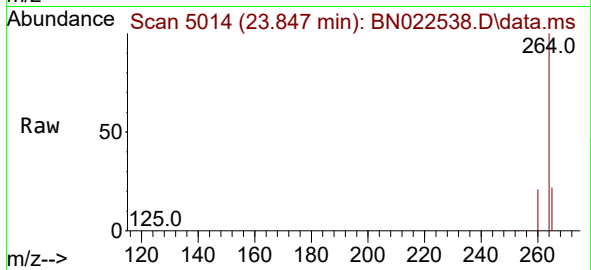

Tgt Ion:252 Resp: 1998
Ion Ratio Lower Upper
252 100
253 59.7 21.0 31.6#
125 57.7 17.9 26.9#

