

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022556.D
 Acq On : 08 Nov 2022 11:35
 Operator : CG/JU
 Sample : PB148836BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 09 01:21:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	1721	0.400	ng/ul	0.00
4) Naphthalene-d8	10.739	136	5876	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.591	164	3688	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.349	188	8149	0.400	ng/ul	0.00
17) Chrysene-d12	21.559	240	6442	0.400	ng/ul	0.00
23) Perylene-d12	24.008	264	5409	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.219	96	13749	6.147	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.340	152	3084	0.347	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	7352	0.340	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.590	166	1107	0.068	ng/ul#	16
20) Pyrene	19.756	202	1023	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	1838	0.085	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022556.D
Acq On : 08 Nov 2022 11:35
Operator : CG/JU
Sample : PB148836BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Nov 09 01:21:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

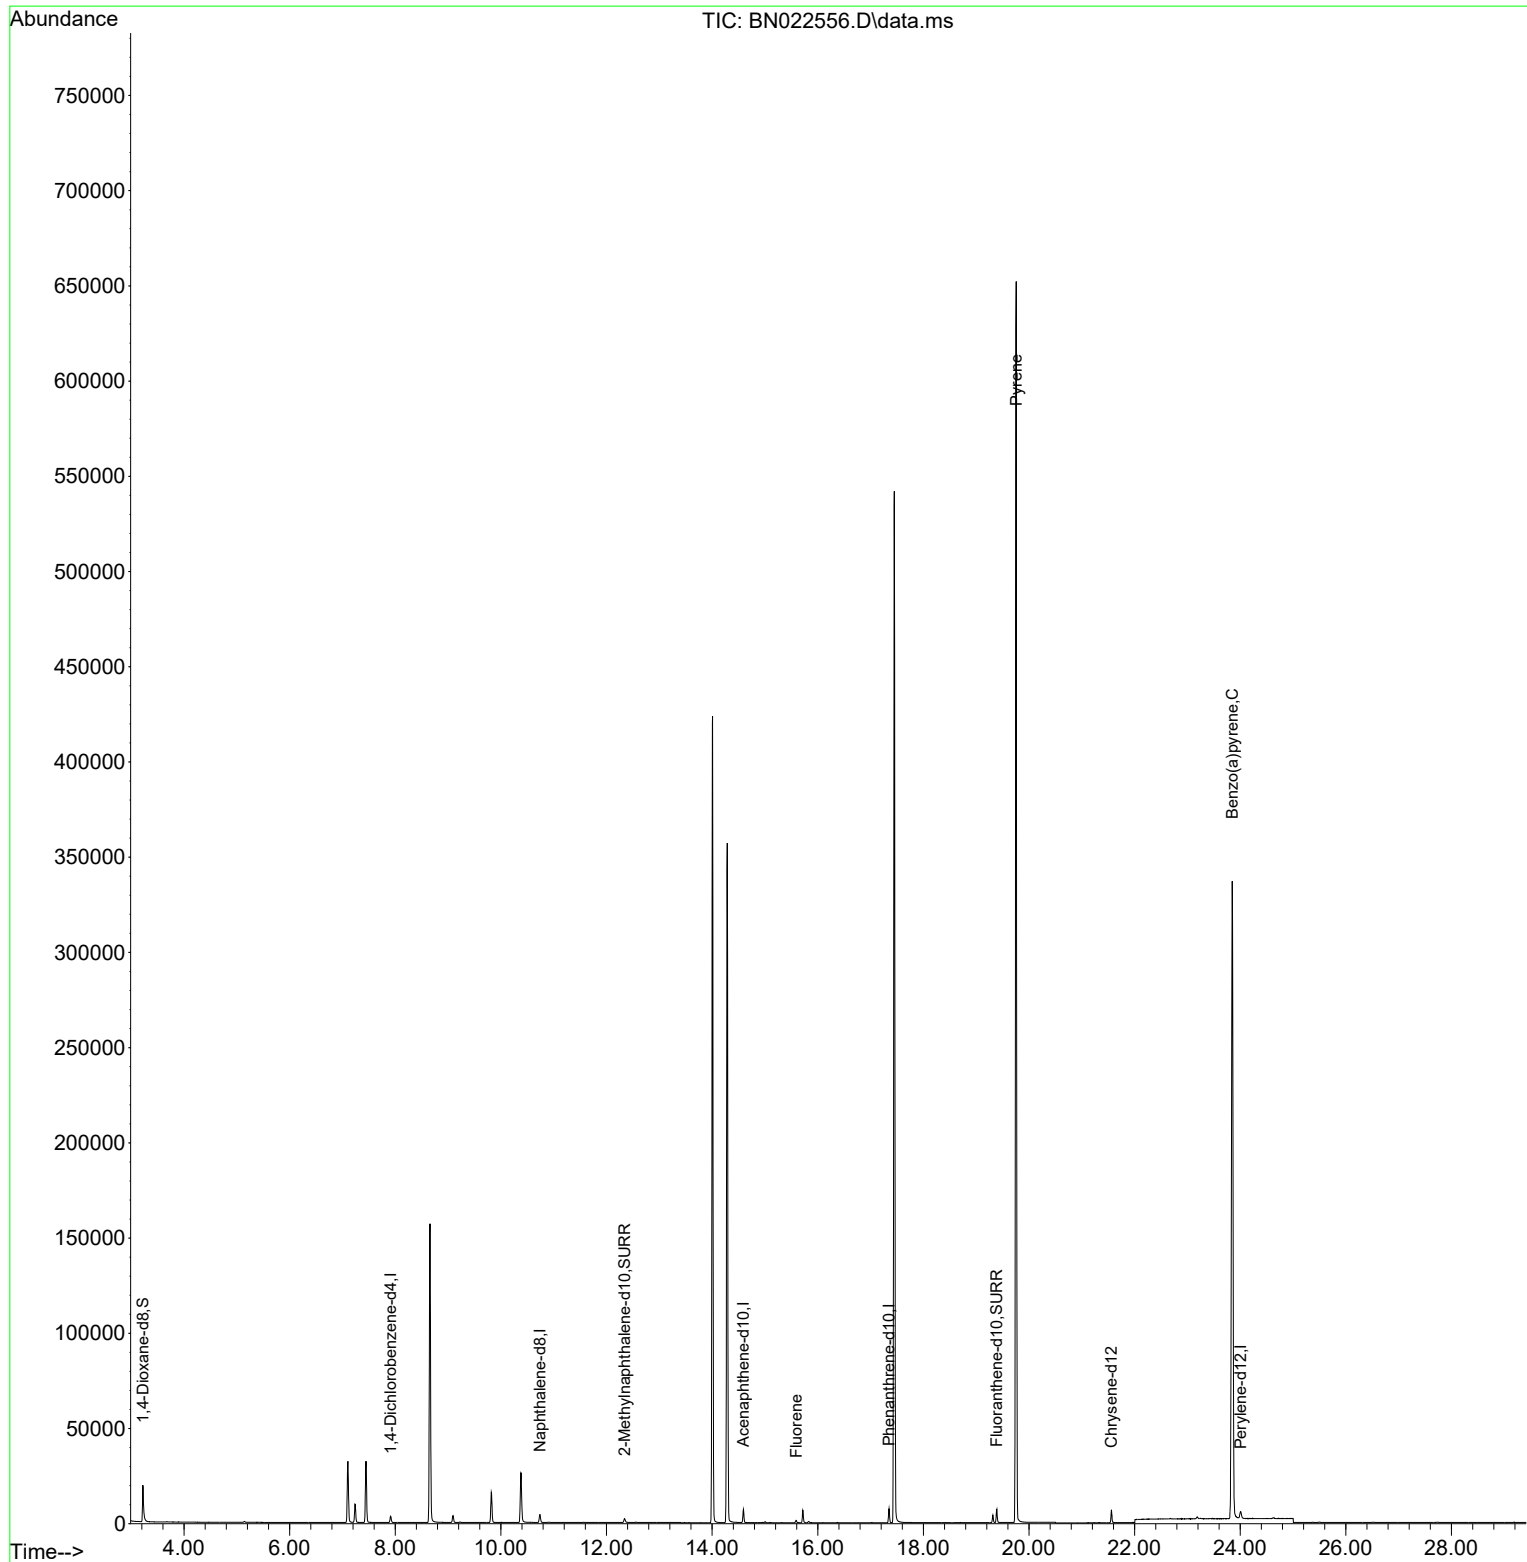



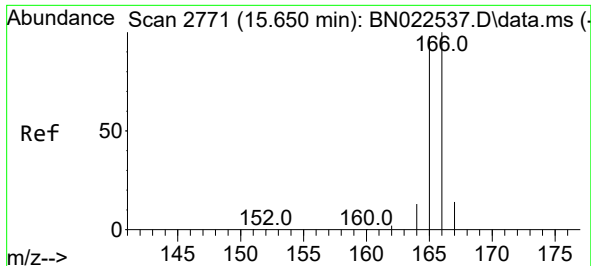


#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.590 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN022556.D
Acq: 08 Nov 2022 11:35

Instrument :
BNA_N
ClientSampleId :



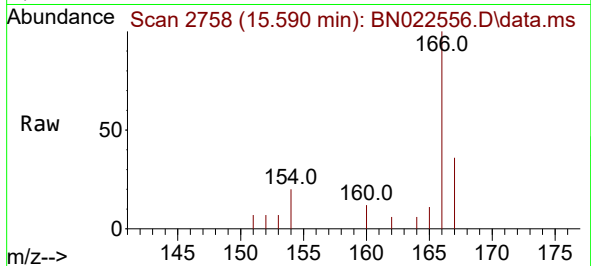



Tgt Ion:166 Resp: 1107
Ion Ratio Lower Upper
166 100
165 10.8 78.2 117.2#
167 36.3 11.0 16.4#

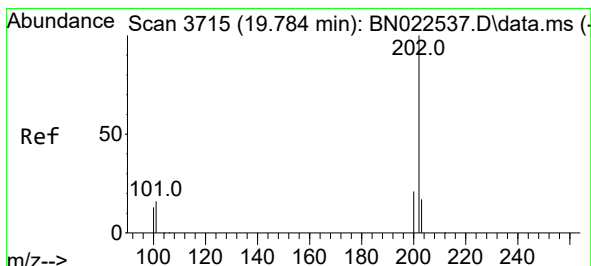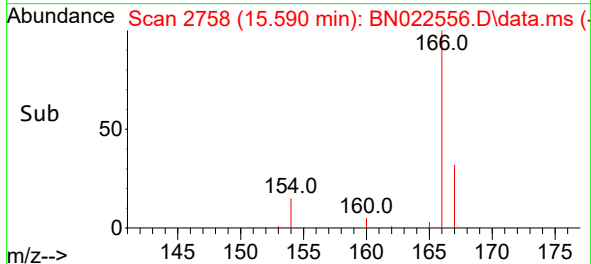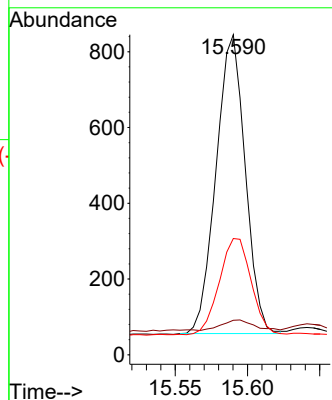

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.756 min Scan# 3709
Delta R.T. -0.028 min
Lab File: BN022556.D
Acq: 08 Nov 2022 11:35


Tgt Ion:202 Resp: 1023
Ion Ratio Lower Upper
202 100
101 186.4 13.1 19.7#
100 1325.3 10.6 16.0#

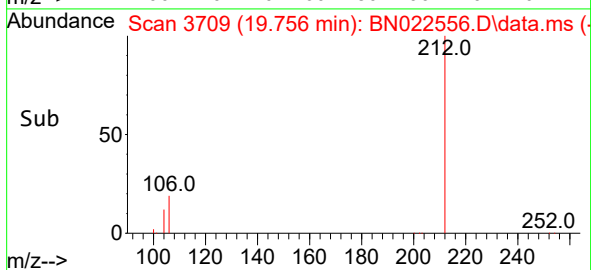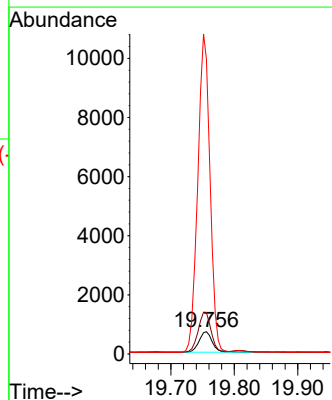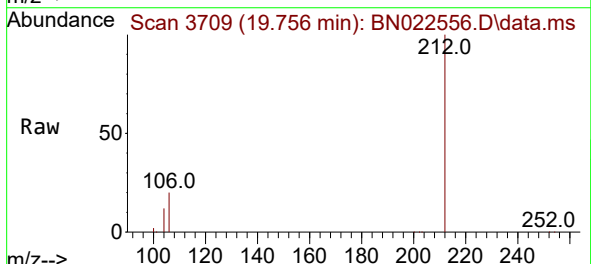

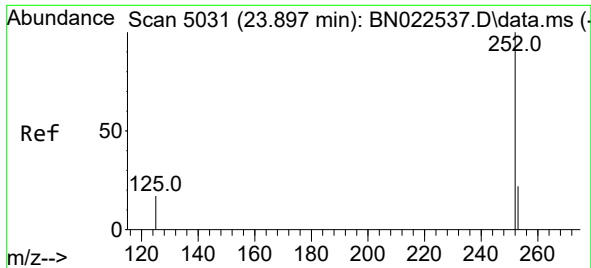

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.847 min Scan# 50
Delta R.T. -0.047 min
Lab File: BN022556.D
Acq: 08 Nov 2022 11:35

Instrument :
BNA_N
ClientSampleId :

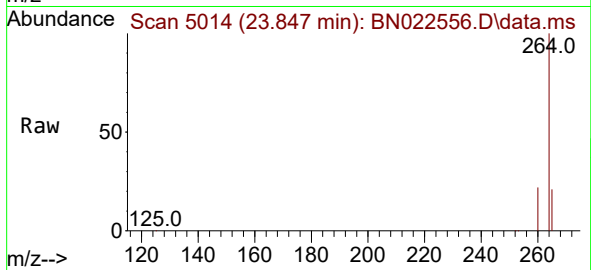

Tgt Ion:252 Resp: 1838
Ion Ratio Lower Upper
252 100
253 55.3 21.0 31.6#
125 55.1 17.9 26.9#

