

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022557.D
 Acq On : 08 Nov 2022 12:13
 Operator : CG/JU
 Sample : PB148837BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 09 01:21:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	1379	0.400	ng/ul	0.00
4) Naphthalene-d8	10.734	136	4850	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.591	164	3135	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.349	188	6952	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	5665	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264	4960	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.219	96	11955	6.671	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.340	152	2848	0.388	ng/ul	0.00
18) Fluoranthene-d10	19.384	212	6964	0.366	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.585	166	1027	0.074	ng/ul#	16
20) Pyrene	19.751	202	975	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.839	252	1858	0.094	ng/ul#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022557.D
Acq On : 08 Nov 2022 12:13
Operator : CG/JU
Sample : PB148837BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Nov 09 01:21:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

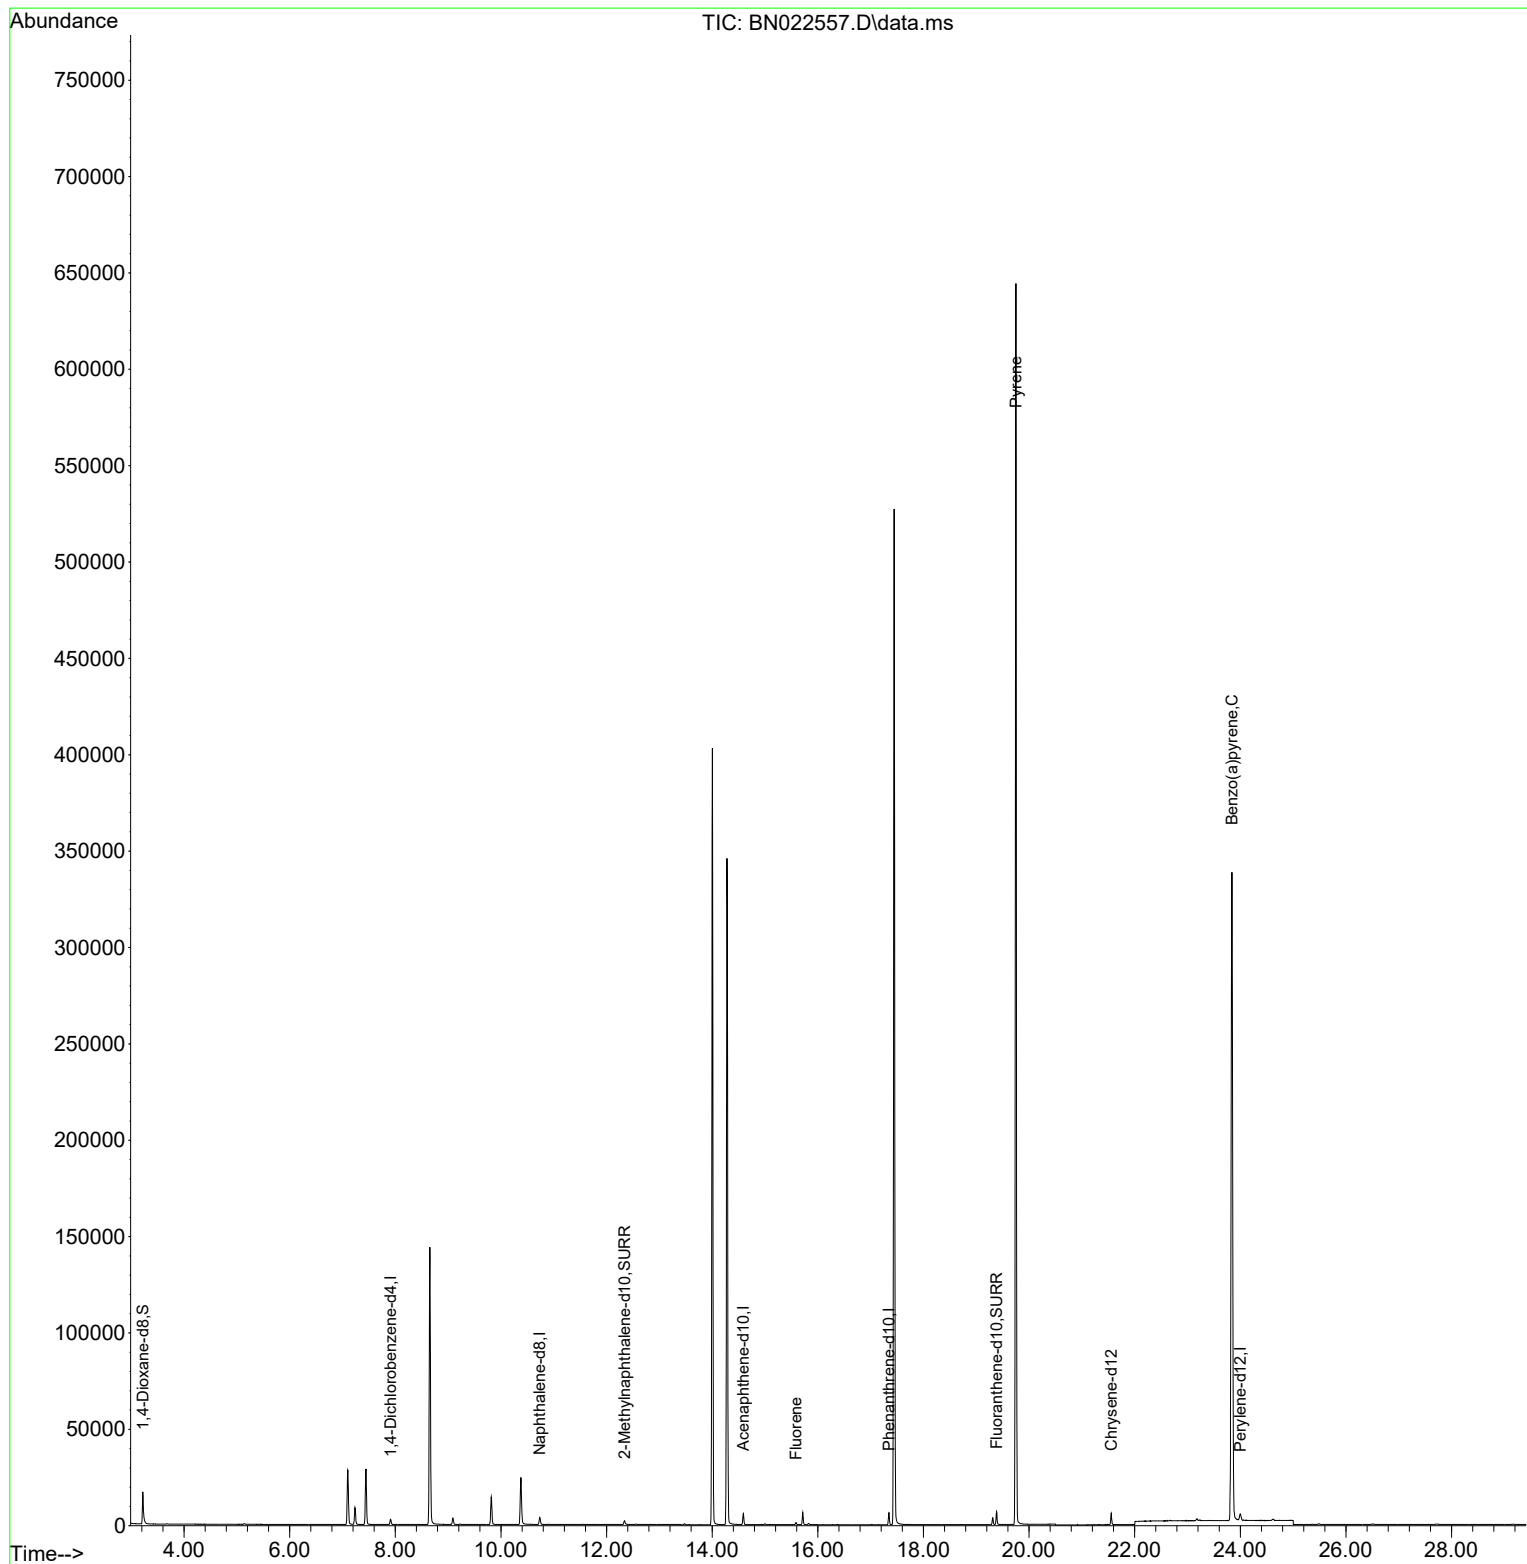



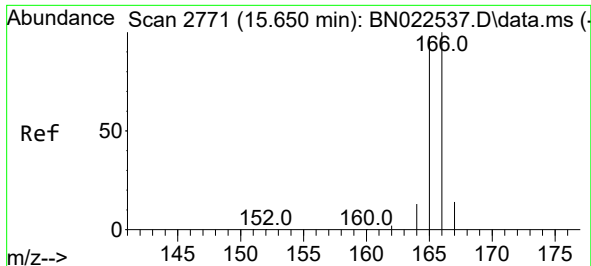


#12
Fluorene
Concen: 0.074 ng/ul
RT: 15.585 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN022557.D
Acq: 08 Nov 2022 12:13

Instrument :
BNA_N
ClientSampleId :



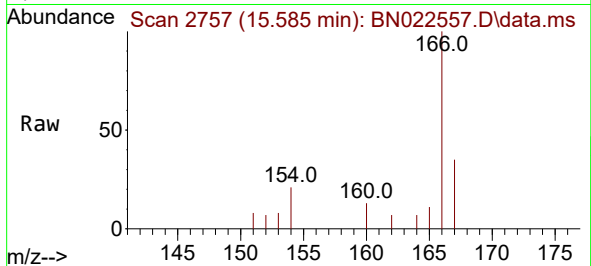



Tgt Ion:166 Resp: 1027
Ion Ratio Lower Upper
166 100
165 10.9 78.2 117.2#
167 35.3 11.0 16.4#

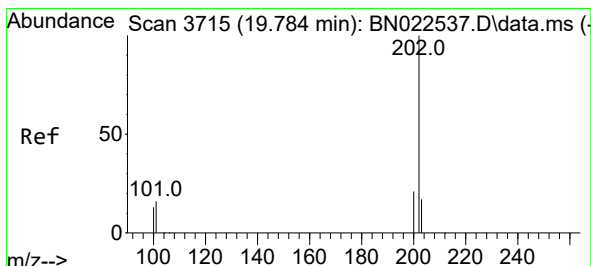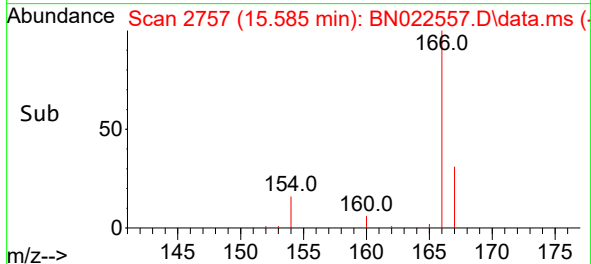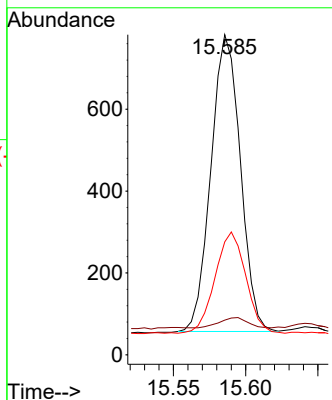

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.751 min Scan# 3708
Delta R.T. -0.033 min
Lab File: BN022557.D
Acq: 08 Nov 2022 12:13


Tgt Ion:202 Resp: 975
Ion Ratio Lower Upper
202 100
101 187.6 13.1 19.7#
100 1353.8 10.6 16.0#

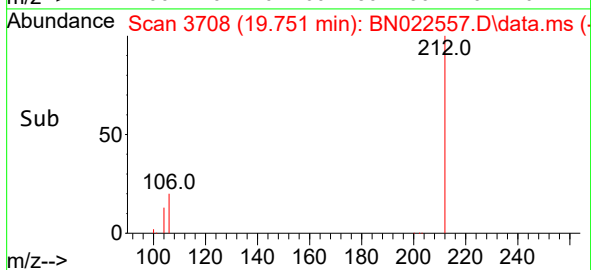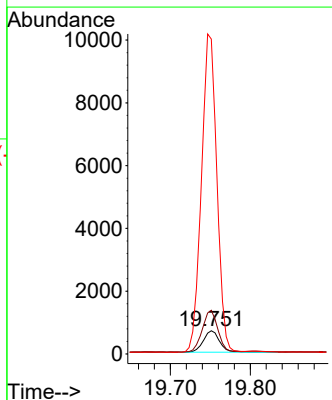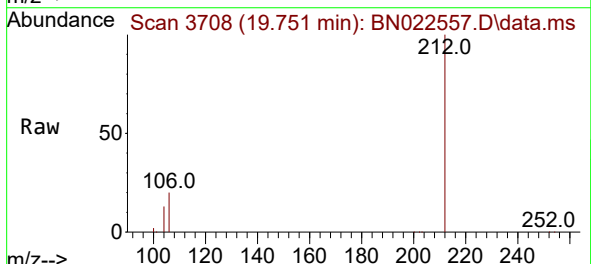

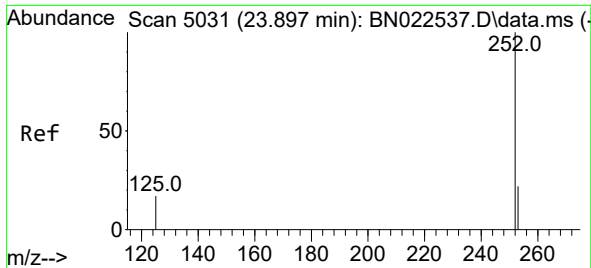

#26
 Benzo(a)pyrene
 Concen: 0.094 ng/ul
 RT: 23.839 min Scan# 5011
 Delta R.T. -0.056 min
 Lab File: BN022557.D
 Acq: 08 Nov 2022 12:13

Instrument :
 BNA_N
 ClientSampleId :

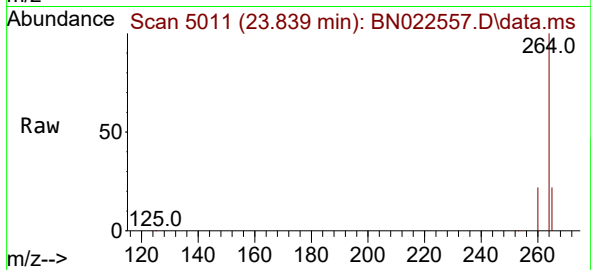

Tgt Ion:252 Resp: 1858
 Ion Ratio Lower Upper
 252 100
 253 56.1 21.0 31.6#
 125 56.3 17.9 26.9#

