

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022565.D
 Acq On : 08 Nov 2022 17:53
 Operator : CG/JU
 Sample : N5408-15
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 09 01:22:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	1627	0.400	ng/ul	0.00
4) Naphthalene-d8	10.734	136	5693	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.586	164	3586	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.345	188	8013	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	6391	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264	5340	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.219	96	7452	3.524	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.334	152	2725	0.316	ng/ul	-0.01
18) Fluoranthene-d10	19.384	212	8372	0.390	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.257	88	398	0.183	ng/ul#	69
20) Pyrene	19.751	202	1093	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.839	252	2008	0.094	ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022565.D
Acq On : 08 Nov 2022 17:53
Operator : CG/JU
Sample : N5408-15
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Nov 09 01:22:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

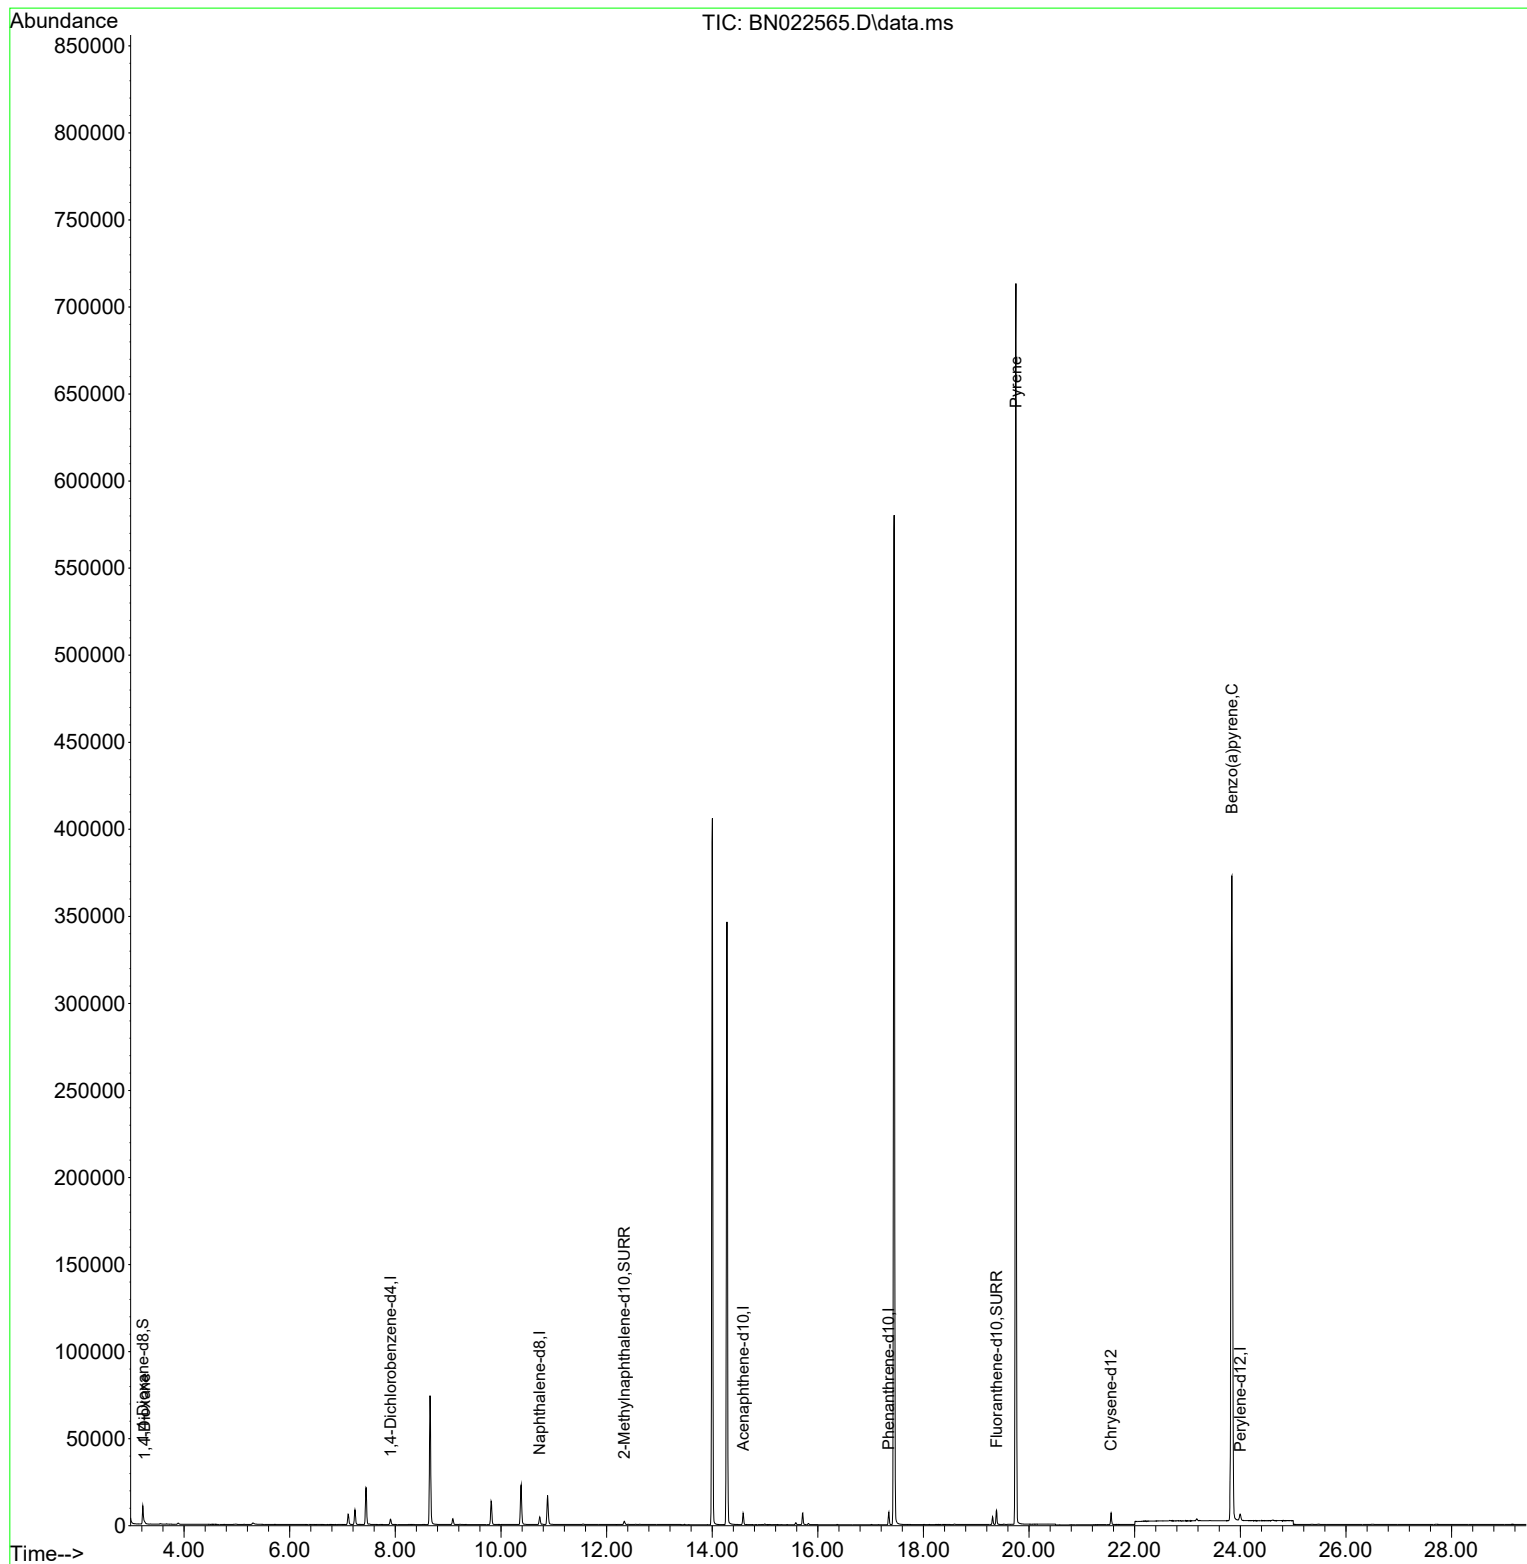



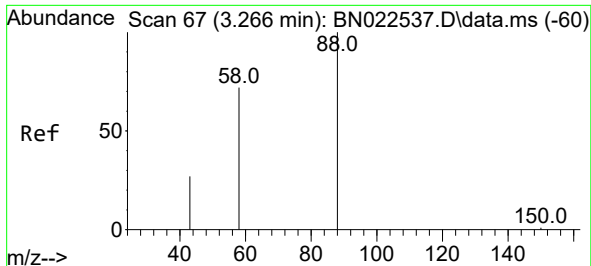


#2
1,4-Dioxane
Concen: 0.183 ng/ul
RT: 3.257 min Scan# 61
Delta R.T. -0.004 min
Lab File: BN022565.D
Acq: 08 Nov 2022 17:53

Instrument :
BNA_N
ClientSampleId :



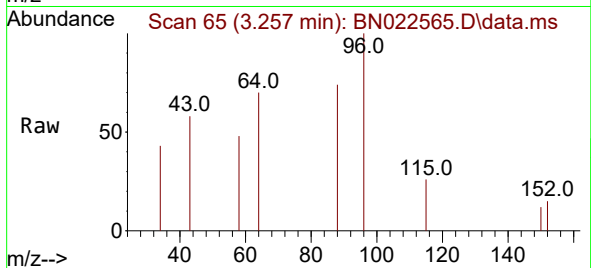



Tgt Ion: 88 Resp: 398
Ion Ratio Lower Upper
88 100
43 78.3 27.4 41.2#
58 64.2 48.2 72.2

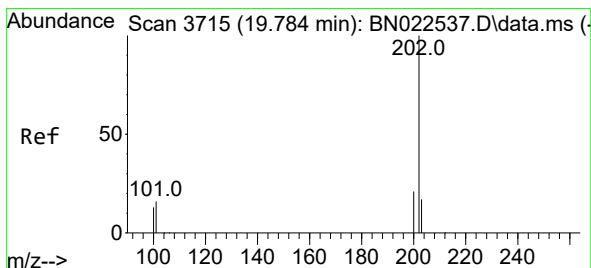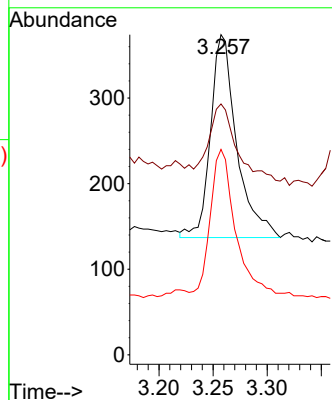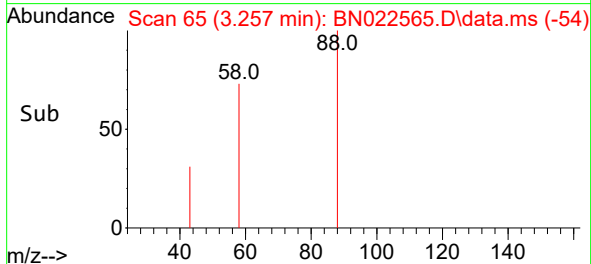

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.751 min Scan# 3708
Delta R.T. -0.033 min
Lab File: BN022565.D
Acq: 08 Nov 2022 17:53


Tgt Ion: 202 Resp: 1093
Ion Ratio Lower Upper
202 100
101 185.2 13.1 19.7#
100 1342.1 10.6 16.0#

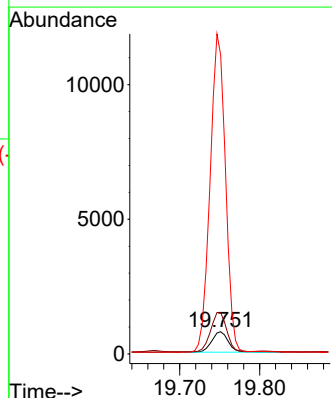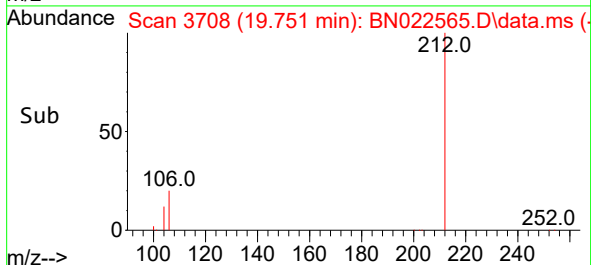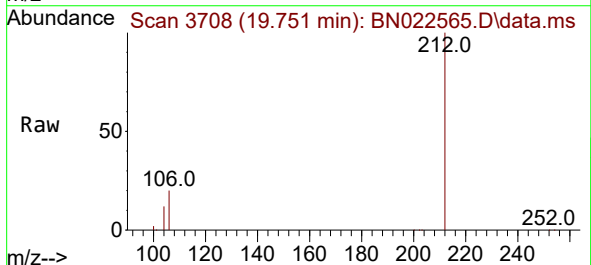

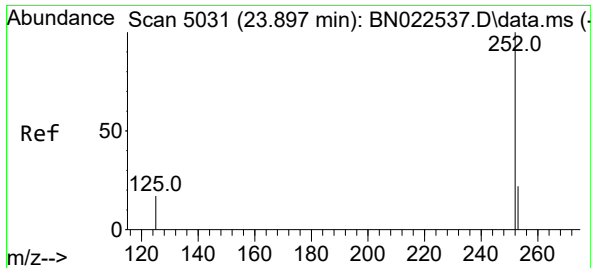

#26
 Benzo(a)pyrene
 Concen: 0.094 ng/ul
 RT: 23.839 min Scan# 5011
 Delta R.T. -0.056 min
 Lab File: BN022565.D
 Acq: 08 Nov 2022 17:53

Instrument :
 BNA_N
 ClientSampleId :

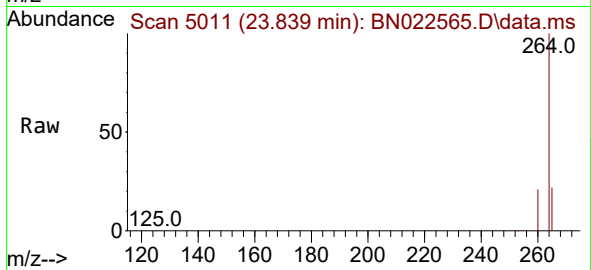

Tgt Ion:252 Resp: 2008
 Ion Ratio Lower Upper
 252 100
 253 56.3 21.0 31.6#
 125 53.5 17.9 26.9#

