

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022531.D
 Acq On : 07 Nov 2022 17:43
 Operator : CG/JU
 Sample : N5408-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

Quant Time: Nov 07 23:34:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:30:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	2141	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.749	136	7810m	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.599	164	5801m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.356	188	14247m	0.400	ng/ul	0.00
17) Chrysene-d12	21.561	240	10975m	0.400	ng/ul	0.00
23) Perylene-d12	24.017	264	8598m	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	17165	6.169	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.344	152	5905m	0.500	ng/ul	0.00
18) Fluoranthene-d10	19.396	212	12603m	0.342	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.261	88	43089	15.082	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022531.D
Acq On : 07 Nov 2022 17:43
Operator : CG/JU
Sample : N5408-01
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
EW4Y1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
Supervised By :mohammad ahmed 11/14/2022


Quant Time: Nov 07 23:34:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:30:37 2022
Response via : Initial Calibration

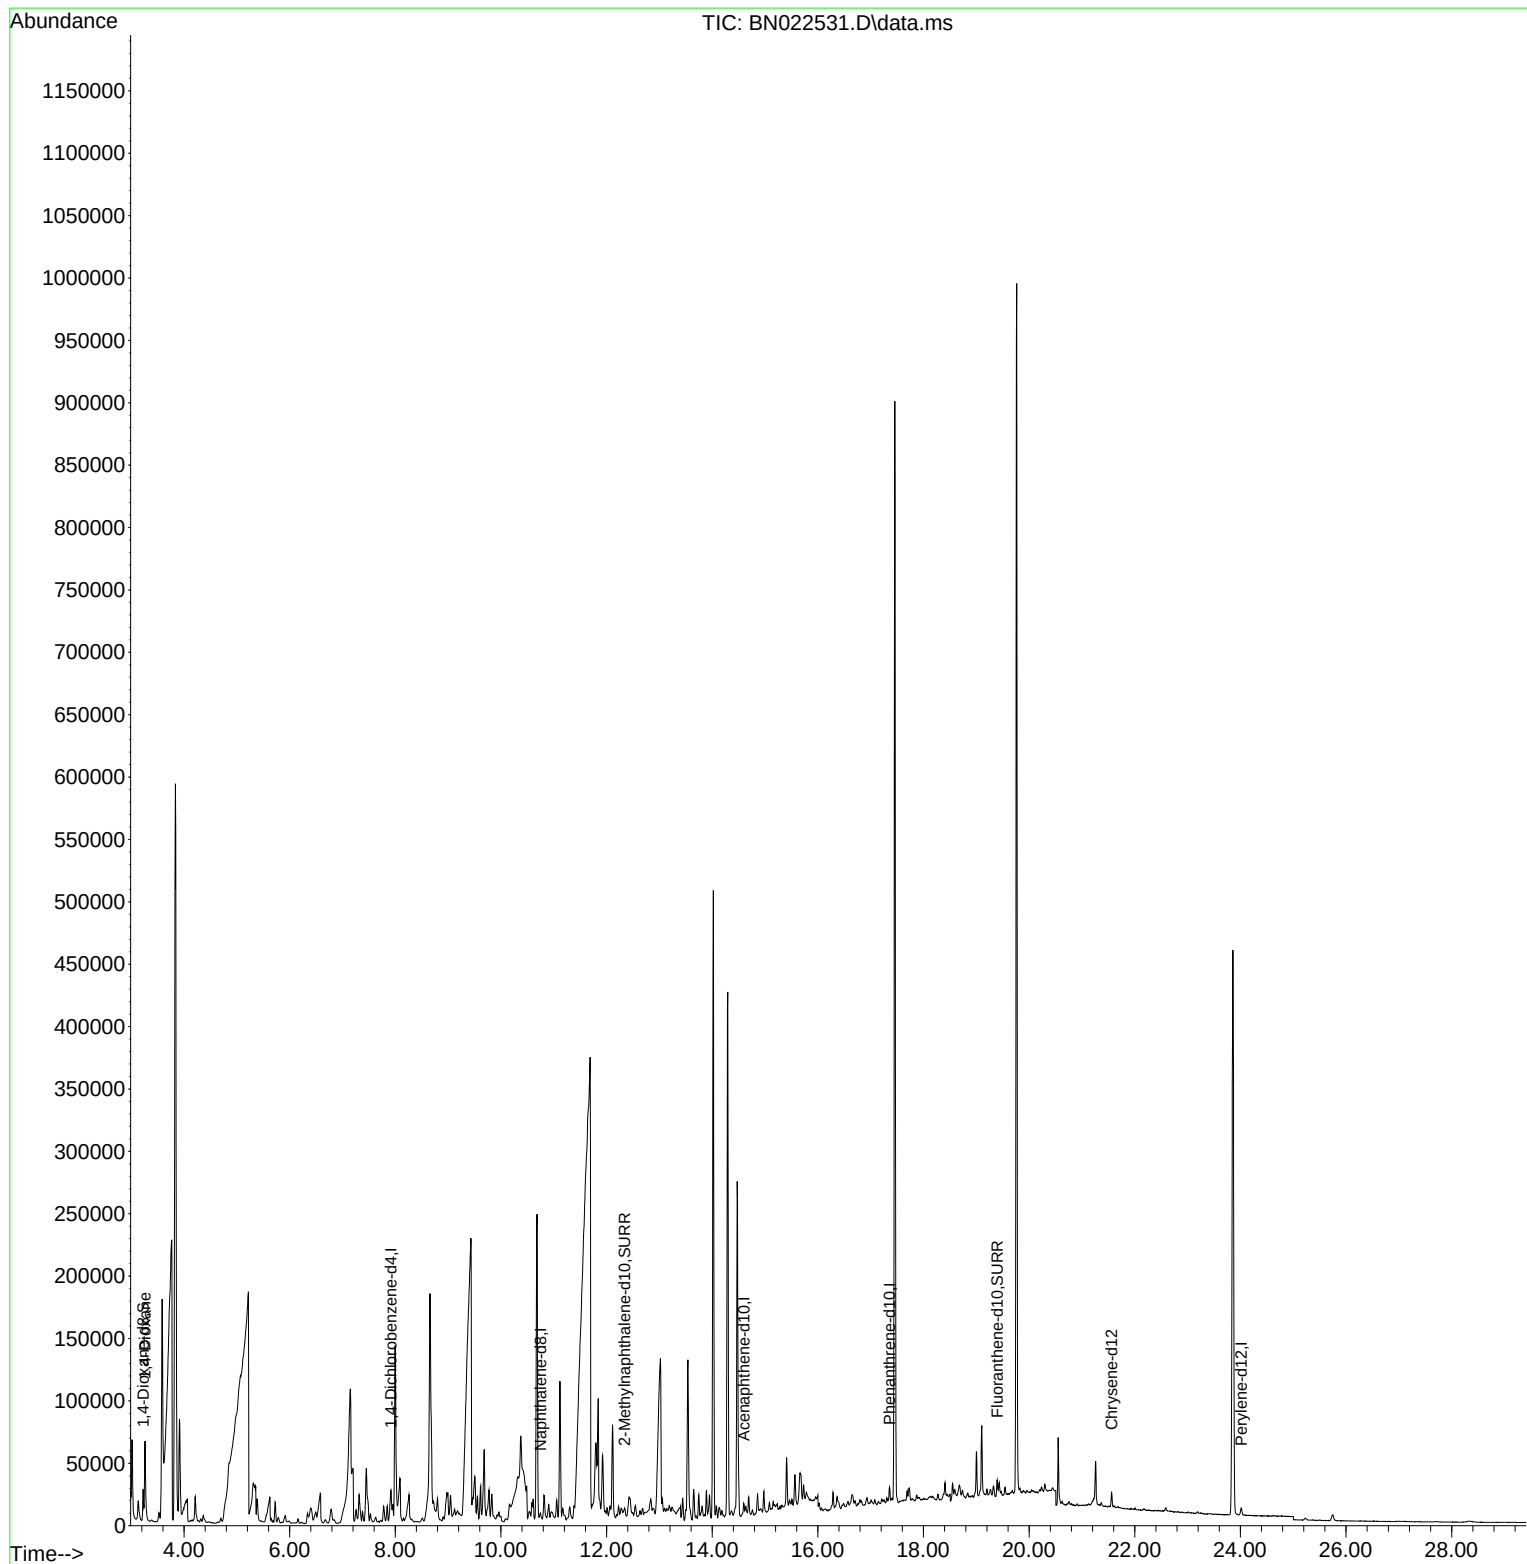

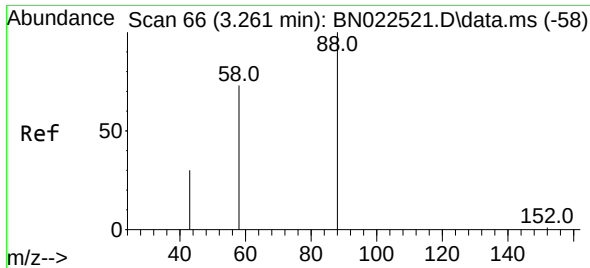

#2
 1,4-Dioxane
 Concen: 15.082 ng/ul
 RT: 3.261 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BN022531.D
 Acq: 07 Nov 2022 17:43

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y1

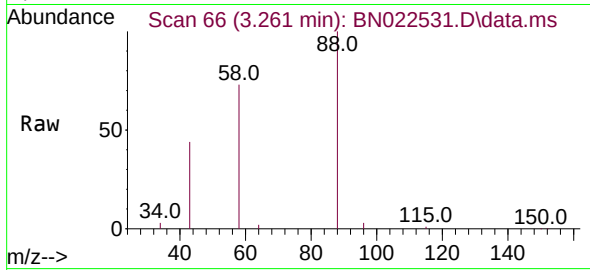

Tgt Ion: 88 Resp: 43089
 Ion Ratio Lower Upper
 88 100
 43 43.6 27.4 41.2
 58 73.4 48.2 72.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/08/2022
 Supervised By :mohammad ahmed 11/14/2022

