

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022533.D
 Acq On : 07 Nov 2022 19:02
 Operator : CG/JU
 Sample : N5408-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y2

Quant Time: Nov 08 00:06:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	2179	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.743	136	10398	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.599	164	10721	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.356	188	13651	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.561	240	11541	0.400	ng/ul	# 0.00
23) Perylene-d12	24.014	264	8386	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	18095	6.390	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.344	152	7073	0.450	ng/ul	0.00
18) Fluoranthene-d10	19.396	212	13501	0.348	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.261	88	23930	8.230	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022533.D
Acq On : 07 Nov 2022 19:02
Operator : CG/JU
Sample : N5408-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Y2


Quant Time: Nov 08 00:06:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

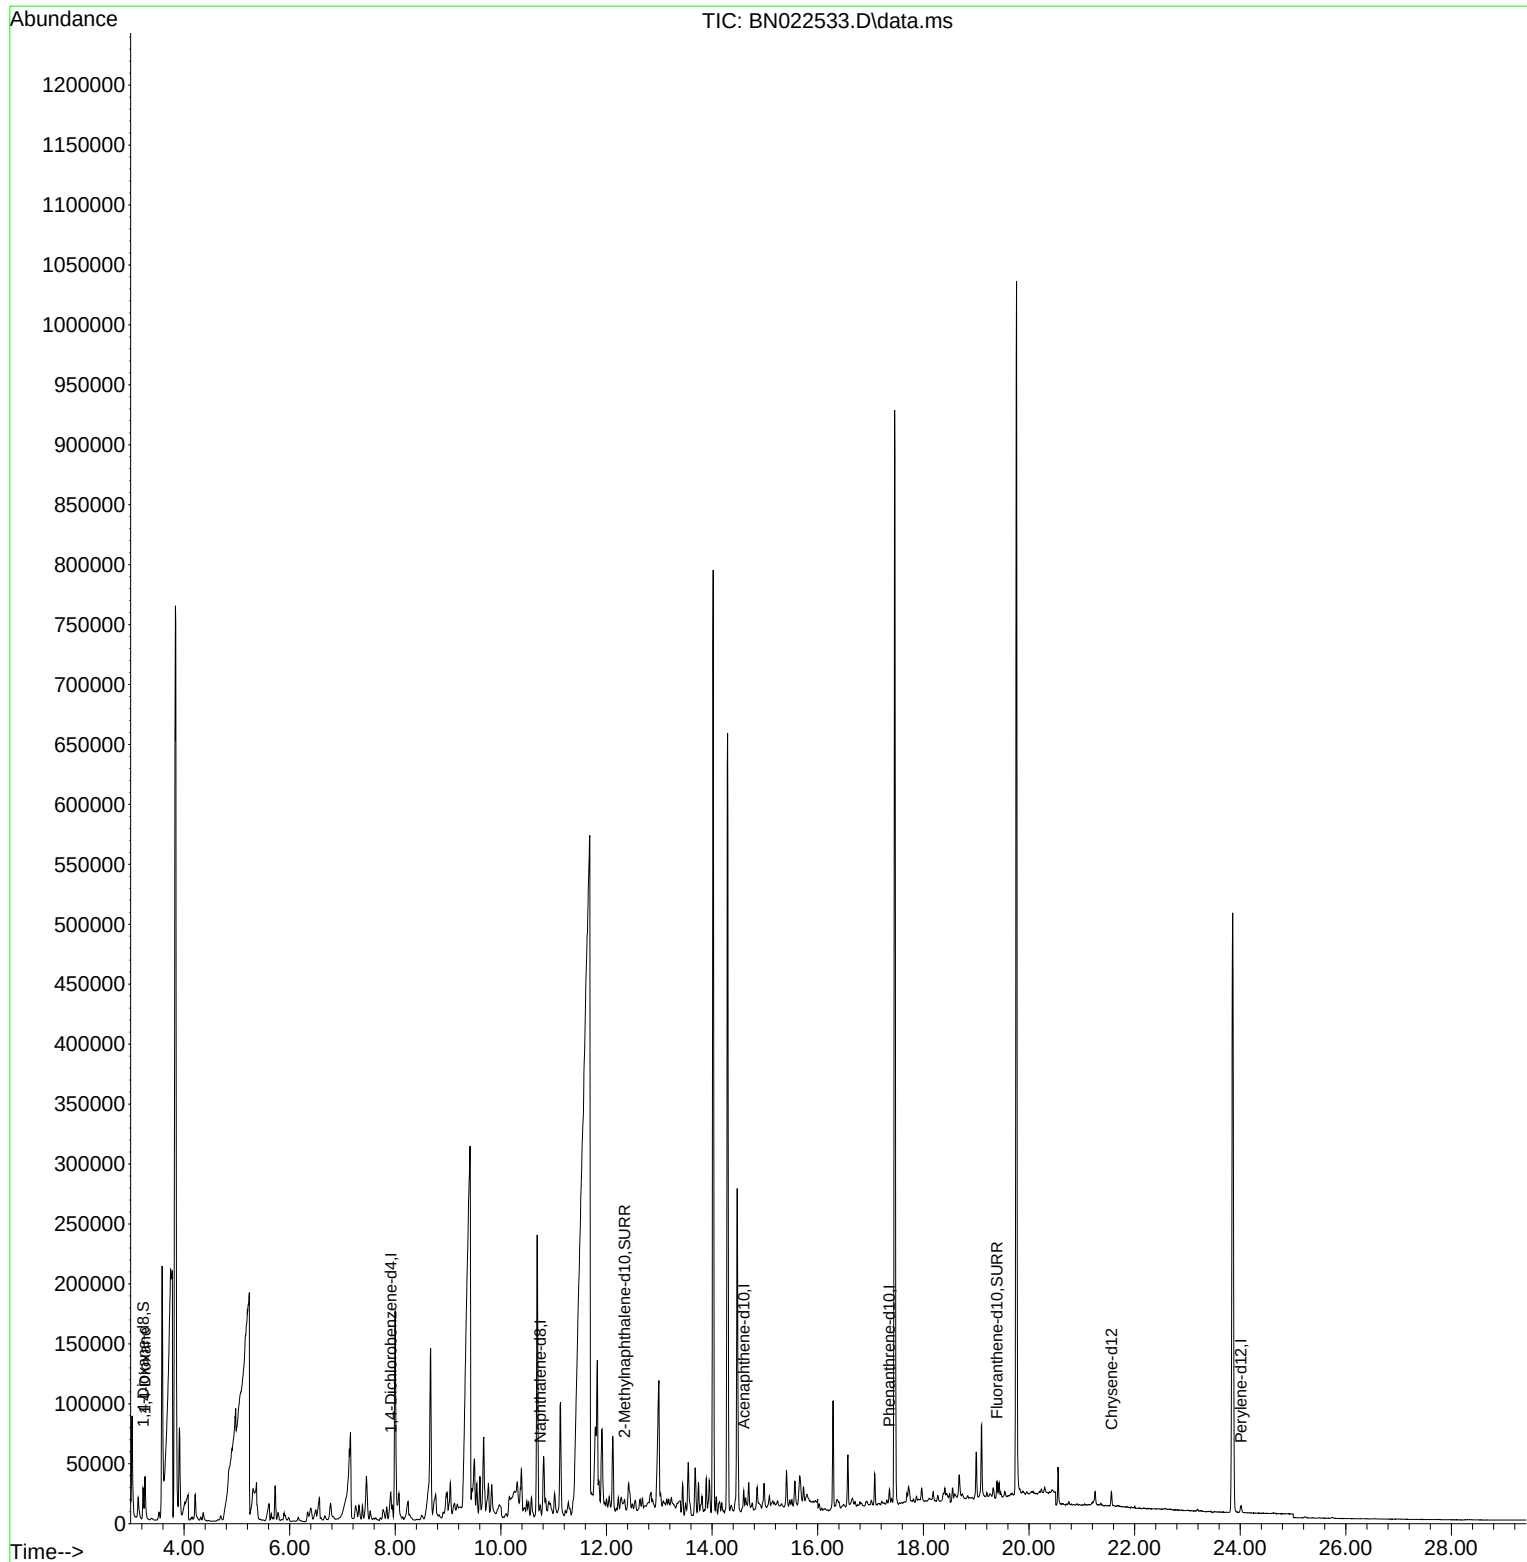

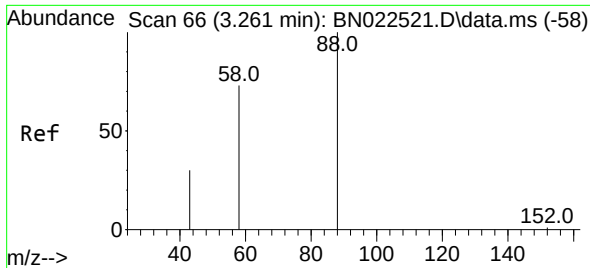

#2
 1,4-Dioxane
 Concen: 8.230 ng/ul
 RT: 3.261 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BN022533.D
 Acq: 07 Nov 2022 19:02

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y2

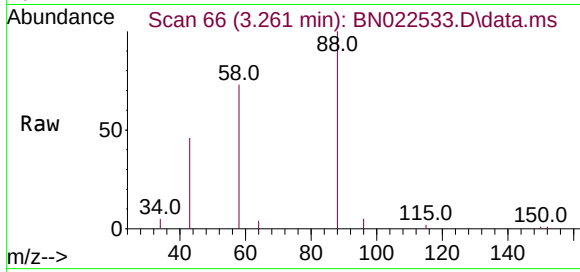

Tgt Ion:	88	Resp:	23930
Ion	Ratio	Lower	Upper
88	100		
43	46.1	27.4	41.2#
58	72.9	48.2	72.2#

