

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022535.D
 Acq On : 07 Nov 2022 20:20
 Operator : CG/JU
 Sample : N5408-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y3

Quant Time: Nov 07 23:35:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:30:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	3378	0.400	ng/u1	0.00
4) Naphthalene-d8	10.745	136	9933	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.595	164	7541	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.353	188	17058	0.400	ng/u1	0.00
17) Chrysene-d12	21.561	240	13351	0.400	ng/u1	0.00
23) Perylene-d12	24.011	264	11052	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	14782	3.367	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.345	152	5862	0.390	ng/u1	0.00
18) Fluoranthene-d10	19.393	212	17137	0.382	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.265	88	714	0.158	ng/u1#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022535.D
Acq On : 07 Nov 2022 20:20
Operator : CG/JU
Sample : N5408-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Y3


Quant Time: Nov 07 23:35:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:30:37 2022
Response via : Initial Calibration

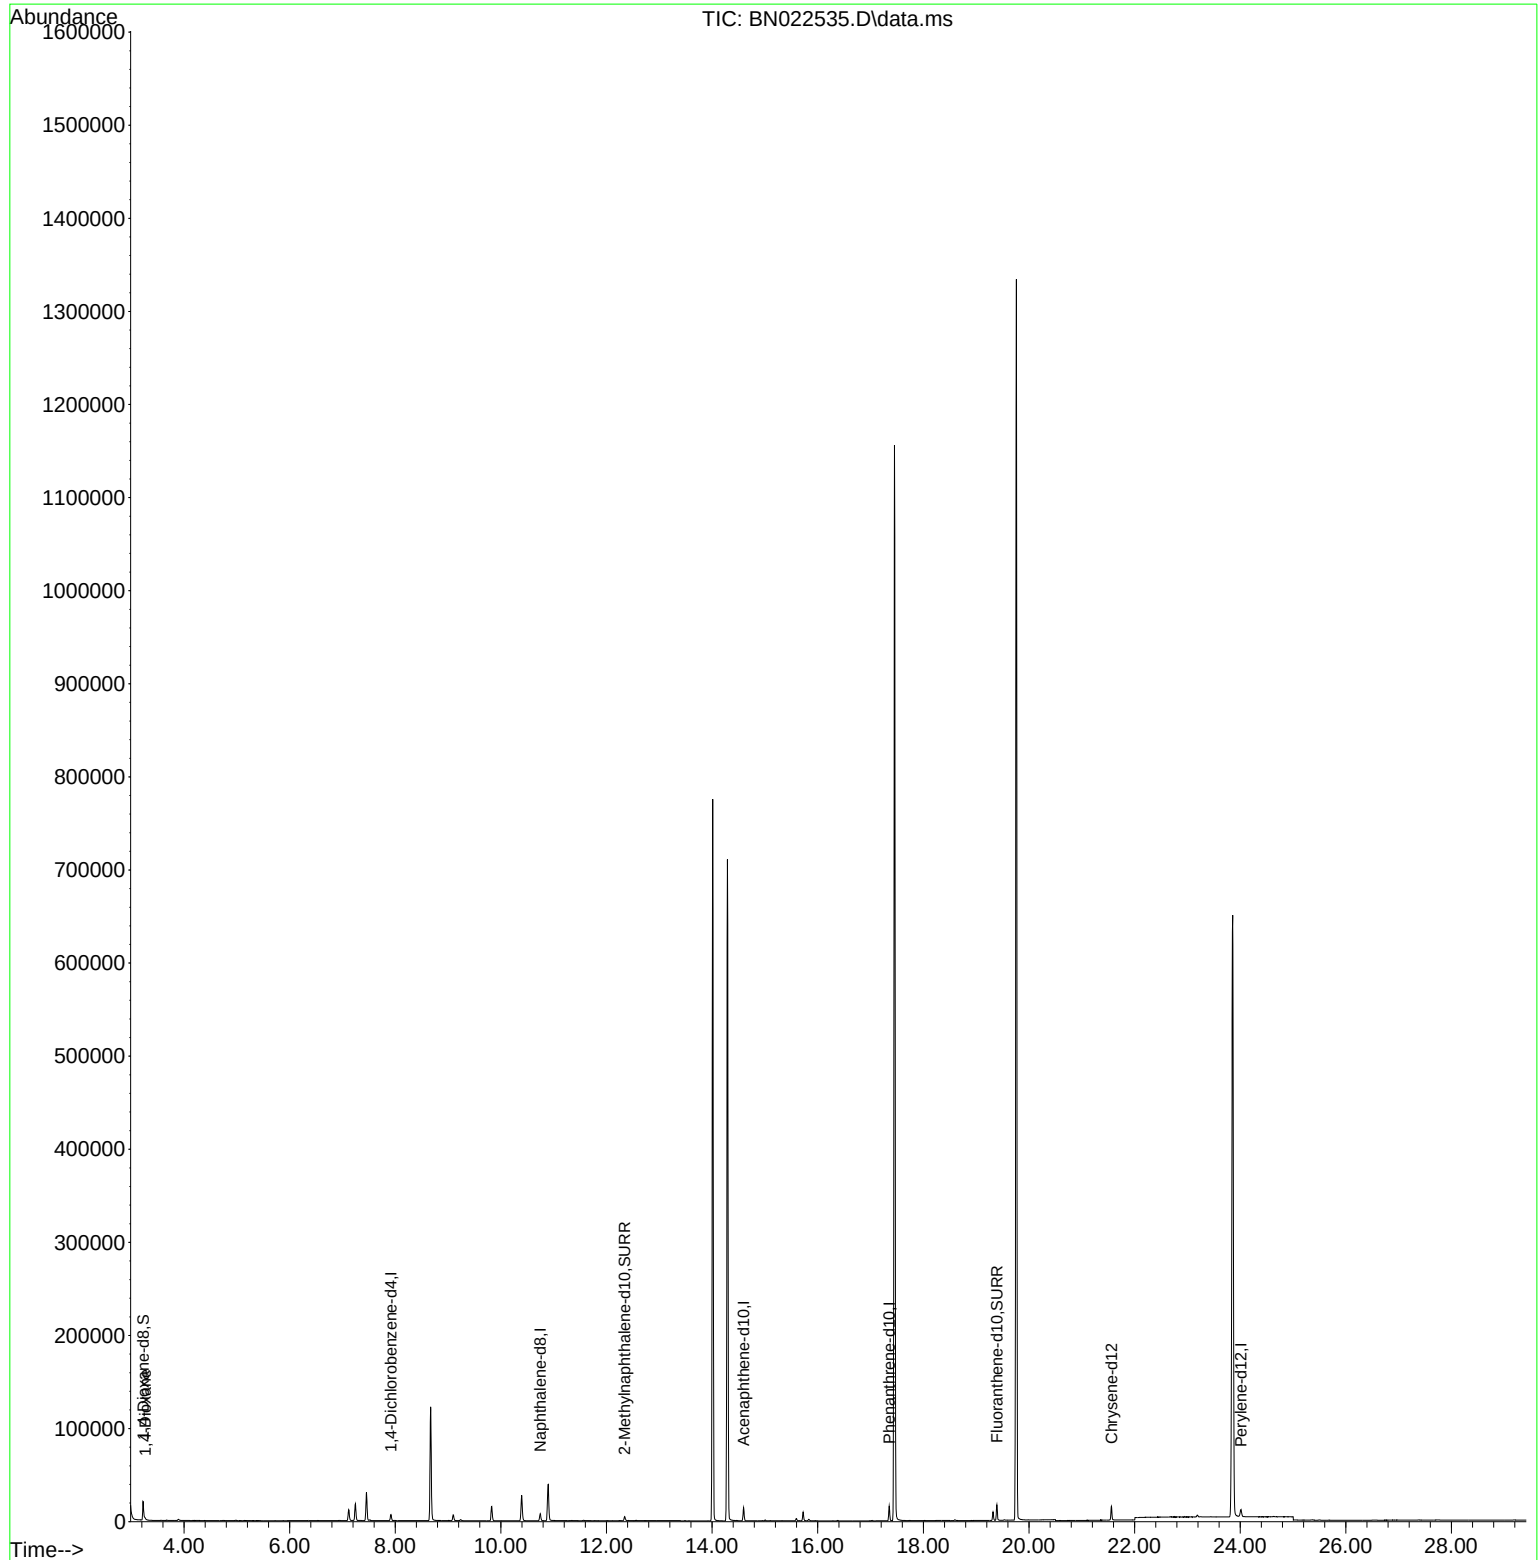

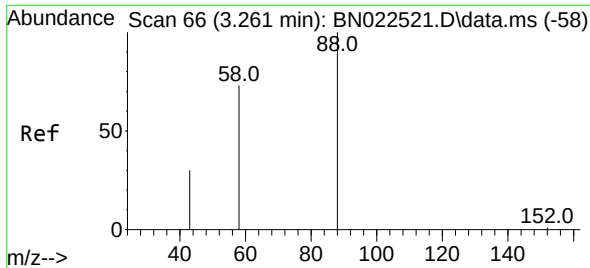

#2
 1,4-Dioxane
 Concen: 0.158 ng/ul
 RT: 3.265 min Scan# 61
 Delta R.T. 0.004 min
 Lab File: BN022535.D
 Acq: 07 Nov 2022 20:20

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y3

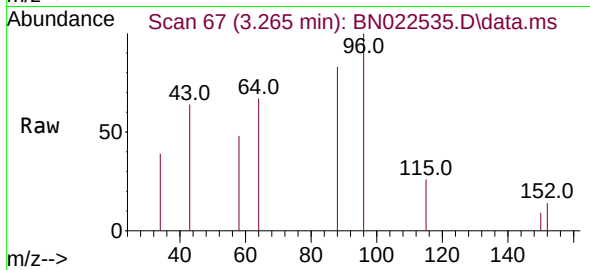

Tgt Ion: 88 Resp: 714

Ion	Ratio	Lower	Upper
88	100		
43	76.9	27.4	41.2#
58	57.6	48.2	72.2

