

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022541.D
 Acq On : 08 Nov 2022 00:46
 Operator : CG/JU
 Sample : N5408-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y5

Quant Time: Nov 08 02:06:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.915	152	1867	0.400	ng/ul	0.00
4) Naphthalene-d8	10.739	136	6630	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.591	164	4319	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.349	188	9761	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	8113	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264	6845	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	9255	3.814	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	3621	0.361	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	10407	0.382	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.261	88	488	0.196	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022541.D
Acq On : 08 Nov 2022 00:46
Operator : CG/JU
Sample : N5408-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Y5


Quant Time: Nov 08 02:06:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

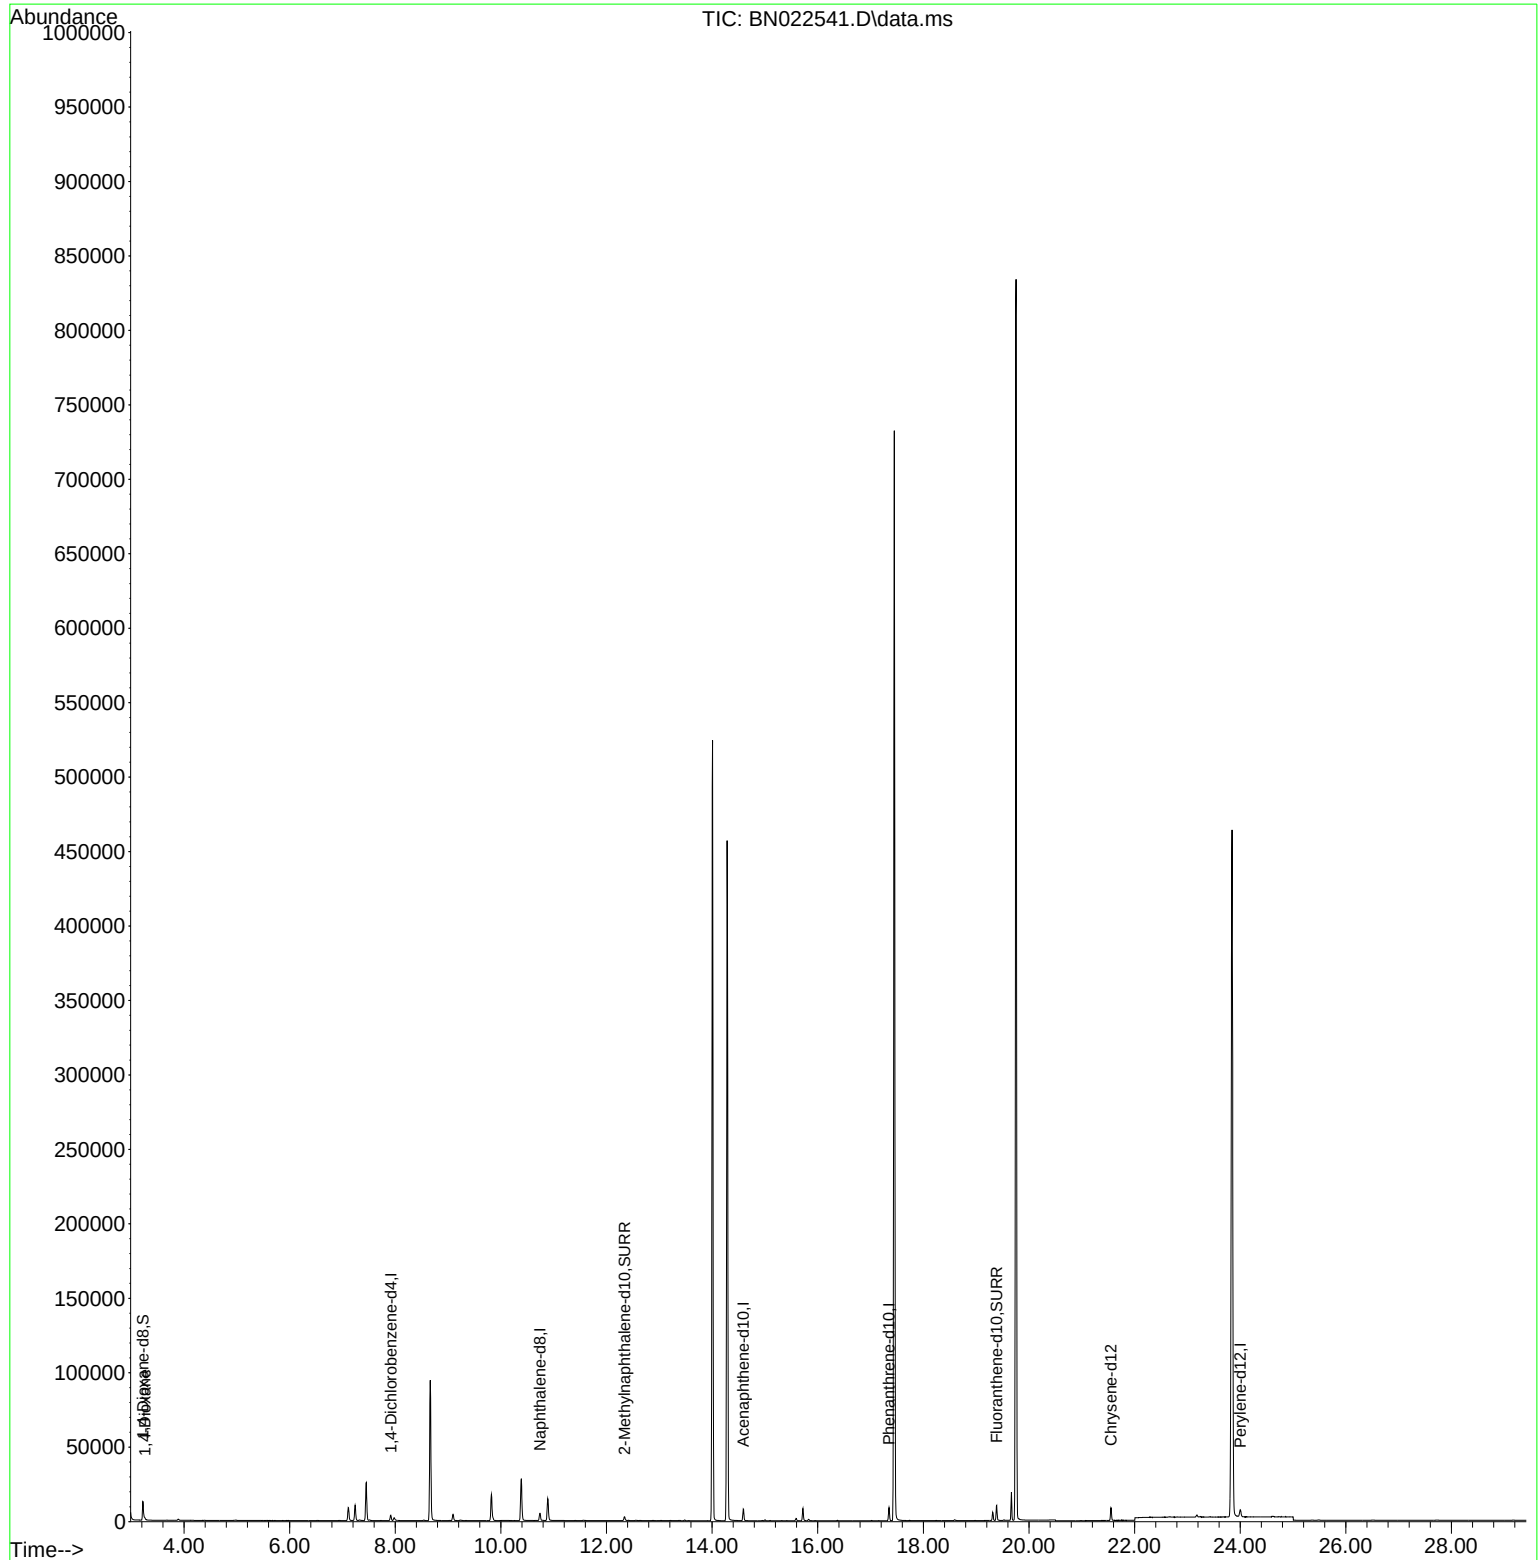

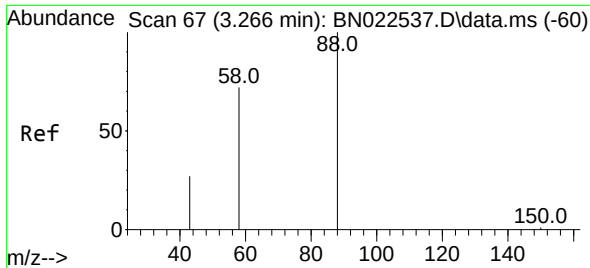

#2
 1,4-Dioxane
 Concen: 0.196 ng/ul
 RT: 3.261 min Scan# 60
 Delta R.T. 0.000 min
 Lab File: BN022541.D
 Acq: 08 Nov 2022 00:46

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y5

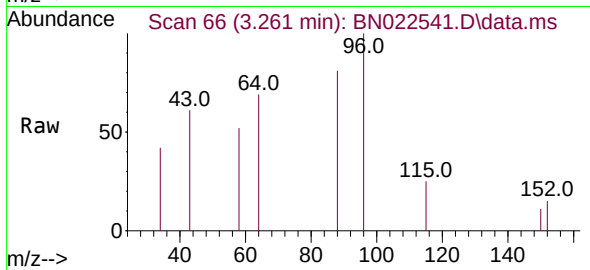

Tgt Ion: 88 Resp: 488

Ion	Ratio	Lower	Upper
88	100		
43	76.3	27.4	41.2#
58	64.9	48.2	72.2

