

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022543.D
 Acq On : 08 Nov 2022 02:01
 Operator : CG/JU
 Sample : N5408-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y6

Quant Time: Nov 08 03:27:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	2306	0.400	ng/ul	0.00
4) Naphthalene-d8	10.739	136	8081	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.591	164	5295	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.349	188	11668	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	9591	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264	7882	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	7134	2.380	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.340	152	826	0.068	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	2210	0.069	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.261	88	464	0.151	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\  
Data File : BN022543.D  
Acq On    : 08 Nov 2022  02:01  
Operator  : CG/JU  
Sample    : N5408-06  
Misc      :  
ALS Vial  : 24    Sample Multiplier: 1
```


Quant Time: Nov 08 03:27:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

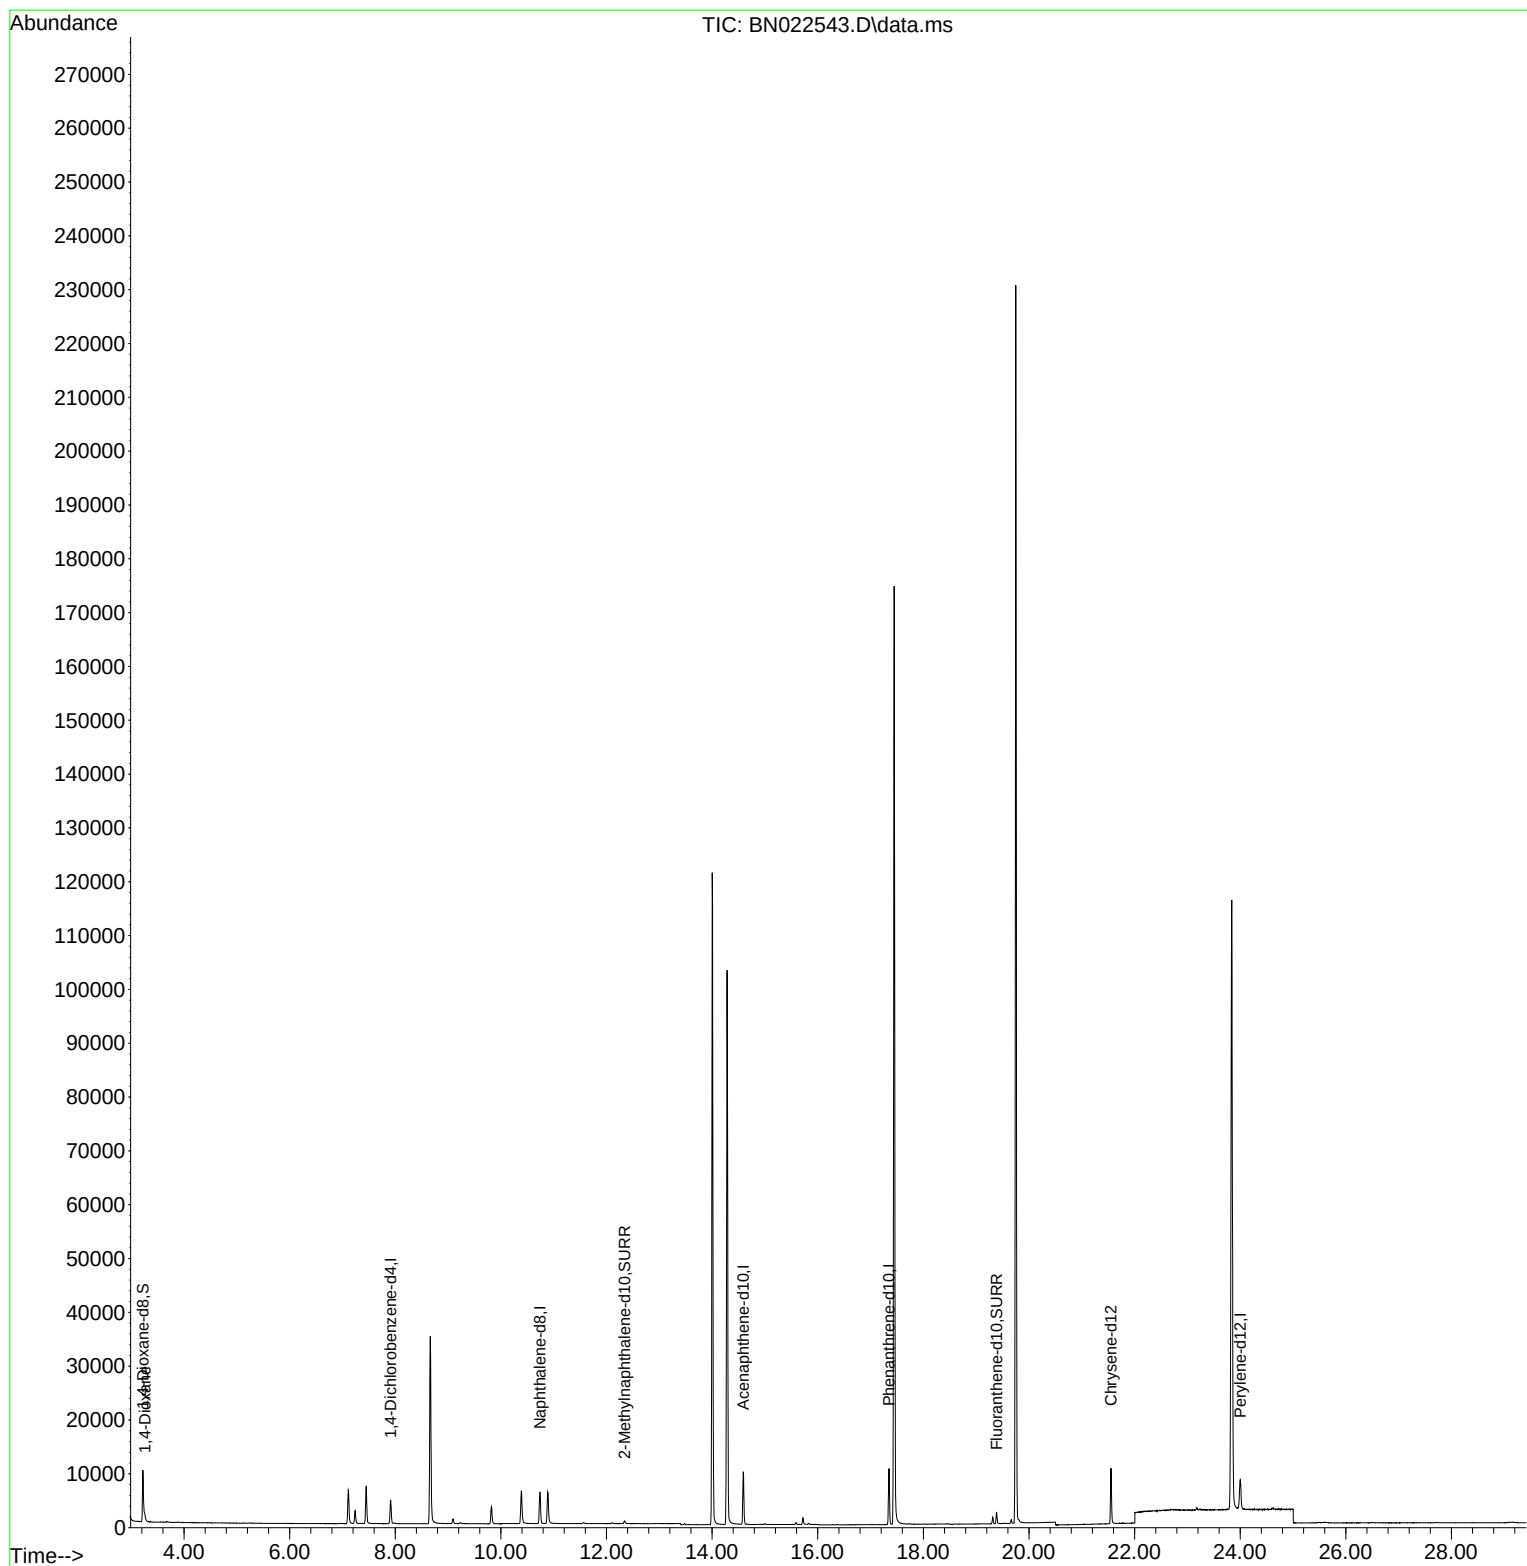

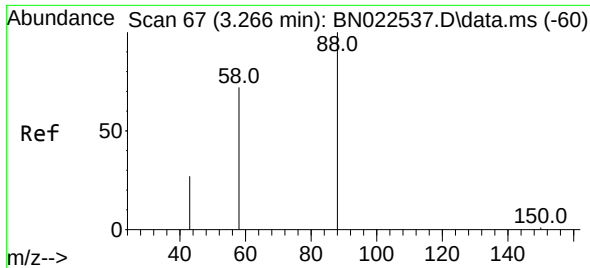

#2
 1,4-Dioxane
 Concen: 0.151 ng/ul
 RT: 3.261 min Scan# 60
 Delta R.T. 0.000 min
 Lab File: BN022543.D
 Acq: 08 Nov 2022 02:01

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y6

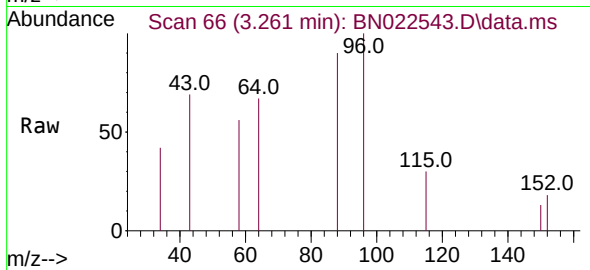

Tgt Ion: 88 Resp: 464
 Ion Ratio Lower Upper
 88 100
 43 76.1 27.4 41.2#
 58 61.7 48.2 72.2

