

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022549.D
 Acq On : 08 Nov 2022 05:43
 Operator : CG/JU
 Sample : N5408-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y9

Quant Time: Nov 08 06:29:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	1748	0.400	ng/ul	0.00
4) Naphthalene-d8	10.739	136	6171	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.591	164	3978	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.345	188	8903	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	7412	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264	6245	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.219	96	9125	4.017	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.340	152	3147	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.384	212	9032	0.363	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.257	88	405	0.174	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022549.D
Acq On : 08 Nov 2022 05:43
Operator : CG/JU
Sample : N5408-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Y9


Quant Time: Nov 08 06:29:54 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

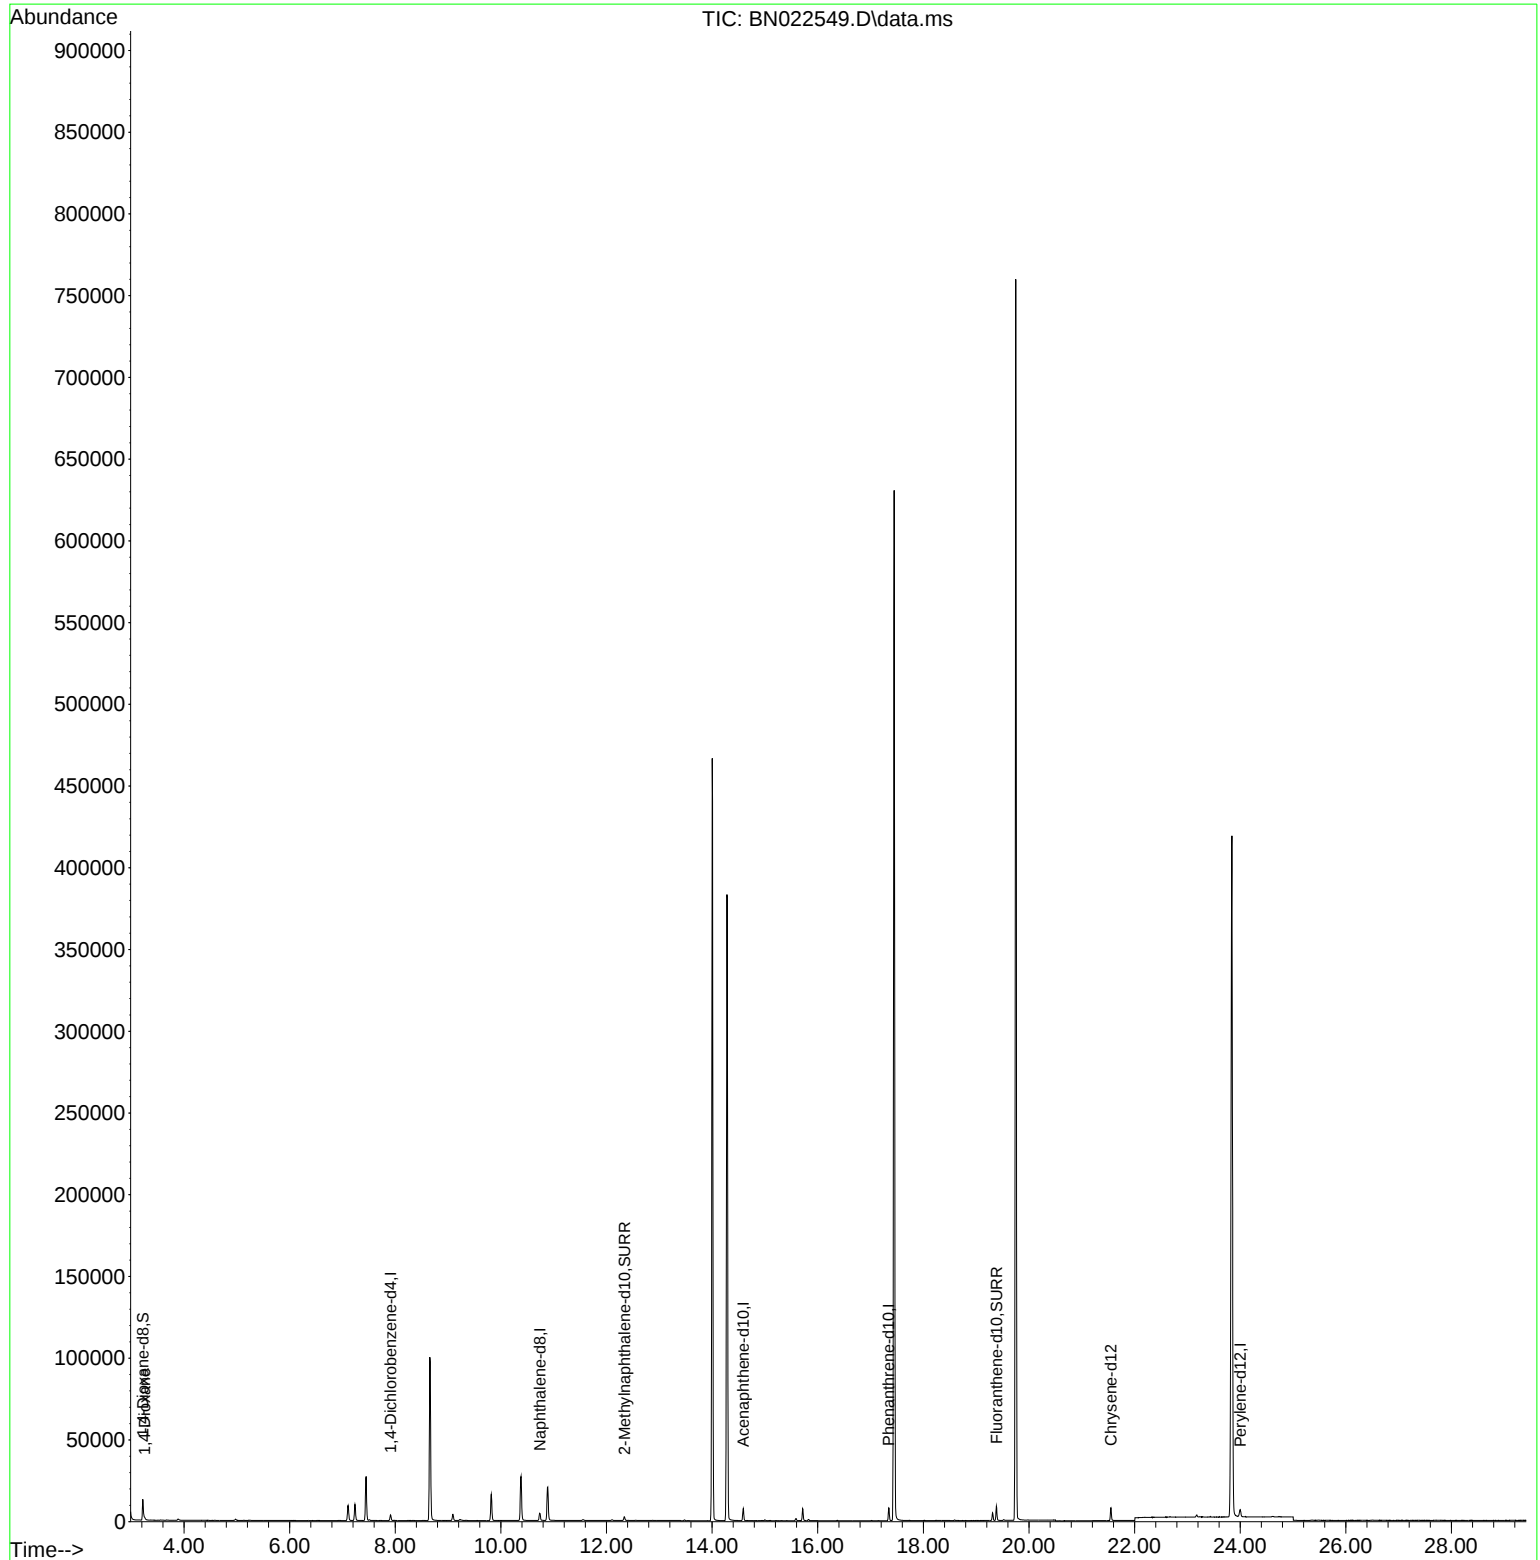

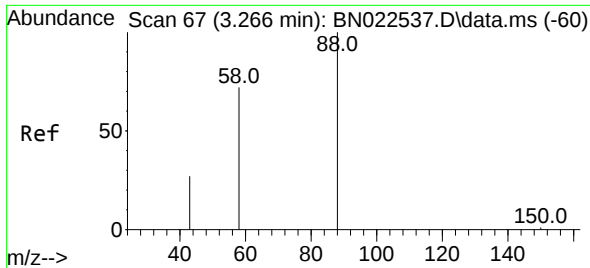

#2
 1,4-Dioxane
 Concen: 0.174 ng/ul
 RT: 3.257 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN022549.D
 Acq: 08 Nov 2022 05:43

Instrument :
 BNA_N
 ClientSampleId :
 EW4Y9

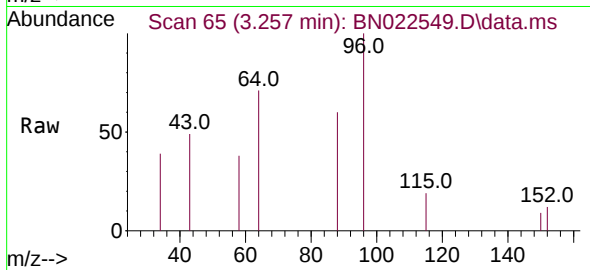

Tgt Ion: 88 Resp: 405

Ion	Ratio	Lower	Upper
88	100		
43	81.0	27.4	41.2#
58	64.0	48.2	72.2

