

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022551.D
 Acq On : 08 Nov 2022 06:57
 Operator : CG/JU
 Sample : N5408-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Z0

Quant Time: Nov 08 07:35:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	1681	0.400	ng/ul	0.00
4) Naphthalene-d8	10.733	136	5952	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.590	164	3818	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.349	188	8619	0.400	ng/ul	0.00
17) Chrysene-d12	21.552	240	7155	0.400	ng/ul	0.00
23) Perylene-d12	23.996	264	6143	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.219	96	10260	4.696	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	3695	0.410	ng/ul	0.00
18) Fluoranthene-d10	19.384	212	10890	0.453	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.261	88	464	0.207	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022551.D
Acq On : 08 Nov 2022 06:57
Operator : CG/JU
Sample : N5408-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Z0


Quant Time: Nov 08 07:35:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

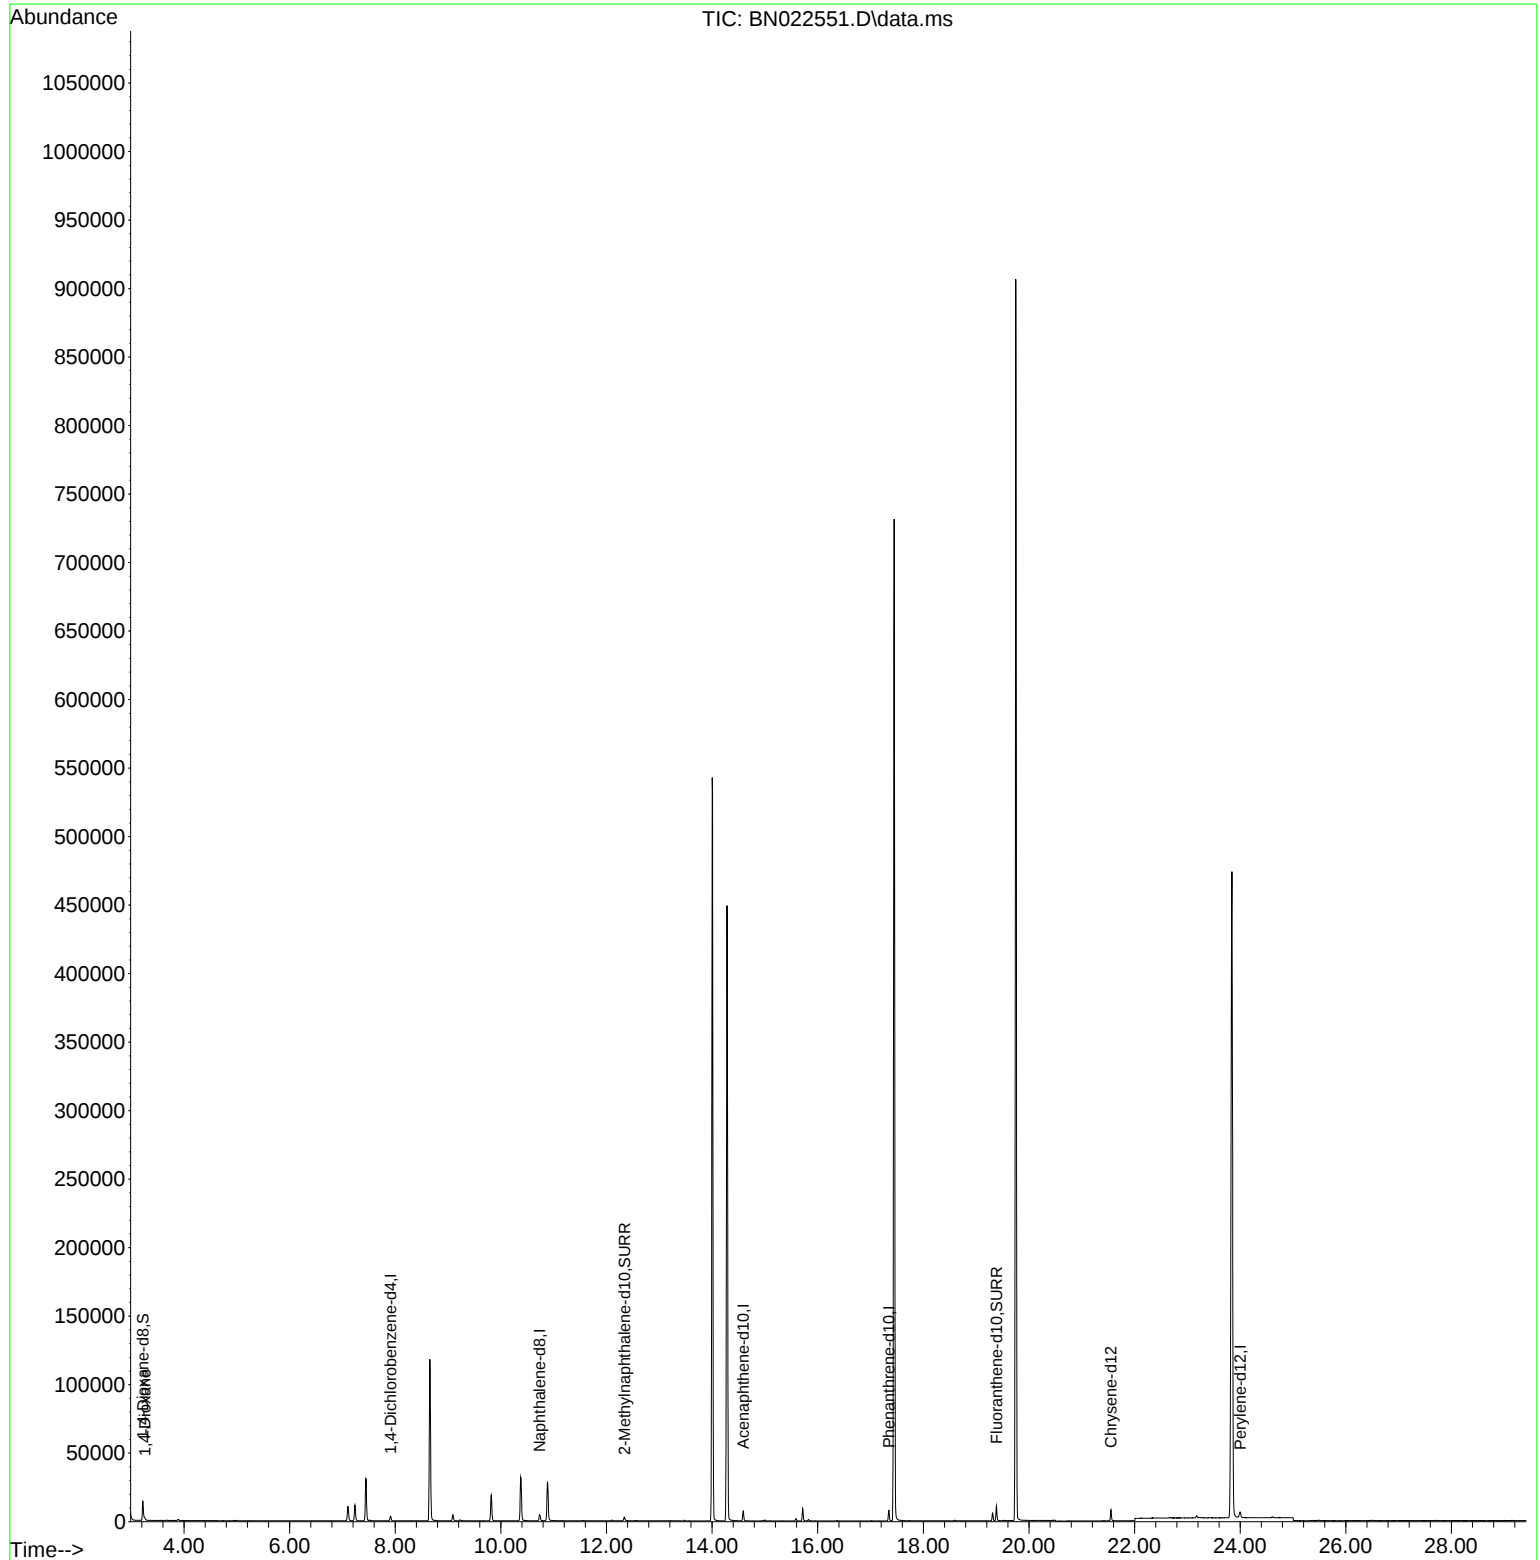

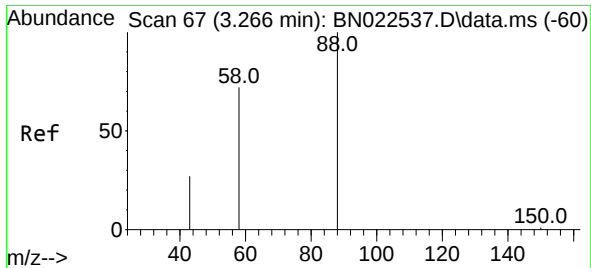

#2
 1,4-Dioxane
 Concen: 0.207 ng/ul
 RT: 3.261 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BN022551.D
 Acq: 08 Nov 2022 06:57

Instrument :
 BNA_N
 ClientSampleId :
 EW4Z0

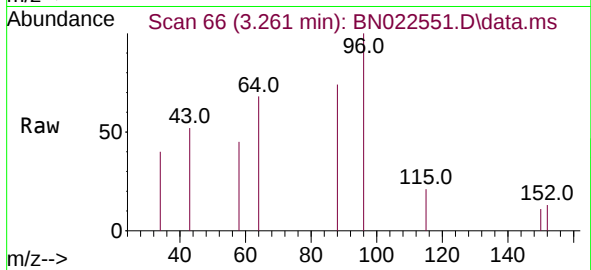

Tgt Ion: 88 Resp: 464

Ion	Ratio	Lower	Upper
88	100		
43	71.0	27.4	41.2#
58	61.0	48.2	72.2

