

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
 Data File : BN022563.D
 Acq On : 08 Nov 2022 16:38
 Operator : CG/JU
 Sample : N5408-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Z1

Quant Time: Nov 09 01:22:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 23:39:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	1359	0.400	ng/ul	0.00
4) Naphthalene-d8	10.734	136	4923	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.586	164	3087	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.345	188	6794	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	5463	0.400	ng/ul	0.00
23) Perylene-d12	23.996	264	4543	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.219	96	8110	4.592	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.334	152	2837	0.381	ng/ul	-0.01
18) Fluoranthene-d10	19.384	212	8602	0.469	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.257	88	349	0.192	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110722\
Data File : BN022563.D
Acq On : 08 Nov 2022 16:38
Operator : CG/JU
Sample : N5408-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Z1


Quant Time: Nov 09 01:22:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 23:39:33 2022
Response via : Initial Calibration

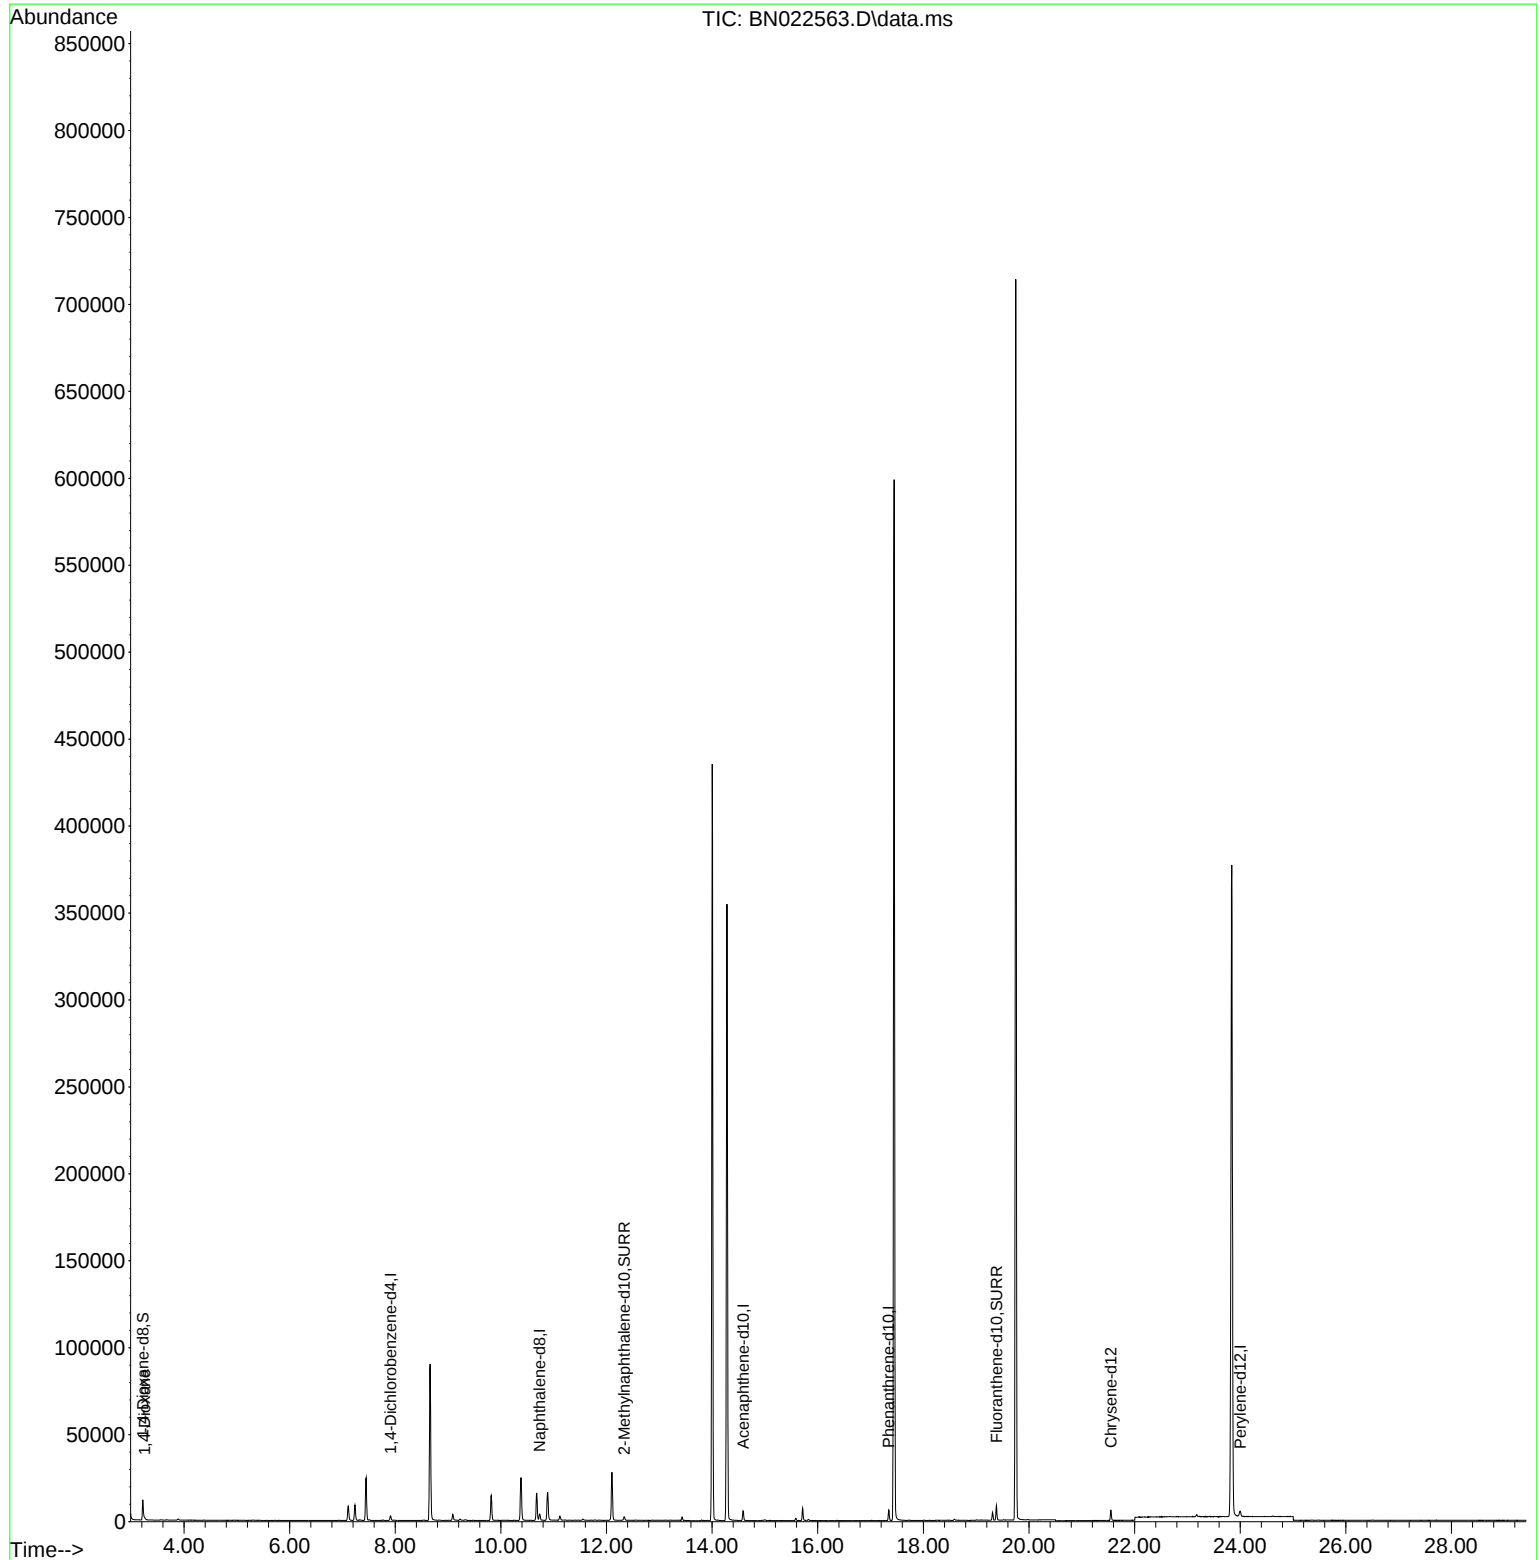

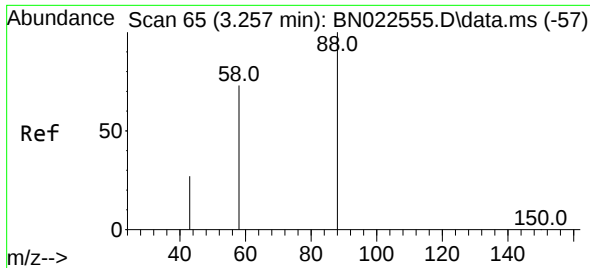

#2
 1,4-Dioxane
 Concen: 0.192 ng/ul
 RT: 3.257 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN022563.D
 Acq: 08 Nov 2022 16:38

Instrument :
 BNA_N
 ClientSampleId :
 EW4Z1

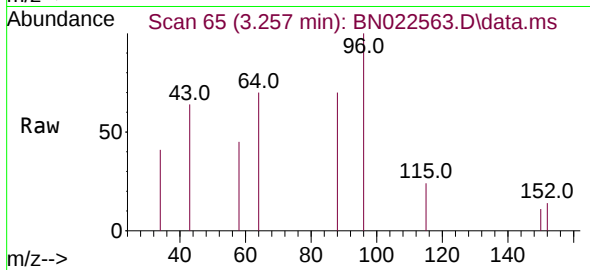

Tgt Ion:	88	Resp:	349
Ion	Ratio	Lower	Upper
88	100		
43	91.4	27.4	41.2#
58	64.2	48.2	72.2

