

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110824\
 Data File : BN034903.D
 Acq On : 08 Nov 2024 11:48
 Operator : RC/JU
 Sample : P4368-09
 Misc : MDL-MDL-WATER-0.2 ng
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-03-QT4-2024

Quant Time: Nov 08 12:29:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 15:02:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	4970	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	14679	0.400	ng	0.00
13) Acenaphthene-d10	14.201	164	6913	0.400	ng	-0.01
19) Phenanthrene-d10	16.957	188	13893	0.400	ng	0.00
29) Chrysene-d12	21.142	240	8589	0.400	ng	# 0.00
35) Perylene-d12	23.317	264	7536	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.192	112	4224	0.305	ng	0.00
5) Phenol-d6	6.752	99	5752	0.313	ng	0.00
8) Nitrobenzene-d5	8.707	82	4031	0.352	ng	0.00
11) 2-Methylnaphthalene-d10	11.935	152	11164	0.558	ng	0.00
14) 2,4,6-Tribromophenol	15.704	330	543	0.307	ng	0.00
15) 2-Fluorobiphenyl	12.832	172	10256	0.351	ng	0.00
27) Fluoranthene-d10	18.987	212	18758	0.599	ng	0.00
31) Terphenyl-d14	19.600	244	5958	0.370	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.184	88	1465	0.233	ng	98
3) n-Nitrosodimethylamine	3.487	42	1862	0.220	ng	95
6) bis(2-Chloroethyl)ether	7.012	93	3502	0.221	ng	100
9) Naphthalene	10.383	128	8883	0.218	ng	99
10) Hexachlorobutadiene	10.682	225	1365	0.210	ng	# 99
12) 2-Methylnaphthalene	12.010	142	5340	0.214	ng	99
16) Acenaphthylene	13.923	152	7032	0.211	ng	100
17) Acenaphthene	14.265	154	4658	0.202	ng	99
18) Fluorene	15.259	166	5879	0.205	ng	99
20) 4,6-Dinitro-2-methylph...	15.345	198	187	0.173	ng	# 74
21) 4-Bromophenyl-phenylether	16.163	248	1503	0.203	ng	99
22) Hexachlorobenzene	16.262	284	1927	0.216	ng	98
23) Atrazine	16.436	200	1035	0.193	ng	96
24) Pentachlorophenol	16.610	266	305	0.174	ng	96
25) Phenanthrene	16.994	178	9435	0.221	ng	99
26) Anthracene	17.081	178	8100	0.220	ng	100
28) Fluoranthene	19.020	202	9501	0.212	ng	99
30) Pyrene	19.382	202	9310	0.214	ng	100
32) Benzo(a)anthracene	21.133	228	7262	0.217	ng	99
33) Chrysene	21.178	228	8087	0.228	ng	98
34) Bis(2-ethylhexyl)phtha...	21.089	149	3582	0.186	ng	100
36) Indeno(1,2,3-cd)pyrene	25.472	276	6940	0.207	ng	98
37) Benzo(b)fluoranthene	22.671	252	7248	0.219	ng	94
38) Benzo(k)fluoranthene	22.671	252	7248	0.210	ng	96
39) Benzo(a)pyrene	23.221	252	5353	0.204	ng	# 87
40) Dibenzo(a,h)anthracene	25.490	278	5285	0.203	ng	96
41) Benzo(g,h,i)perylene	26.124	276	5642	0.205	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110824\
Data File : BN034903.D
Acq On : 08 Nov 2024 11:48
Operator : RC/JU
Sample : P4368-09
Misc : MDL-MDL-WATER-0.2 ng
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Quant Time: Nov 08 12:29:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 15:02:36 2024
Response via : Initial Calibration

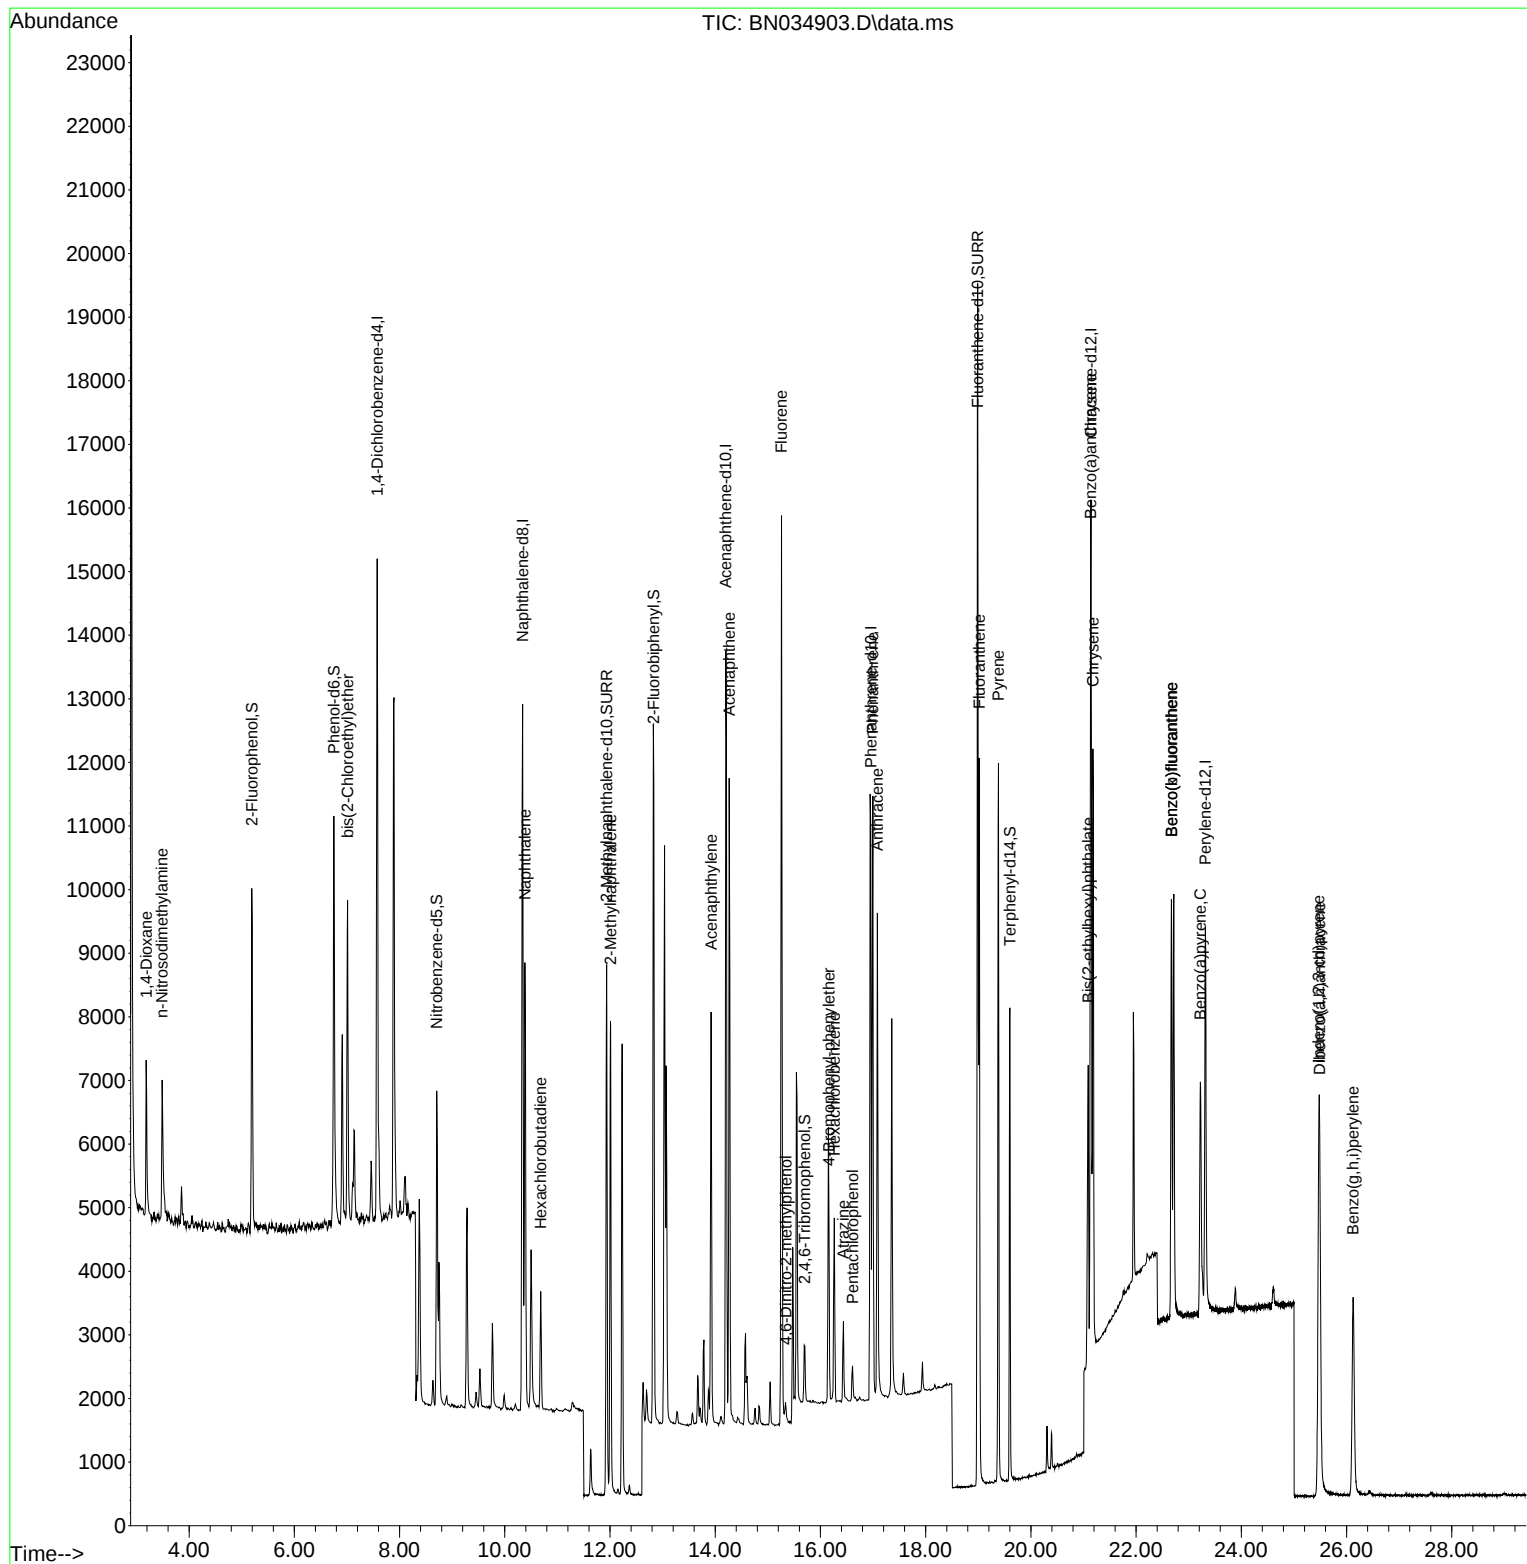






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.575 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN034903.D
 Acq: 08 Nov 2024 11:48

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-03-QT4-2024



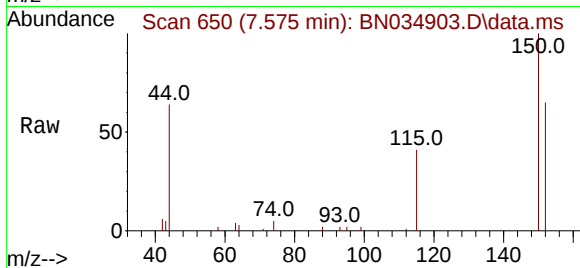



Tgt Ion:152 Resp: 4970
 Ion Ratio Lower Upper
 152 100
 150 154.9 124.4 186.6
 115 62.8 50.5 75.7

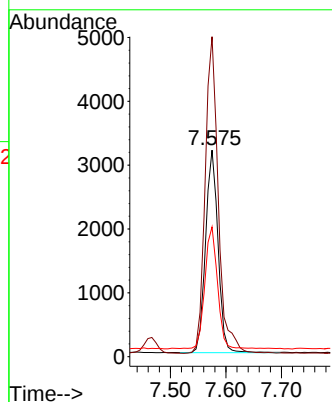

#2
 1,4-Dioxane
 Concen: 0.233 ng
 RT: 3.184 min Scan# 42
 Delta R.T. 0.000 min
 Lab File: BN034903.D
 Acq: 08 Nov 2024 11:48

Tgt Ion: 88 Resp: 1465
 Ion Ratio Lower Upper
 88 100
 43 38.6 28.2 42.2
 58 83.9 67.1 100.7




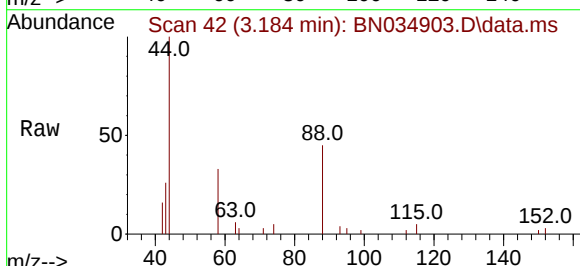


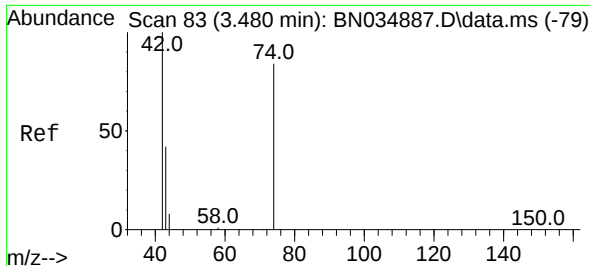

#3
n-Nitrosodimethylamine
Concen: 0.220 ng
RT: 3.487 min Scan# 84
Delta R.T. 0.007 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Tgt Ion: 42 Resp: 1862
Ion Ratio Lower Upper
42 100
74 99.5 83.4 125.2
44 12.5 8.6 12.8

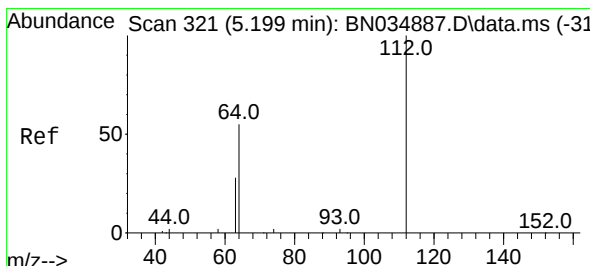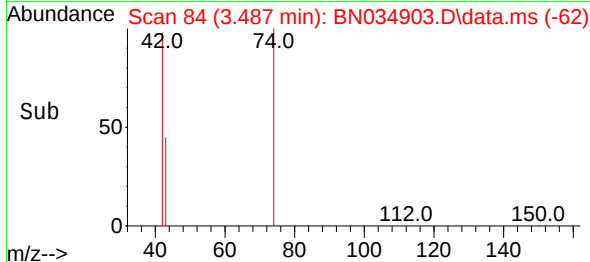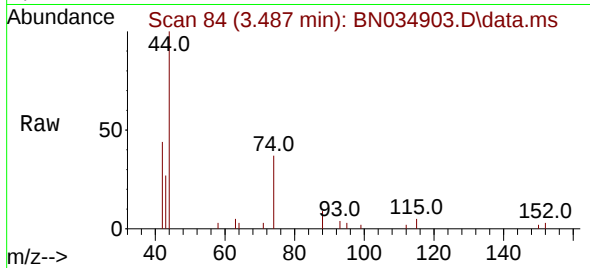

#4
2-Fluorophenol
Concen: 0.305 ng
RT: 5.192 min Scan# 320
Delta R.T. -0.007 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48

Tgt Ion: 112 Resp: 4224
Ion Ratio Lower Upper
112 100
64 62.2 49.6 74.4
63 33.1 26.3 39.5


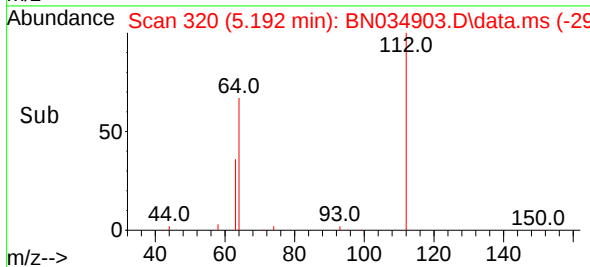

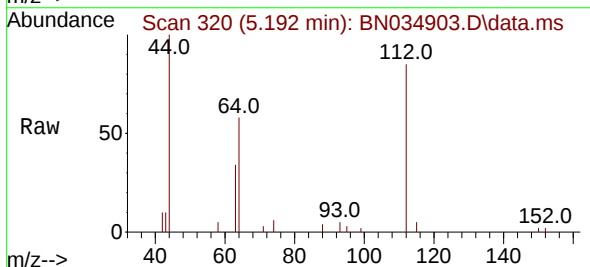




#5
Phenol-d6
Concen: 0.313 ng
RT: 6.752 min Scan# 536
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Tgt Ion: 99 Resp: 5752
Ion Ratio Lower Upper
99 100
42 24.7 20.2 30.2
71 31.3 25.4 38.0

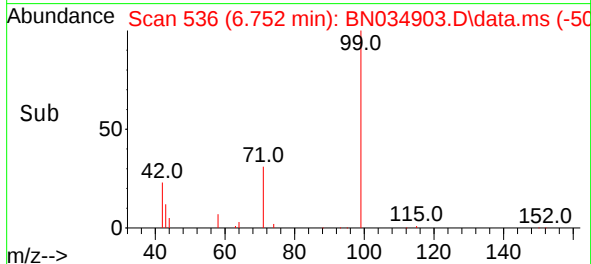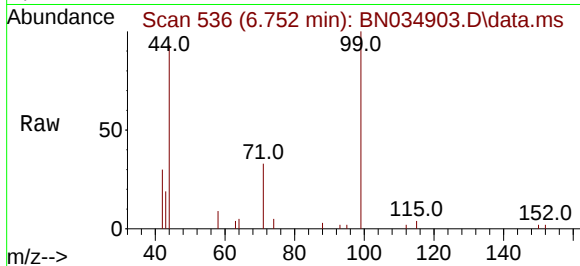

#6
bis(2-Chloroethyl)ether
Concen: 0.221 ng
RT: 7.012 min Scan# 572
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48

Tgt Ion: 93 Resp: 3502
Ion Ratio Lower Upper
93 100
63 84.7 67.5 101.3
95 32.6 25.7 38.5




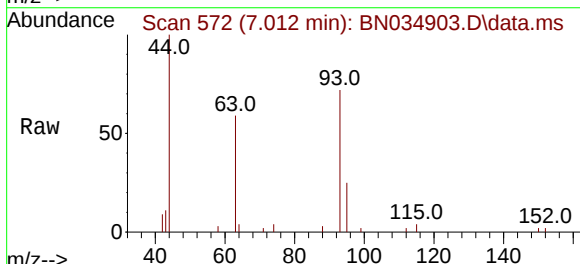




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.340 min Scan# 942
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Tgt Ion:	136	Resp:	14679
Ion	Ratio	Lower	Upper
136	100		
137	11.4	8.9	13.3
54	8.5	6.9	10.3
68	6.2	5.4	8.0

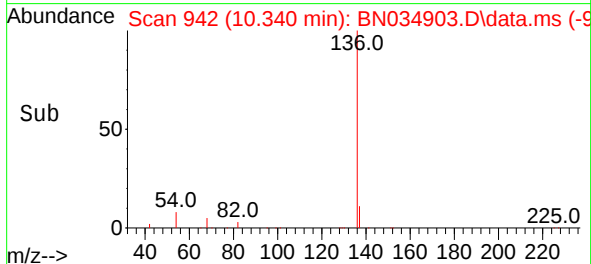

#8
Nitrobenzene-d5
Concen: 0.352 ng
RT: 8.707 min Scan# 789
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48

Tgt Ion:	82	Resp:	4031
Ion	Ratio	Lower	Upper
82	100		
128	36.6	28.1	42.1
54	61.0	49.8	74.6



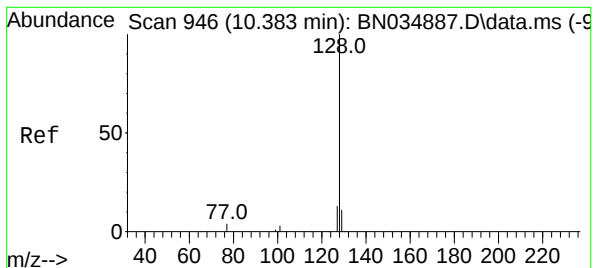

#9

Naphthalene

Concen: 0.218 ng

RT: 10.383 min Scan# 946

Delta R.T. 0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT4-2024





Tgt Ion:128 Resp: 8883

Ion Ratio Lower Upper

128 100

129 11.8 9.0 13.4

127 13.8 10.8 16.2

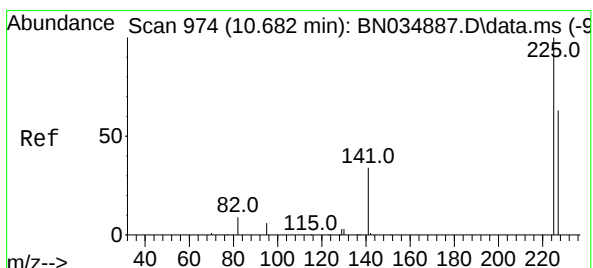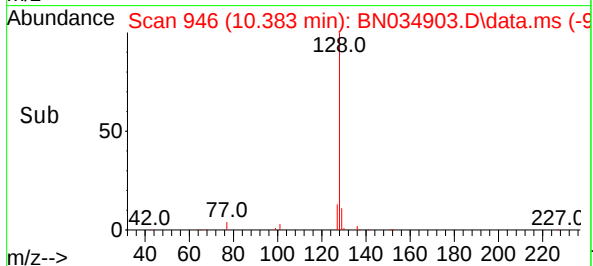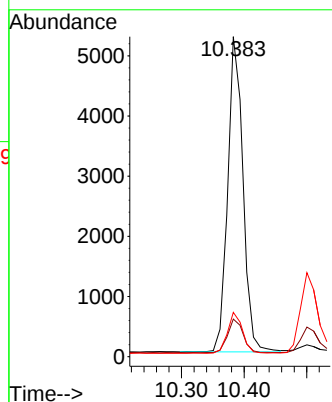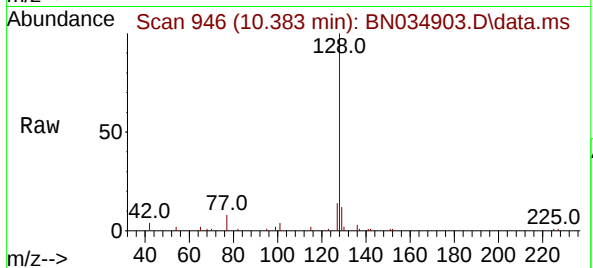

#10

Hexachlorobutadiene

Concen: 0.210 ng

RT: 10.682 min Scan# 974

Delta R.T. 0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:225 Resp: 1365


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 64.0 52.0 78.0

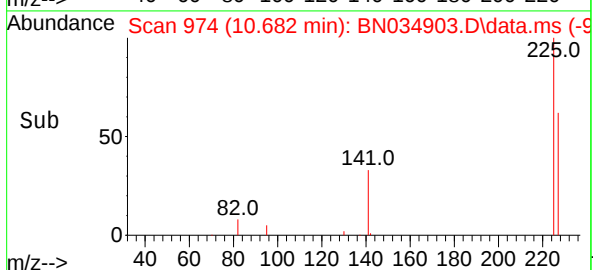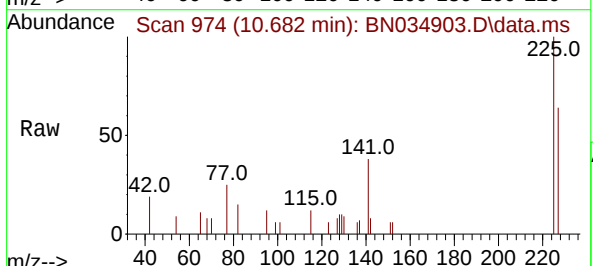

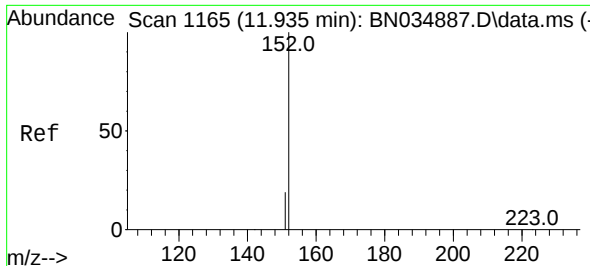

#11

2-Methylnaphthalene-d10

Concen: 0.558 ng

RT: 11.935 min Scan# 1165

Delta R.T. 0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :





MDL-WATER-03-QT4-2024

Tgt Ion:152 Resp: 11164

Ion Ratio Lower Upper

152 100

151 20.4 17.1 25.7

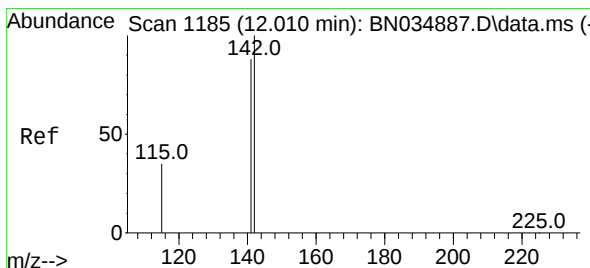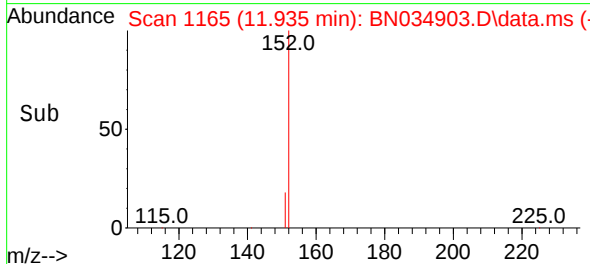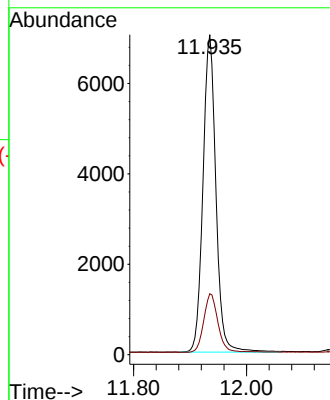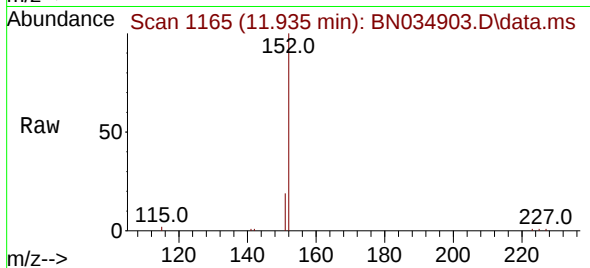

#12

2-Methylnaphthalene

Concen: 0.214 ng

RT: 12.010 min Scan# 1185

Delta R.T. 0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:142 Resp: 5340


Ion Ratio Lower Upper

142 100

141 87.1 70.5 105.7

115 37.6 29.4 44.2

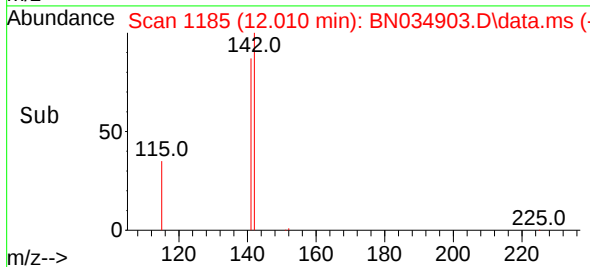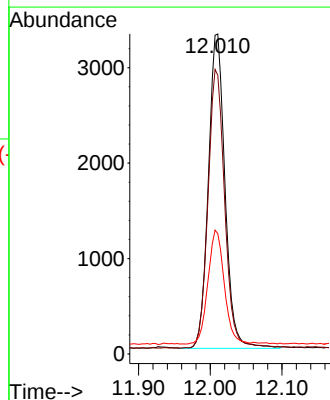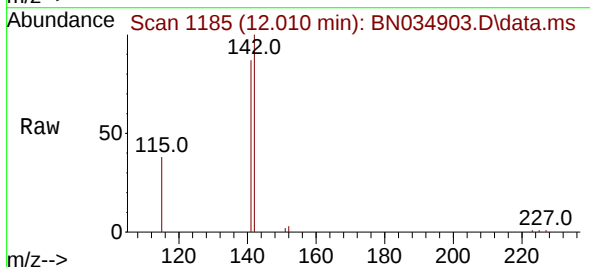



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.201 min Scan# 1492

Delta R.T. -0.010 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT4-2024





Tgt Ion:164 Resp: 6913

Ion Ratio Lower Upper

164 100

162 107.4 81.9 122.9

160 59.5 43.5 65.3

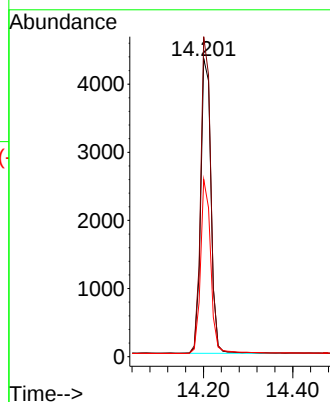

#14

2,4,6-Tribromophenol

Concen: 0.307 ng

RT: 15.704 min Scan# 1630

Delta R.T. -0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:330 Resp: 543


Ion Ratio Lower Upper

330 100

332 92.1 77.1 115.7

141 66.9 54.1 81.1

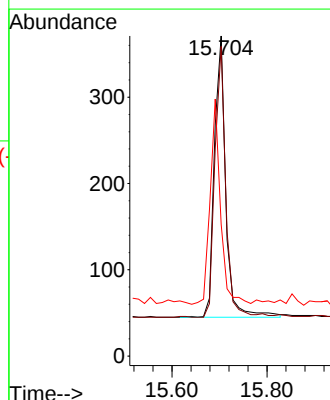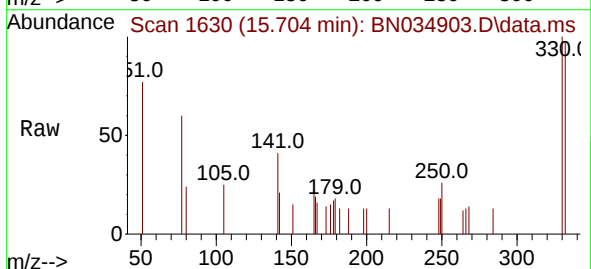



#15

2-Fluorobiphenyl

Concen: 0.351 ng

RT: 12.832 min Scan# 1364

Delta R.T. 0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT4-2024





Tgt Ion:172 Resp: 10256

Ion Ratio Lower Upper

172 100

171 33.3 27.9 41.9

170 22.9 19.0 28.4

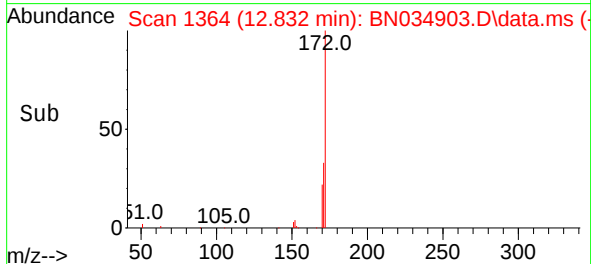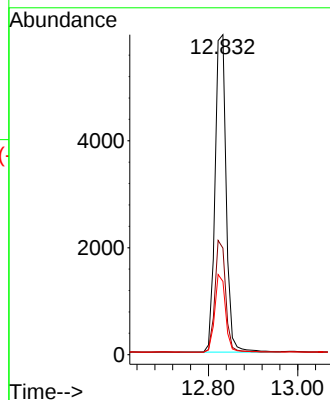

#16

Acenaphthylene

Concen: 0.211 ng

RT: 13.923 min Scan# 1466

Delta R.T. 0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:152 Resp: 7032


Ion Ratio Lower Upper

152 100

151 19.1 15.2 22.8

153 13.2 10.4 15.6



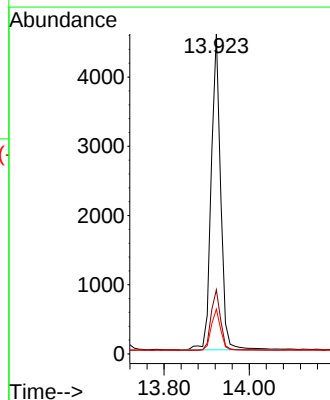





#17
Acenaphthene
Concen: 0.202 ng
RT: 14.265 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Tgt Ion:154 Resp: 4658
Ion Ratio Lower Upper
154 100
153 116.2 92.2 138.2
152 65.8 51.1 76.7

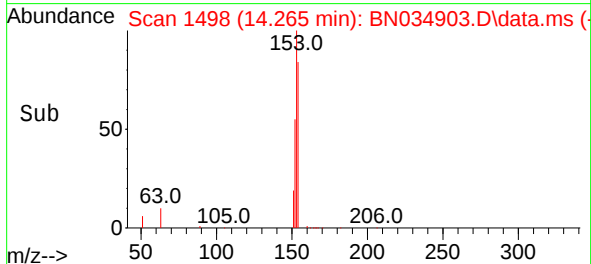

#18
Fluorene
Concen: 0.205 ng
RT: 15.259 min Scan# 1591
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48

Tgt Ion:166 Resp: 5879
Ion Ratio Lower Upper
166 100
165 101.1 79.5 119.3
167 13.3 10.6 16.0





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.957 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT4-2024





Tgt Ion:188 Resp: 13893

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 10.2 8.6 12.8

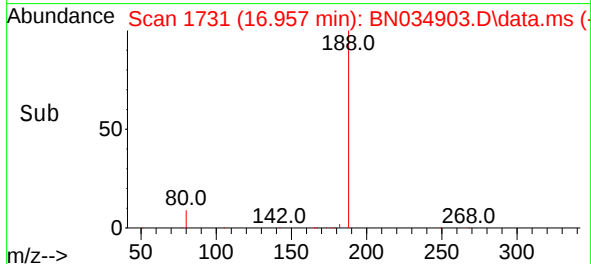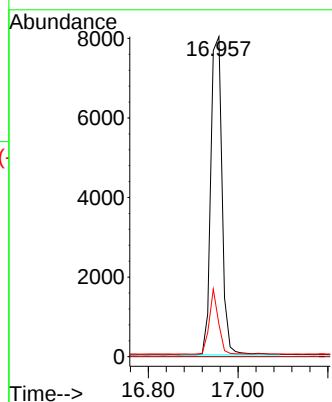

#20

4,6-Dinitro-2-methylphenol

Concen: 0.173 ng

RT: 15.345 min Scan# 1599

Delta R.T. 0.011 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:198 Resp: 187


Ion Ratio Lower Upper

198 100

51 227.2 141.8 212.8#

105 85.7 75.6 113.4







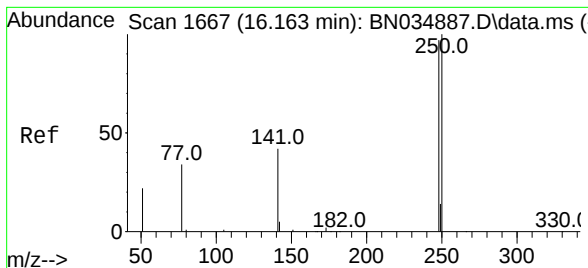

#21
4-Bromophenyl-phenylether
Concen: 0.203 ng
RT: 16.163 min Scan# 1667
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Tgt Ion:	248	Resp:	1503
Ion	Ratio	Lower	Upper
248	100		
250	103.1	82.2	123.4
141	44.2	36.2	54.2

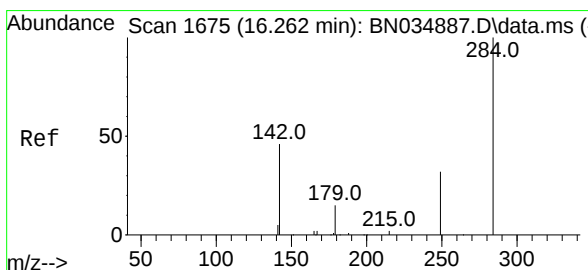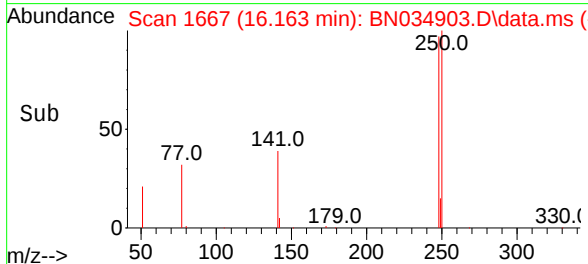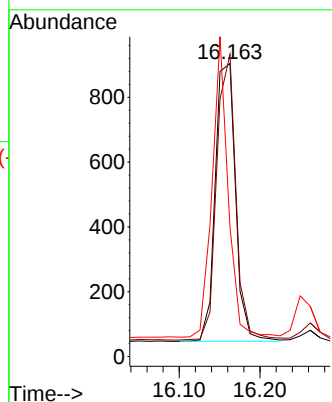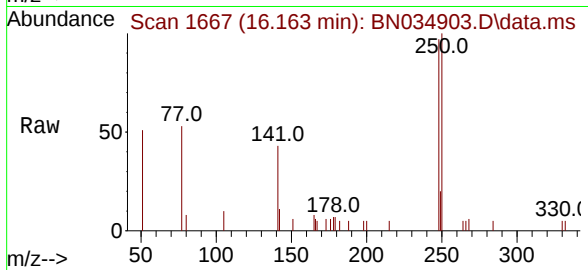

#22
Hexachlorobenzene
Concen: 0.216 ng
RT: 16.262 min Scan# 1675
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48

Tgt Ion:	284	Resp:	1927
Ion	Ratio	Lower	Upper
284	100		
142	52.9	43.4	65.2
249	34.0	25.8	38.6


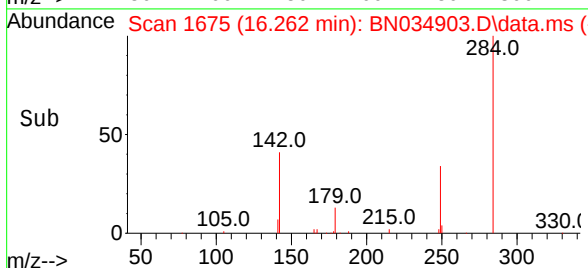

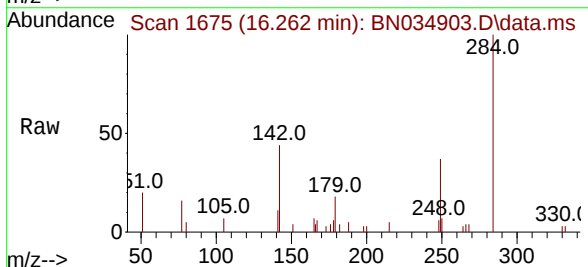




#23
Atrazine
Concen: 0.193 ng
RT: 16.436 min Scan# 1689
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Tgt Ion:200 Resp: 1035
Ion Ratio Lower Upper
200 100
173 32.0 23.4 35.2
215 46.4 35.4 53.0

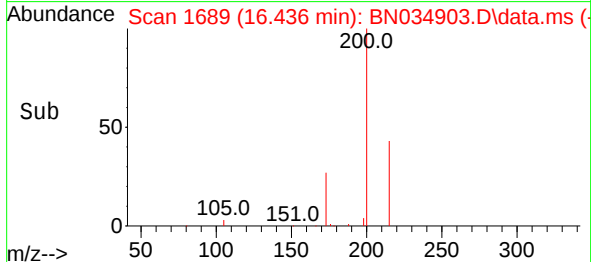

#24
Pentachlorophenol
Concen: 0.174 ng
RT: 16.610 min Scan# 1703
Delta R.T. -0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48

Tgt Ion:266 Resp: 305
Ion Ratio Lower Upper
266 100
264 61.6 51.3 76.9
268 62.6 53.0 79.6




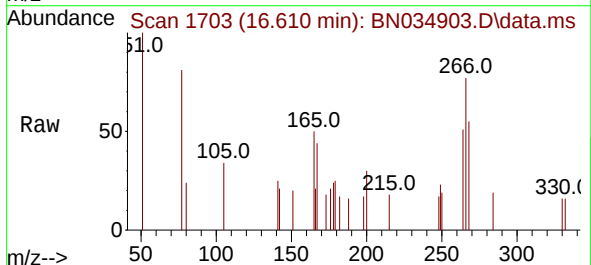


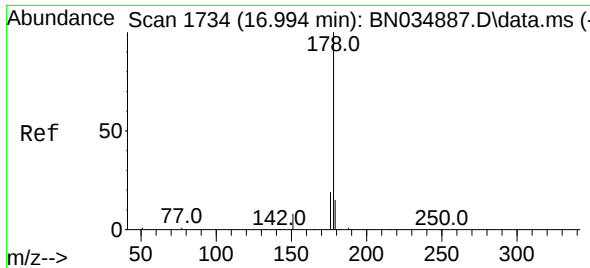

#25
Phenanthrene
Concen: 0.221 ng
RT: 16.994 min Scan# 1734
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Tgt Ion:178 Resp: 9435
Ion Ratio Lower Upper
178 100
176 19.6 15.5 23.3
179 15.9 12.2 18.2

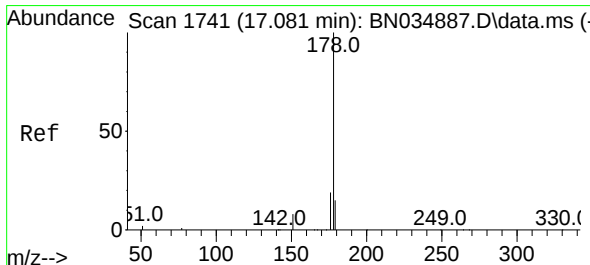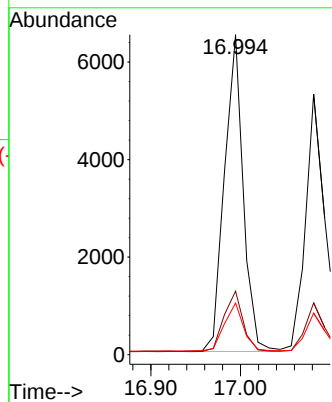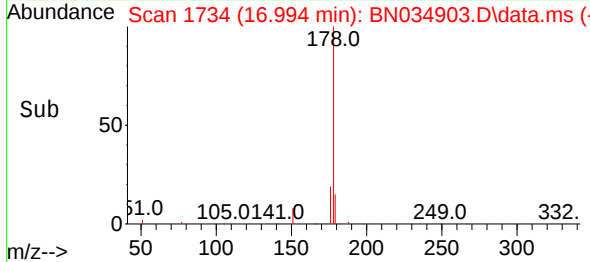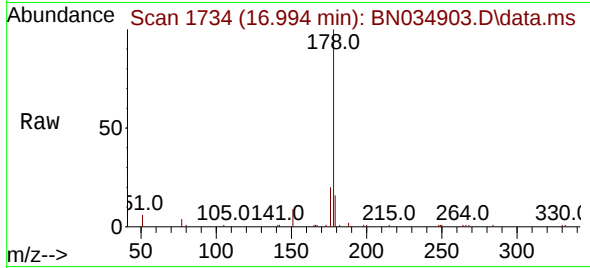

#26
Anthracene
Concen: 0.220 ng
RT: 17.081 min Scan# 1741
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48

Tgt Ion:178 Resp: 8100
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.6
179 14.9 12.1 18.1


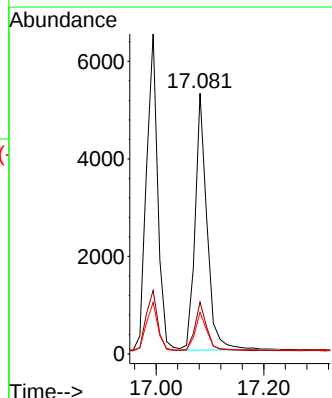
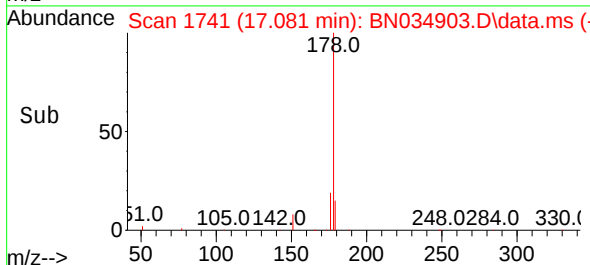
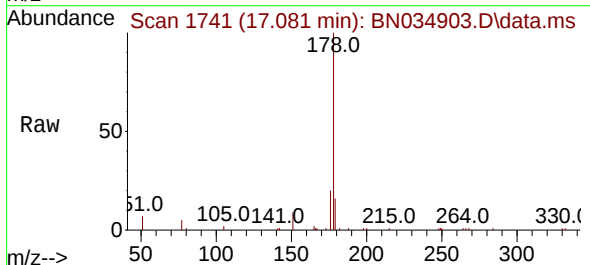


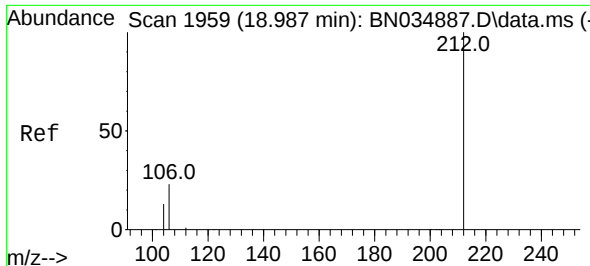

#27
Fluoranthene-d10
Concen: 0.599 ng
RT: 18.987 min Scan# 1959
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT4-2024


Tgt Ion:212 Resp: 18758
Ion Ratio Lower Upper
212 100
106 23.2 18.2 27.4
104 13.6 10.6 15.8

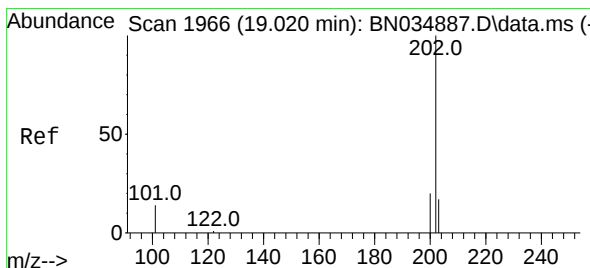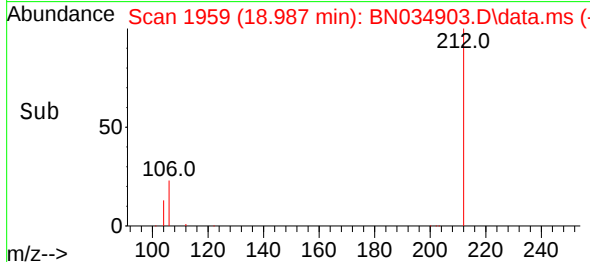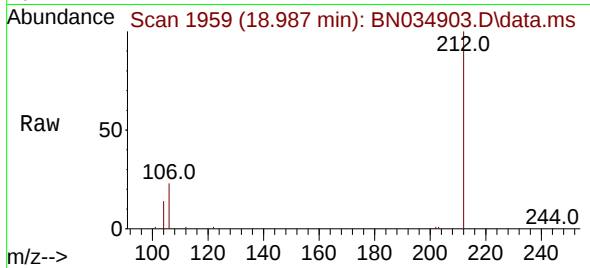

#28
Fluoranthene
Concen: 0.212 ng
RT: 19.020 min Scan# 1966
Delta R.T. 0.000 min
Lab File: BN034903.D
Acq: 08 Nov 2024 11:48

Tgt Ion:202 Resp: 9501
Ion Ratio Lower Upper
202 100
101 16.9 12.7 19.1
203 16.9 13.7 20.5

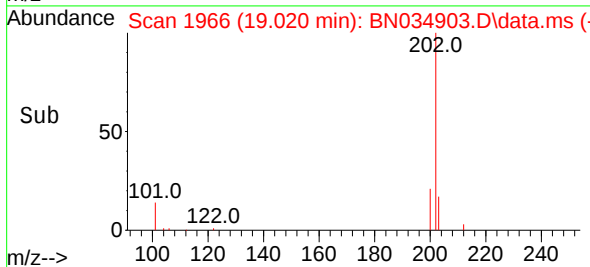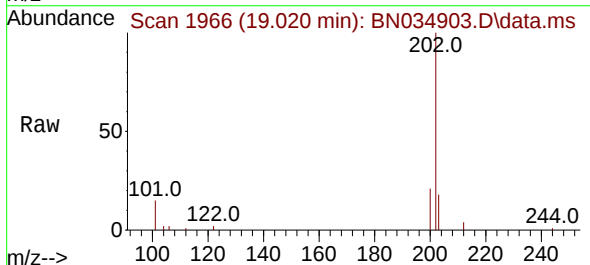



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.142 min Scan# 2409

Delta R.T. -0.009 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT4-2024





Tgt Ion:240 Resp: 8589

Ion Ratio Lower Upper

240 100

120 31.9 13.8 20.8#

236 30.6 23.8 35.6

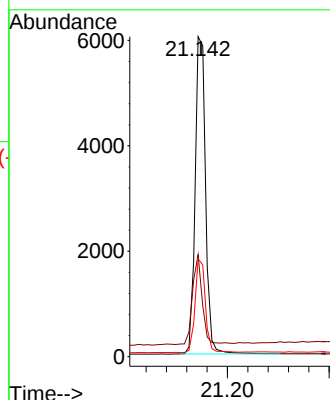

#30

Pyrene

Concen: 0.214 ng

RT: 19.382 min Scan# 2044

Delta R.T. 0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:202 Resp: 9310


Ion Ratio Lower Upper

202 100

200 20.8 16.8 25.2

203 17.6 14.1 21.1



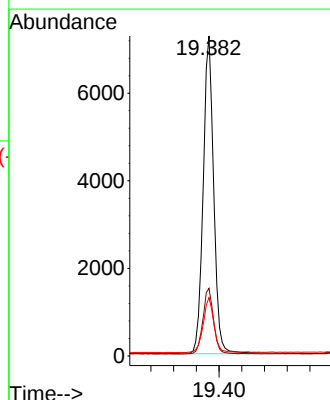





#31
 Terphenyl-d14
 Concen: 0.370 ng
 RT: 19.600 min Scan# 2091
 Delta R.T. 0.000 min
 Lab File: BN034903.D
 Acq: 08 Nov 2024 11:48




Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-03-QT4-2024


Tgt Ion:244 Resp: 5958
 Ion Ratio Lower Upper
 244 100
 212 11.9 9.4 14.0
 122 29.1 23.0 34.4

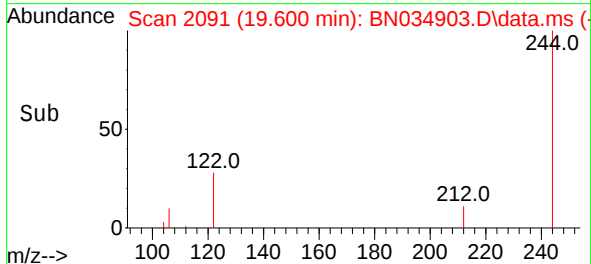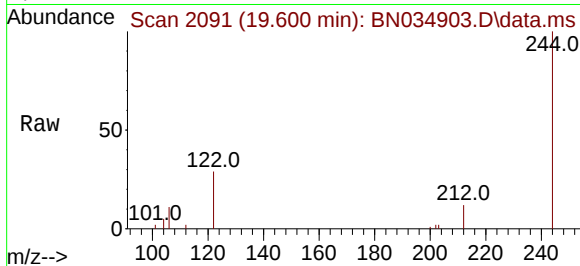

#32
 Benzo(a)anthracene
 Concen: 0.217 ng
 RT: 21.133 min Scan# 2408
 Delta R.T. 0.000 min
 Lab File: BN034903.D
 Acq: 08 Nov 2024 11:48

Tgt Ion:228 Resp: 7262
 Ion Ratio Lower Upper
 228 100
 226 27.1 22.2 33.2
 229 20.2 16.0 24.0

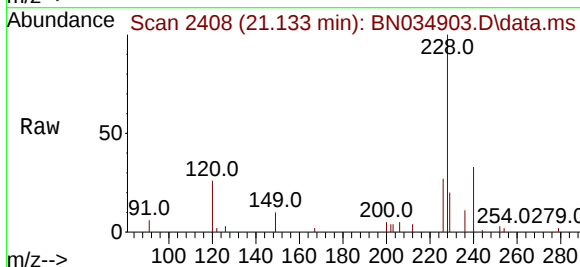

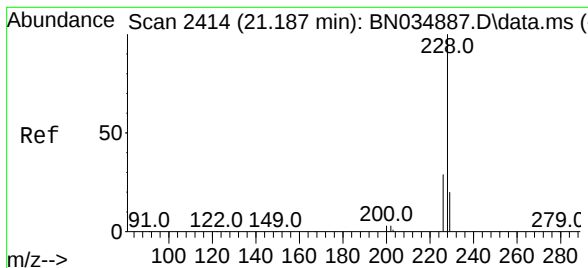

#33

Chrysene

Concen: 0.228 ng

RT: 21.178 min Scan# 2414

Delta R.T. -0.009 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT4-2024





Tgt Ion:228 Resp: 8087

Ion Ratio Lower Upper

228 100

226 31.2 23.7 35.5

229 19.5 16.3 24.5

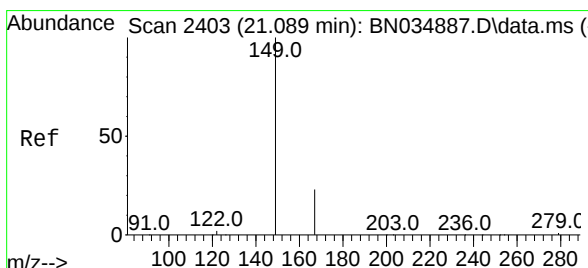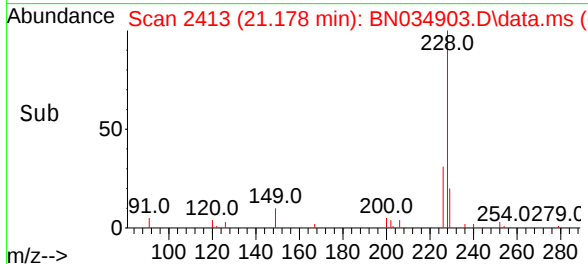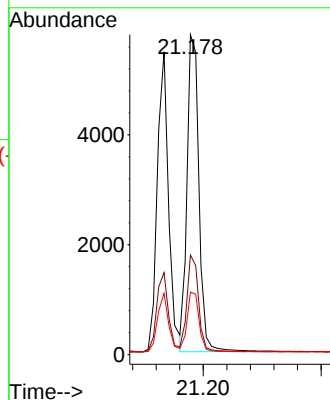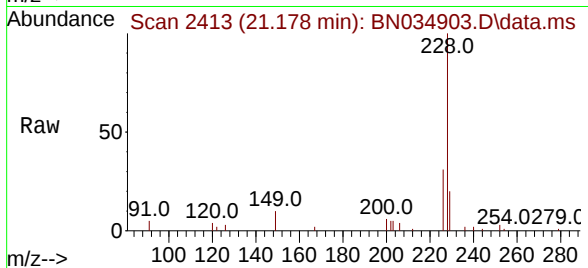

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.186 ng

RT: 21.089 min Scan# 2403

Delta R.T. -0.000 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:149 Resp: 3582


Ion Ratio Lower Upper

149 100

167 22.8 18.1 27.1

279 1.8 1.2 1.8

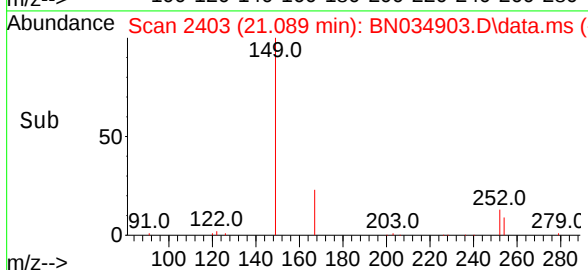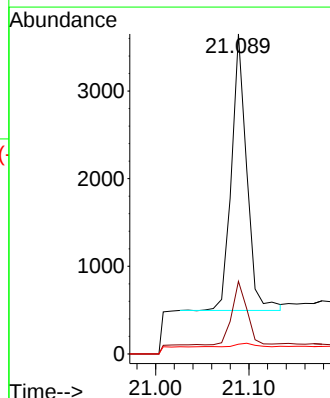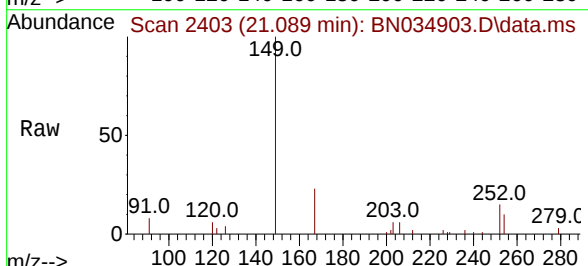




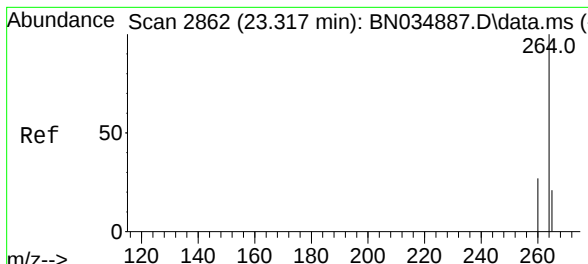


#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.317 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN034903.D
 Acq: 08 Nov 2024 11:48

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-03-QT4-2024

Tgt Ion:264 Resp: 7536




Ion	Ratio	Lower	Upper
264	100		
260	28.2	22.2	33.2
265	66.3	60.9	91.3

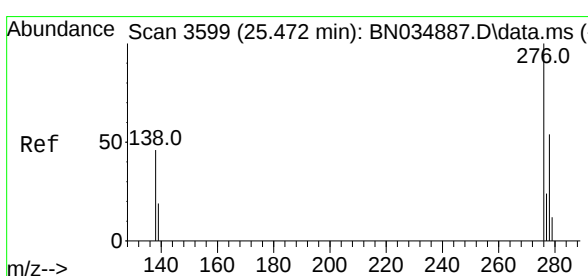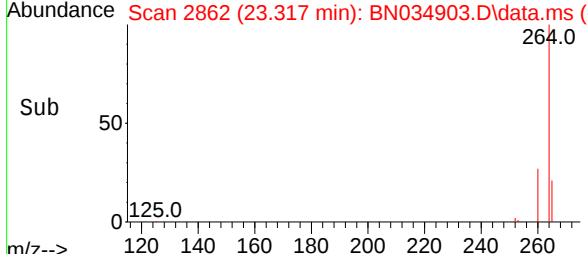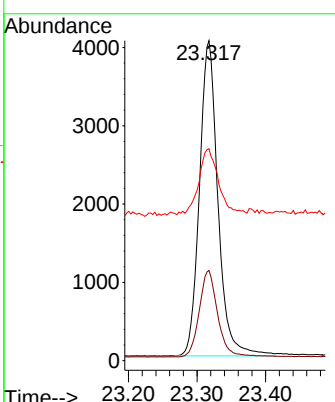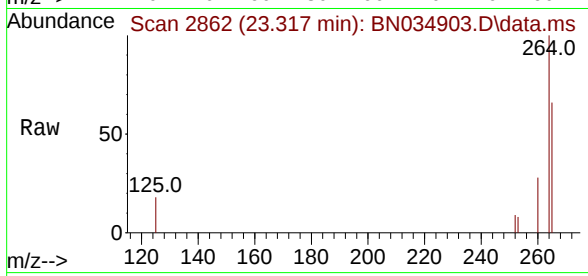


#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.207 ng
 RT: 25.472 min Scan# 3599
 Delta R.T. 0.000 min
 Lab File: BN034903.D
 Acq: 08 Nov 2024 11:48

Tgt Ion:276 Resp: 6940

Ion	Ratio	Lower	Upper
276	100		
138	49.8	38.4	57.6
277	24.3	19.4	29.2

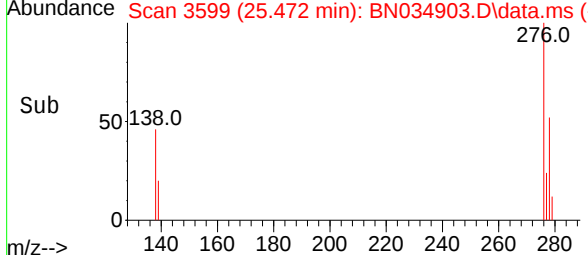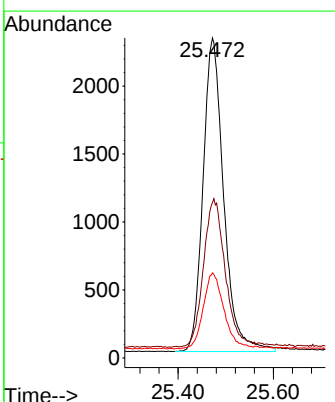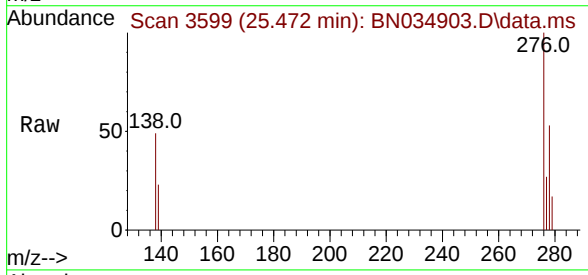



#37

Benzo(b)fluoranthene

Concen: 0.219 ng

RT: 22.671 min Scan# 2641

Delta R.T. 0.003 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT4-2024





Tgt Ion:252 Resp: 7248

Ion Ratio Lower Upper

252 100

253 25.8 19.4 29.2

125 31.1 21.4 32.2



#38

Benzo(k)fluoranthene

Concen: 0.210 ng

RT: 22.671 min Scan# 2641

Delta R.T. -0.041 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:252 Resp: 7248


Ion Ratio Lower Upper

252 100

253 25.8 19.8 29.8

125 31.1 22.6 33.8

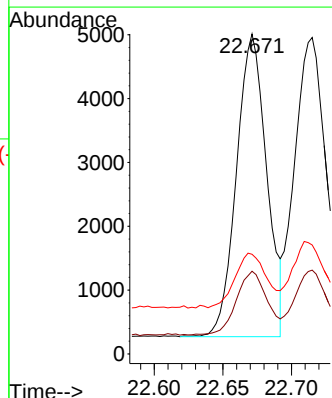



#39

Benzo(a)pyrene

Concen: 0.204 ng

RT: 23.221 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT4-2024





Tgt Ion:252 Resp: 5353

Ion Ratio Lower Upper

252 100

253 30.6 21.4 32.2

125 45.0 27.8 41.6#

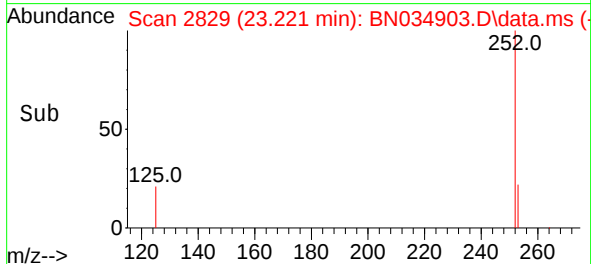

#40

Dibenzo(a,h)anthracene

Concen: 0.203 ng

RT: 25.490 min Scan# 3605

Delta R.T. 0.003 min

Lab File: BN034903.D

Acq: 08 Nov 2024 11:48




Tgt Ion:278 Resp: 5285


Ion Ratio Lower Upper

278 100

139 36.1 27.2 40.8

279 29.2 21.4 32.0



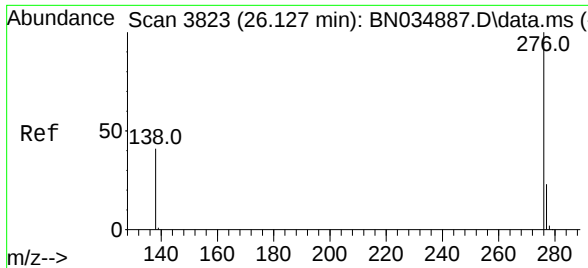

#41
 Benzo(g,h,i)perylene
 Concen: 0.205 ng
 RT: 26.124 min Scan# 3822
 Delta R.T. -0.003 min
 Lab File: BN034903.D
 Acq: 08 Nov 2024 11:48

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-03-QT4-2024

Tgt Ion:	276	Resp:	5642
Ion Ratio	Lower	Upper	
276	100		
277	26.5	20.2	30.2
138	45.2	33.9	50.9

