
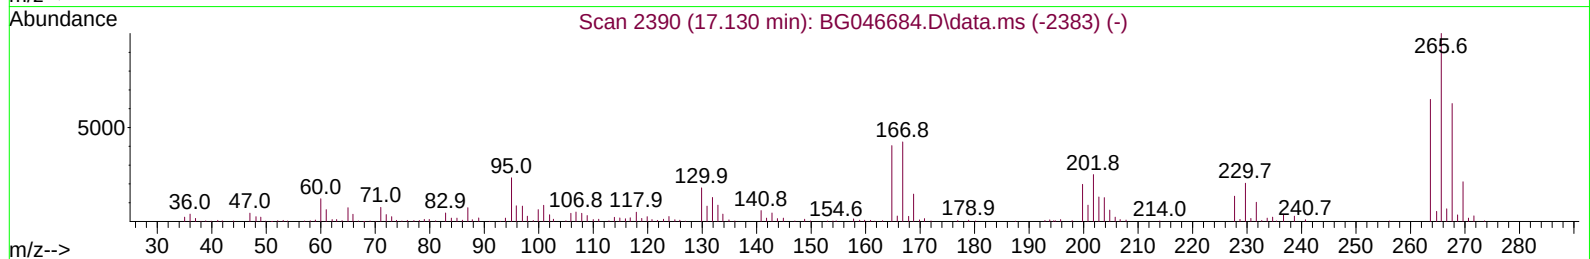
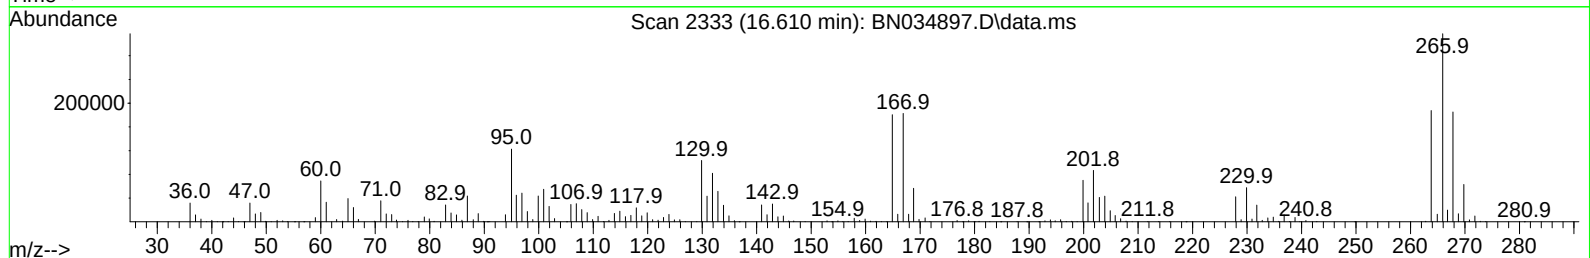


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110824\  
Data File : BN034897.D  
Acq On : 08 Nov 2024 07:50  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 04:05:38 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 09 04:05:27 2024  
Response via : Initial Calibration

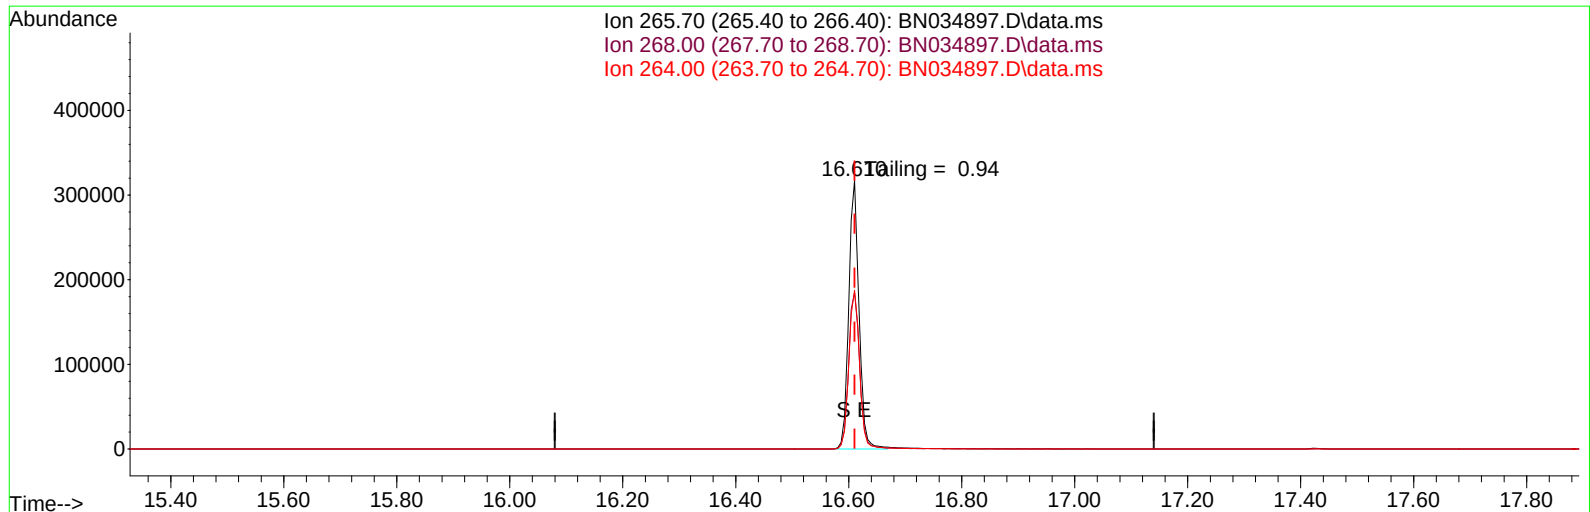

TIC: BN034897.D\data.ms

**(70) Pentachlorophenol (C)**




16.610min ( 0.000) 20617.49 ng

response 407091

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 58.38  |
| 264.00 | 61.60  | 59.14  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110824\  
Data File : BN034897.D  
Acq On : 08 Nov 2024 07:50  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 04:05:38 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 09 04:05:27 2024  
Response via : Initial Calibration

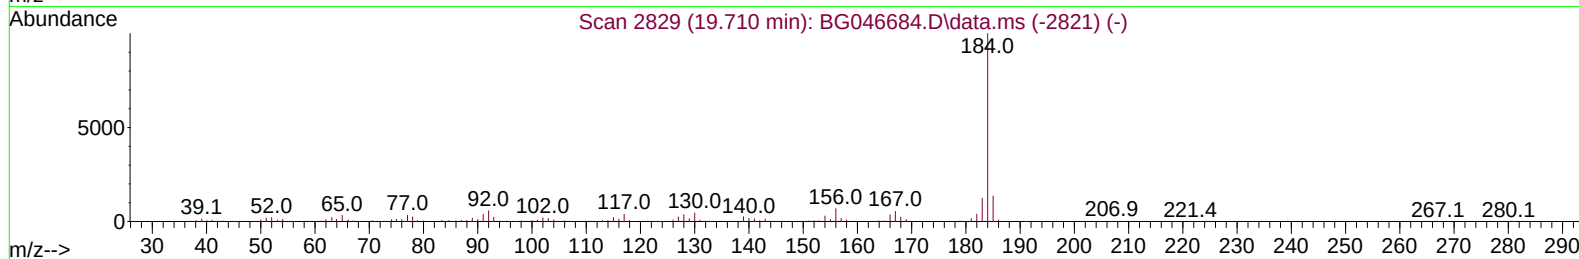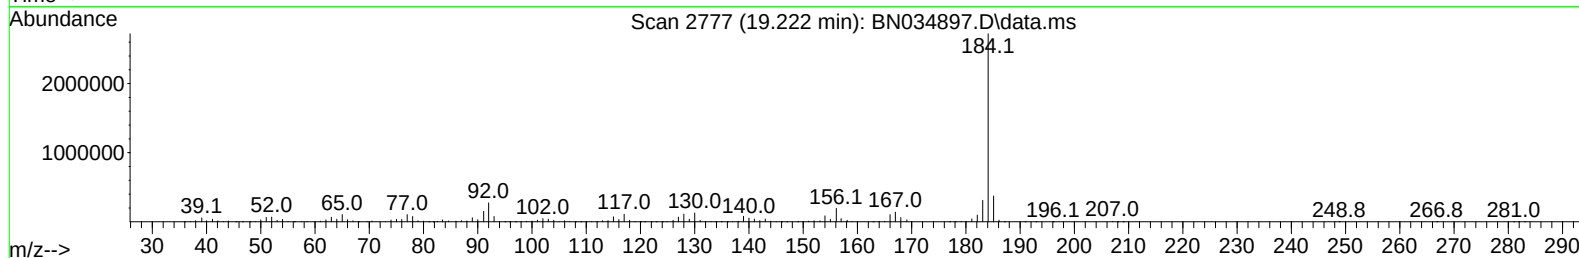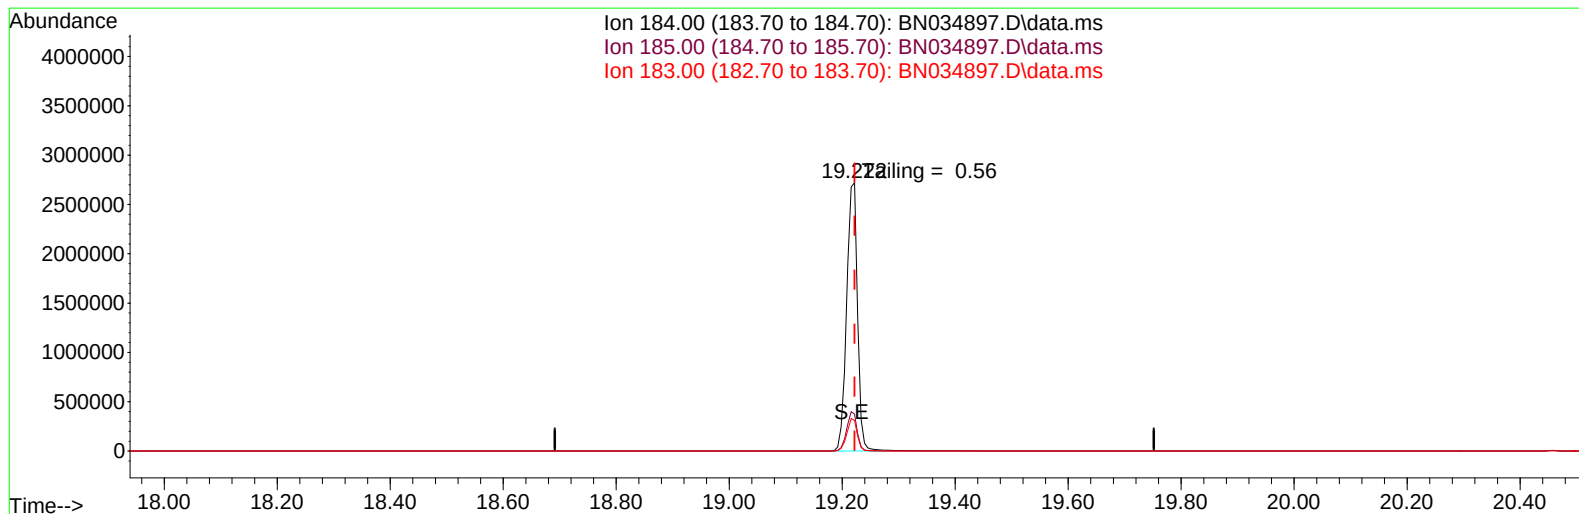

TIC: BN034897.D\data.ms

**(77) Benzidine**

19.222min ( 0.000) 0.00 ng

response 3642384

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.73  |
| 183.00 | 13.20  | 11.43  |
| 0.00   | 0.00   | 0.00   |