
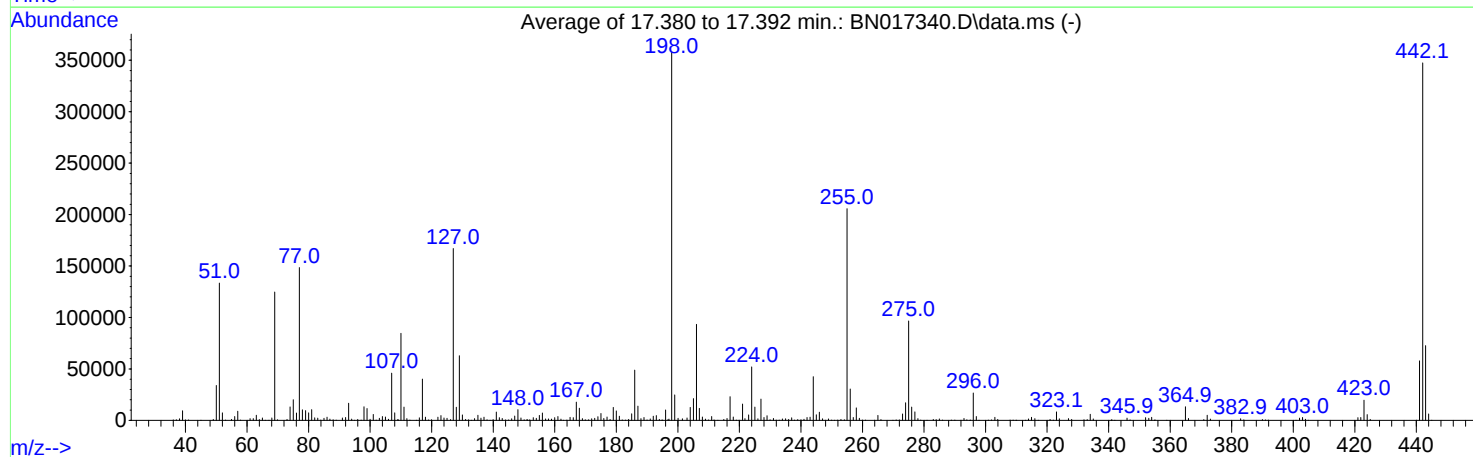


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110921\
 Data File : BN017340.D
 Acq On : 09 Nov 2021 09:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 10 11:00:44 2021

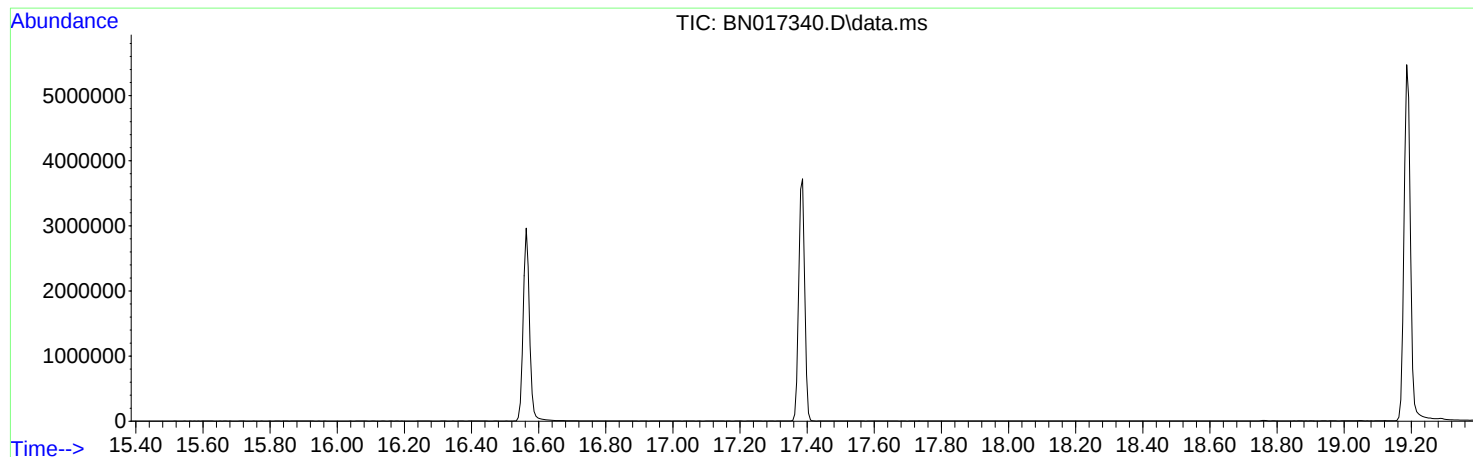




AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	133483	PASS
68	69	0.00	2	1.8	2295	PASS
69	198	0.00	100	34.9	124685	PASS
70	69	0.00	2	0.5	600	PASS
127	198	10	80	46.7	166984	PASS
197	198	0.00	2	0.3	1237	PASS
198	198	100	100	100.0	357525	PASS
199	198	5	9	6.9	24774	PASS
275	198	10	60	27.0	96589	PASS
365	198	1	100	3.7	13179	PASS
441	198	0.01	100	16.2	57779	PASS
442	442	50	100	100.0	347328	PASS
443	442	15	24	20.9	72619	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110921\
Data File : BN017340.D
Acq On : 09 Nov 2021 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 09 14:18:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

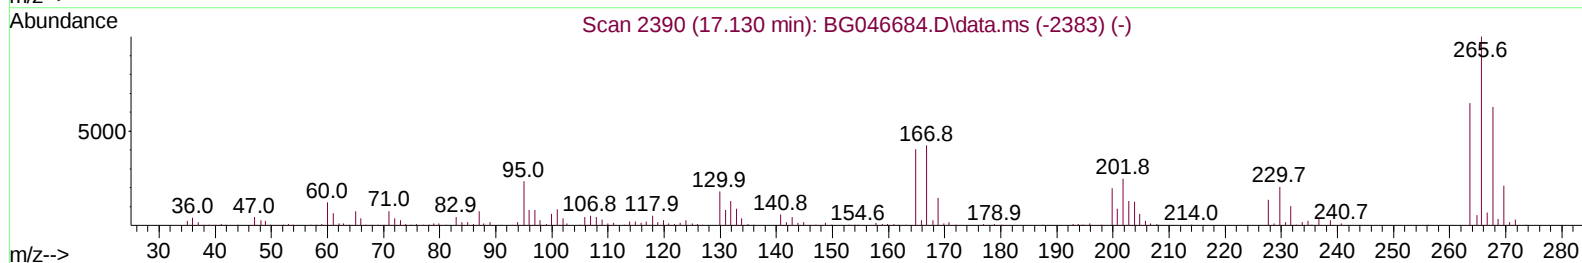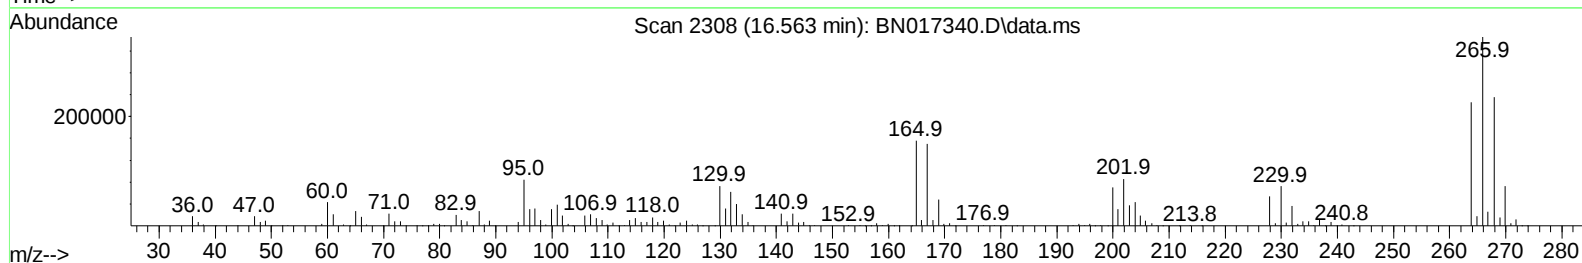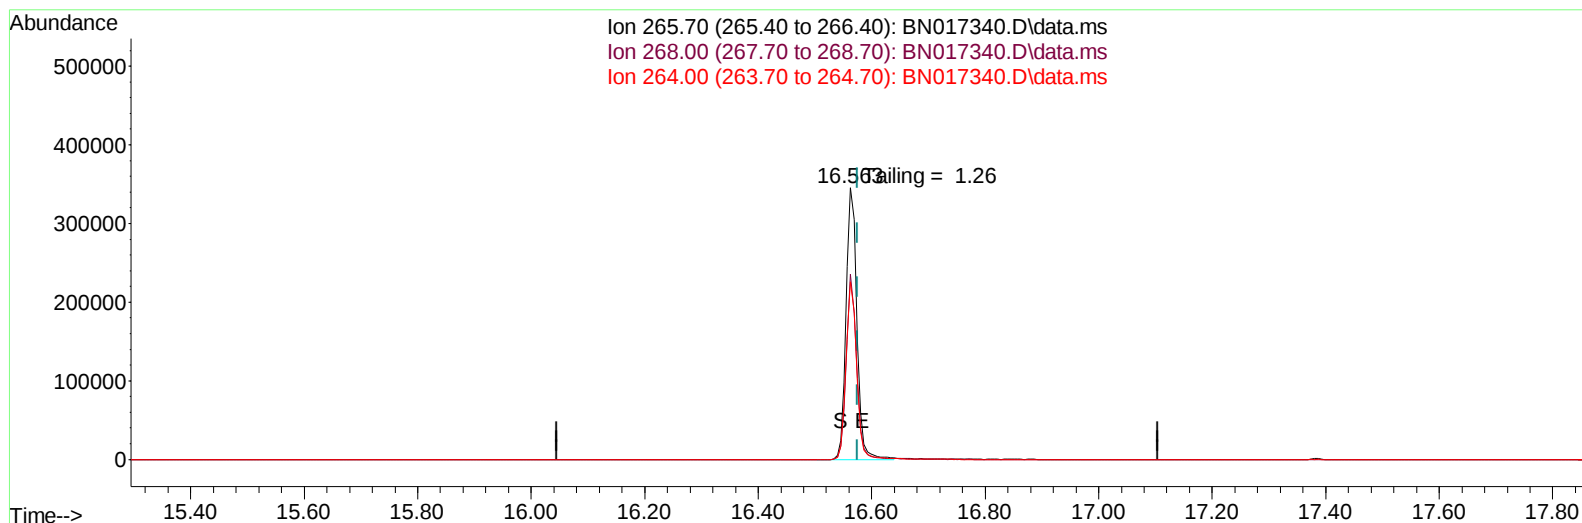

TIC: BN017340.D\data.ms

(70) Pentachlorophenol (C)

16.563min (-0.012) 22840.24 ng




response 457611

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.30
264.00	61.60	65.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110921\
 Data File : BN017340.D
 Acq On : 09 Nov 2021 09:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 09 14:18:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 01 19:02:51 2021
 Response via : Initial Calibration

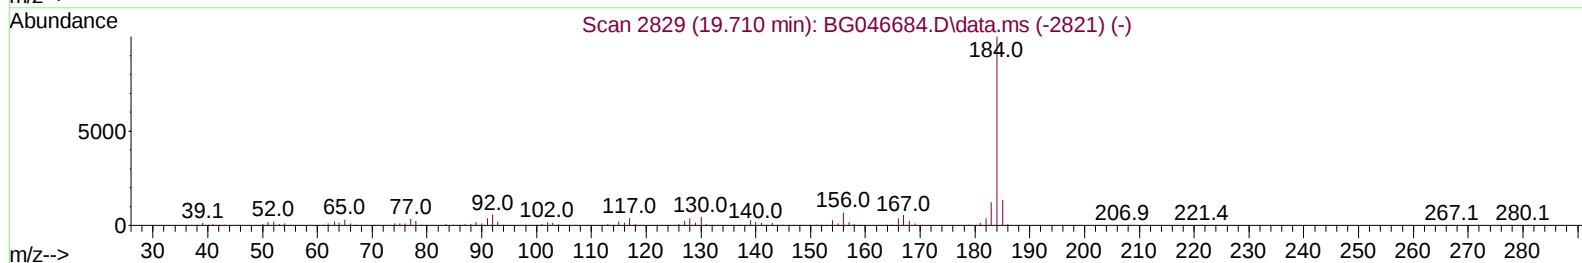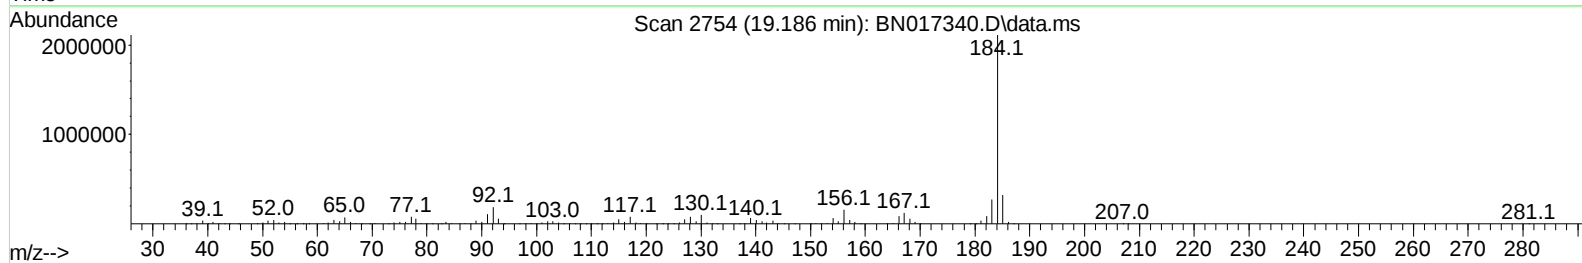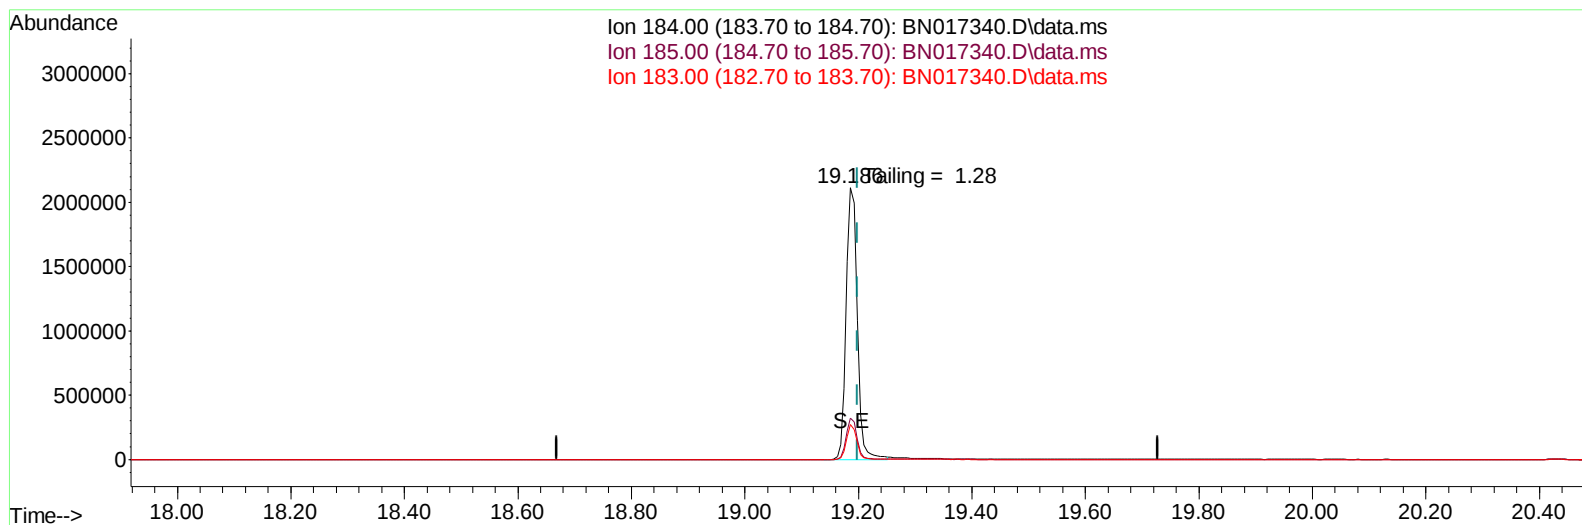

TIC: BN017340.D\data.ms

(77) Benzidine

19.186min (-0.012) 0.00 ng

response 2942688

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.31
183.00	13.20	12.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2021	BNA_N	<u>BN017340.D</u>
Compound Name	Response	Retention Time
DDT	1379814	20.433
DDD	4189	19.986
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4189	1384003	0.30

Instrument :
BNA_N
ClientSampleId :
DFTPP