


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110921\  
 Data File : BN017359.D  
 Acq On : 09 Nov 2021 21:34  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN110921.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Nov 10 11:00:44 2021

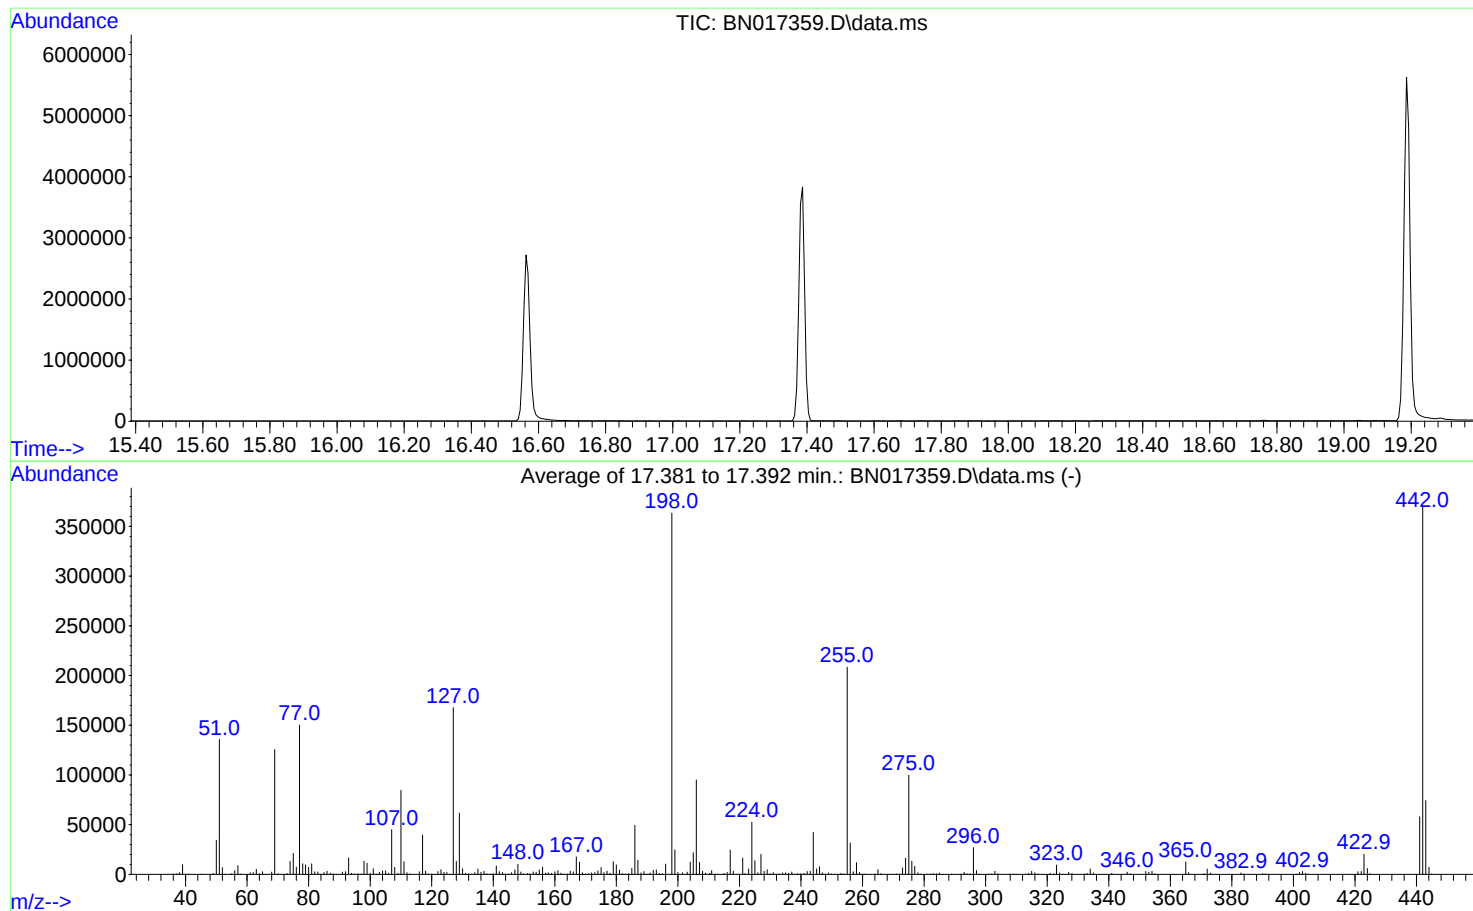




AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 37.3         | 135616     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 2278       | PASS                |
| 69             | 198             | 0.00            | 100             | 34.6         | 125621     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 632        | PASS                |
| 127            | 198             | 10              | 80              | 46.1         | 167669     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 363435     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 24635      | PASS                |
| 275            | 198             | 10              | 60              | 27.5         | 99805      | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 12575      | PASS                |
| 441            | 198             | 0.01            | 100             | 16.0         | 58005      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 370027     | PASS                |
| 443            | 442             | 15              | 24              | 20.0         | 74173      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110921\  
Data File : BN017359.D  
Acq On : 09 Nov 2021 21:34  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Nov 10 17:10:53 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 01 19:02:51 2021  
Response via : Initial Calibration

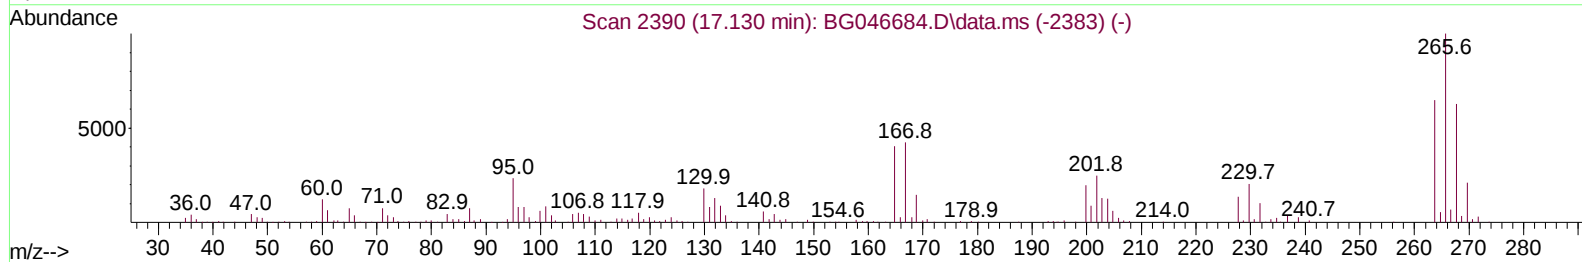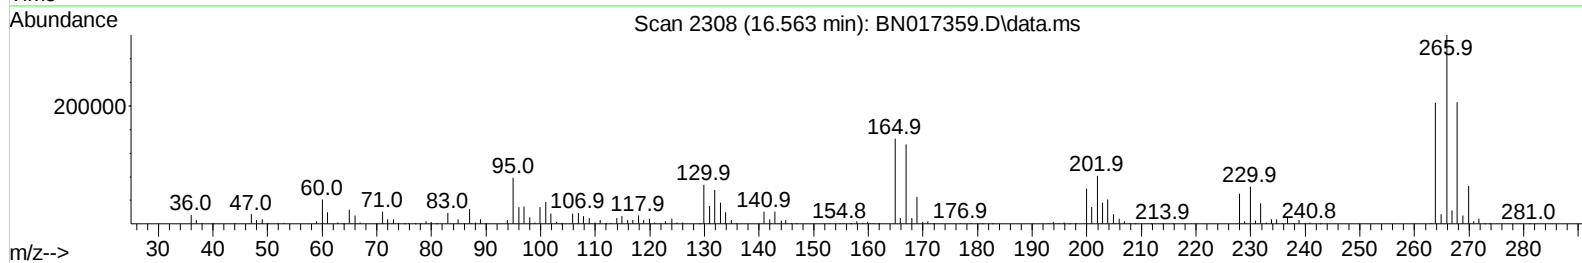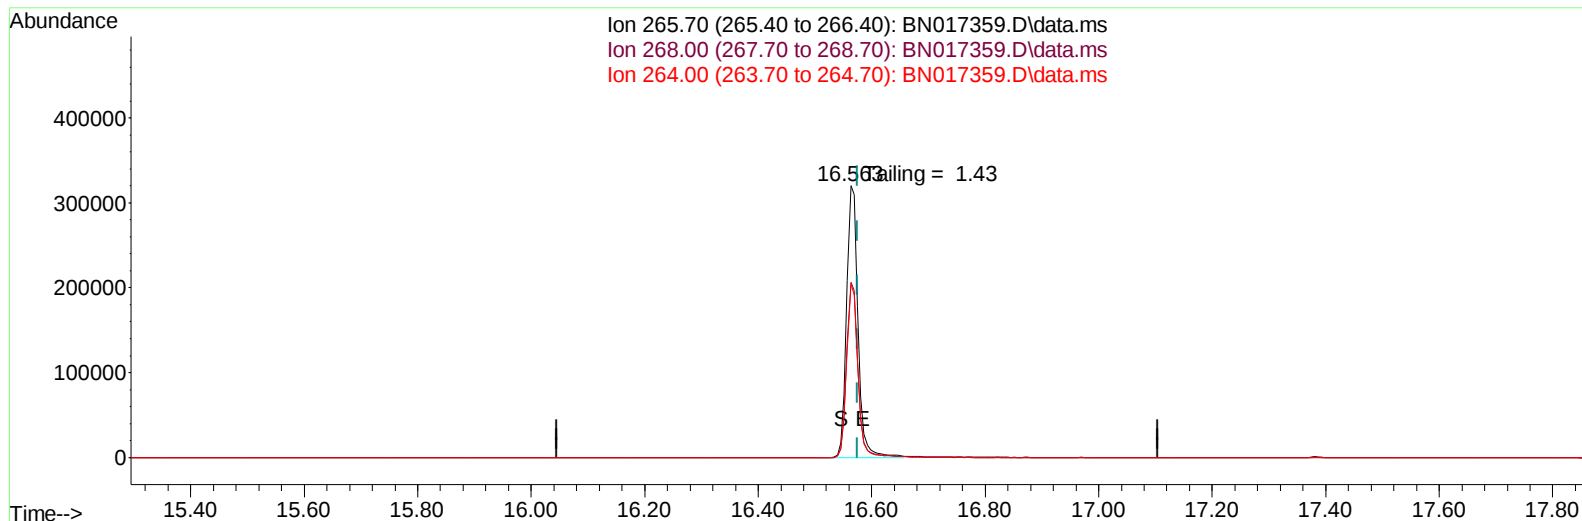

TIC: BN017359.D\data.ms

**(70) Pentachloropheno1 (C)**

**16.563min (-0.012) 25302.55 ng**




**response 449558**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.50  |
| 264.00 | 61.60  | 64.12  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110921\  
 Data File : BN017359.D  
 Acq On : 09 Nov 2021 21:34  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Nov 10 17:10:53 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Nov 01 19:02:51 2021  
 Response via : Initial Calibration

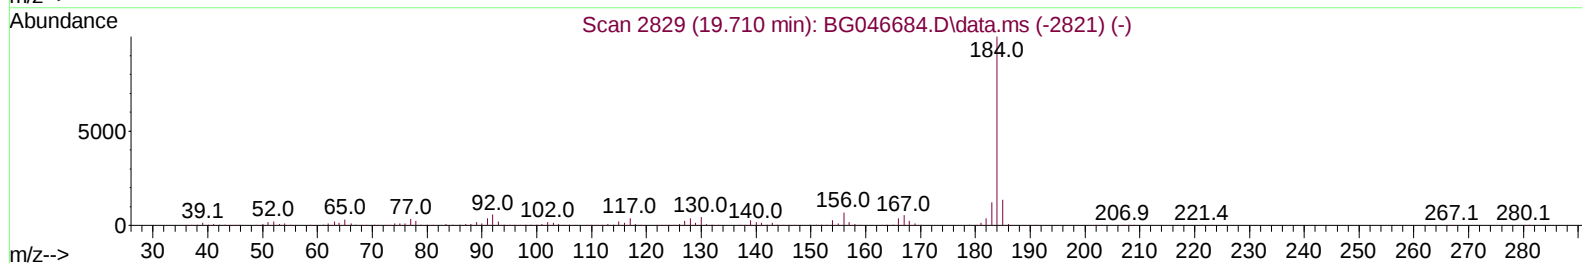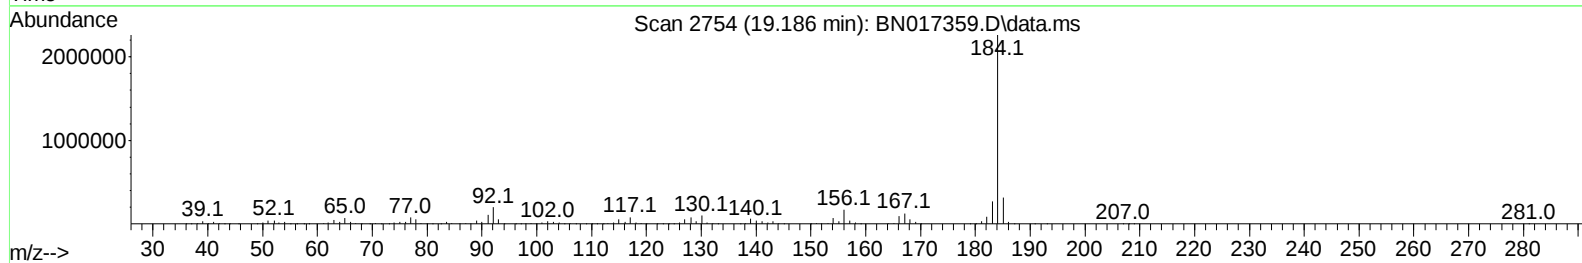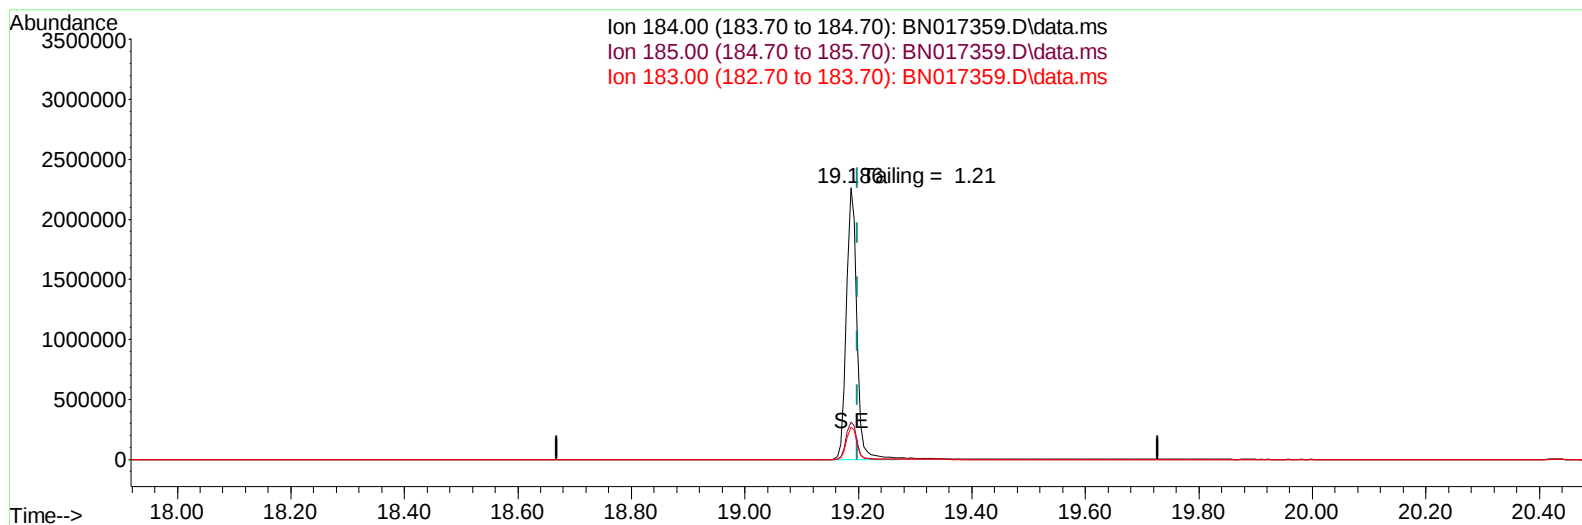

TIC: BN017359.D\data.ms

**(77) Benzidine****19.186min (-0.012) 0.00 ng****response 2931838**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.87  |
| 183.00 | 13.20  | 11.92  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/9/2021     | BNA_N            | <u>BN017359.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1378477          | 20.428             |
| DDD           | 12898            | 19.986             |
| DDE           | 0                | 19.58              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 12898         | 1391375          | 0.93               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP