


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110922\
 Data File : BN022571.D
 Acq On : 09 Nov 2022 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 09 23:46:48 2022

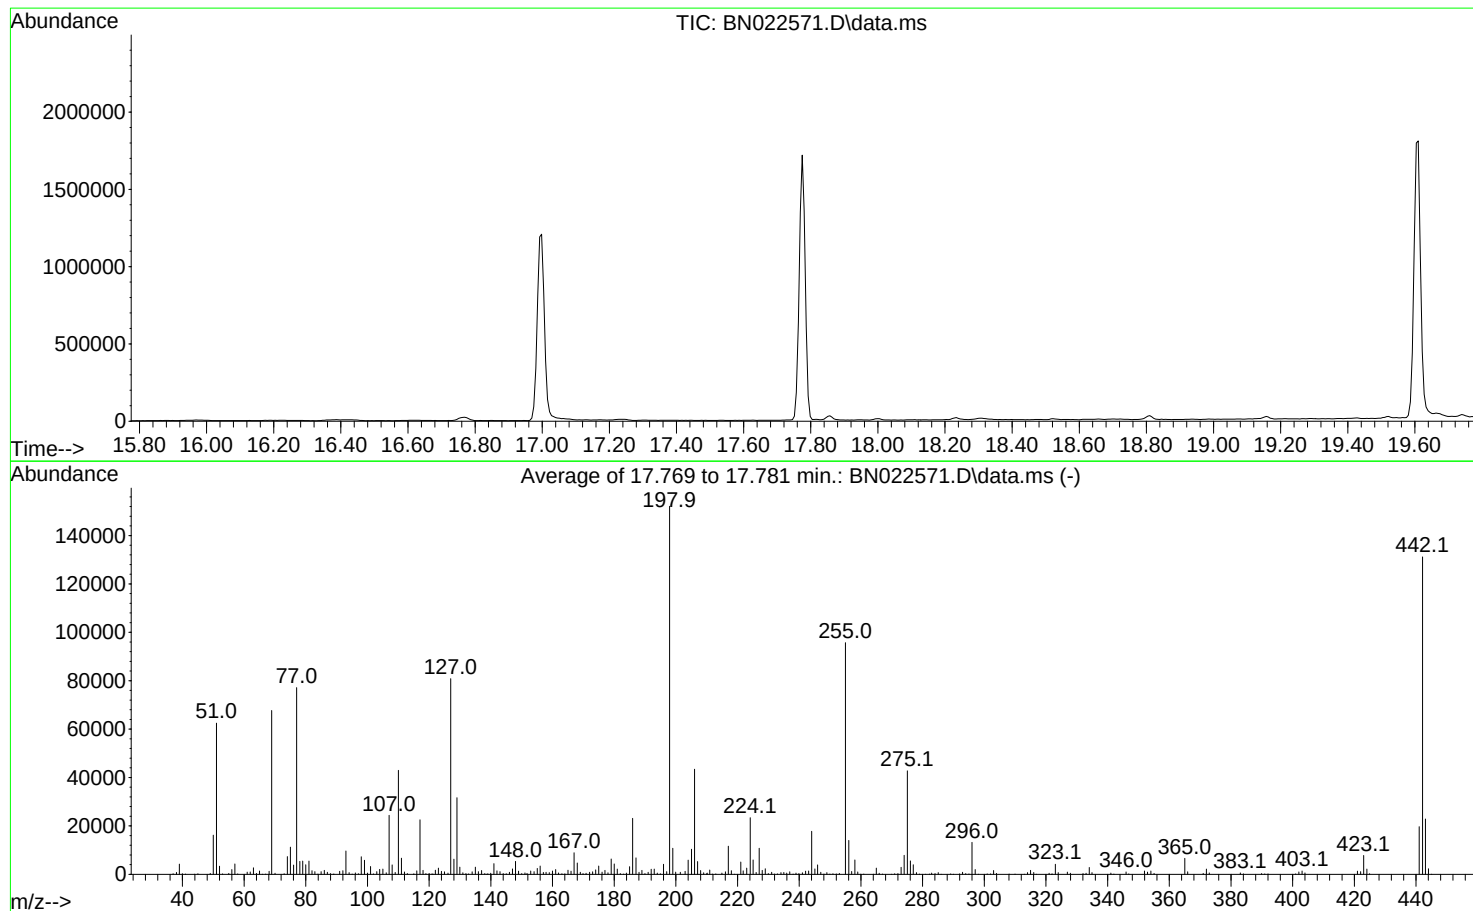




AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	62440	PASS
68	69	0.00	2	1.8	1244	PASS
69	198	0.00	100	44.5	67710	PASS
70	69	0.00	2	0.6	424	PASS
127	198	10	80	53.2	80877	PASS
197	198	0.00	2	0.7	1076	PASS
198	198	100	100	100.0	152043	PASS
199	198	5	9	7.1	10733	PASS
275	198	10	60	28.1	42784	PASS
365	198	1	100	4.3	6606	PASS
441	198	0.01	100	12.9	19689	PASS
442	442	50	100	100.0	131187	PASS
443	442	15	24	17.4	22845	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110922\
Data File : BN022571.D
Acq On : 09 Nov 2022 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 10 07:57:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 07:57:47 2022
Response via : Initial Calibration

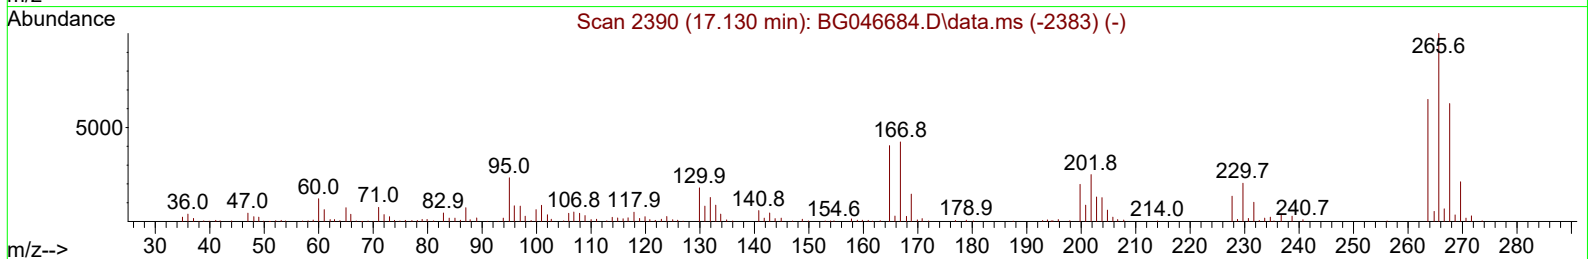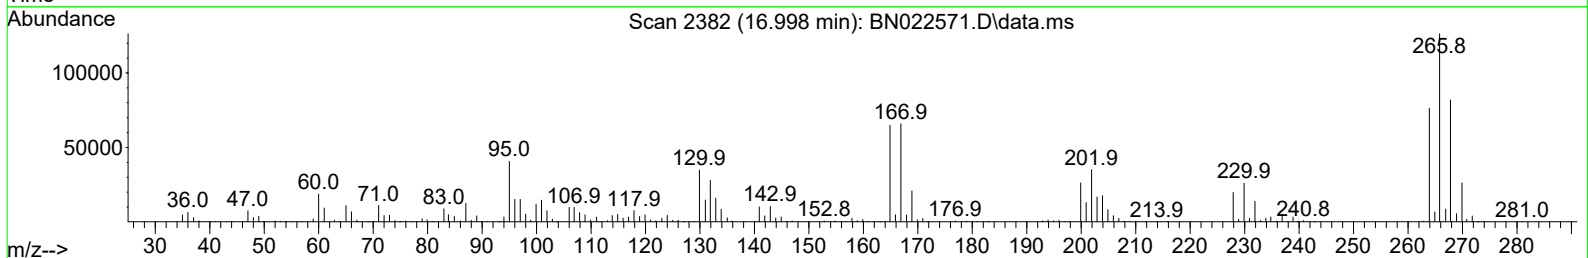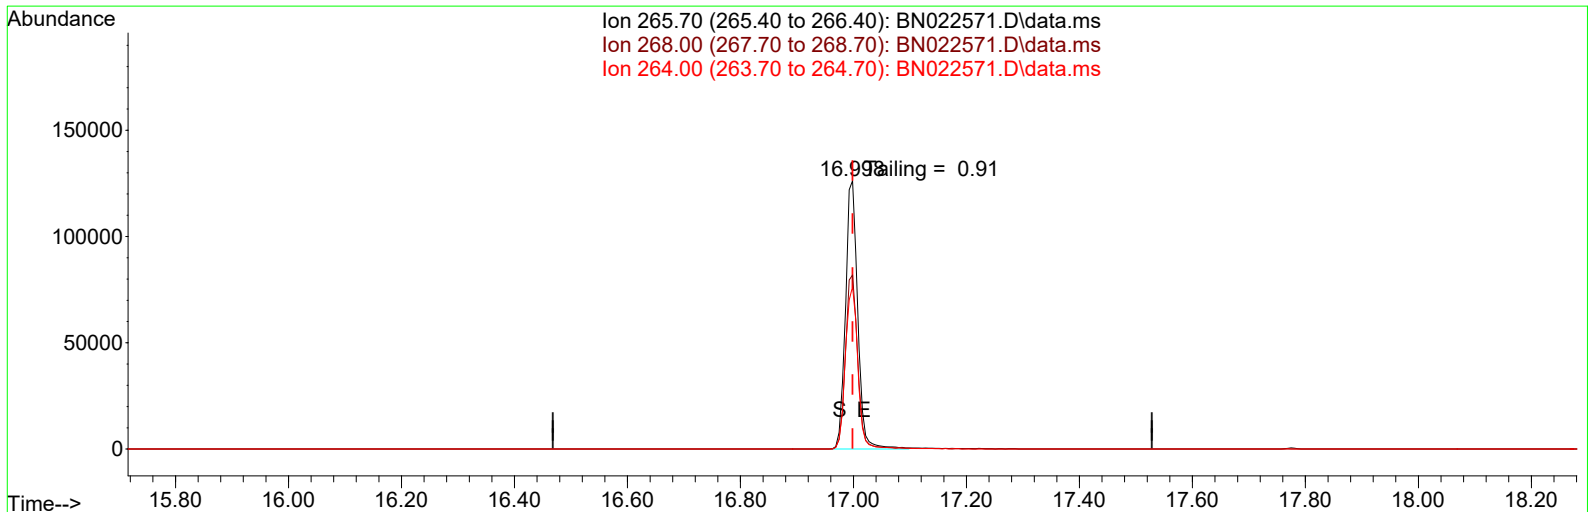

TIC: BN022571.D\data.ms

(70) Pentachlorophenol (C)

16.998min (0.000) 21639.13 ng




response 189857

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.85
264.00	61.60	60.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110922\
 Data File : BN022571.D
 Acq On : 09 Nov 2022 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 10 07:57:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 10 07:57:47 2022
 Response via : Initial Calibration

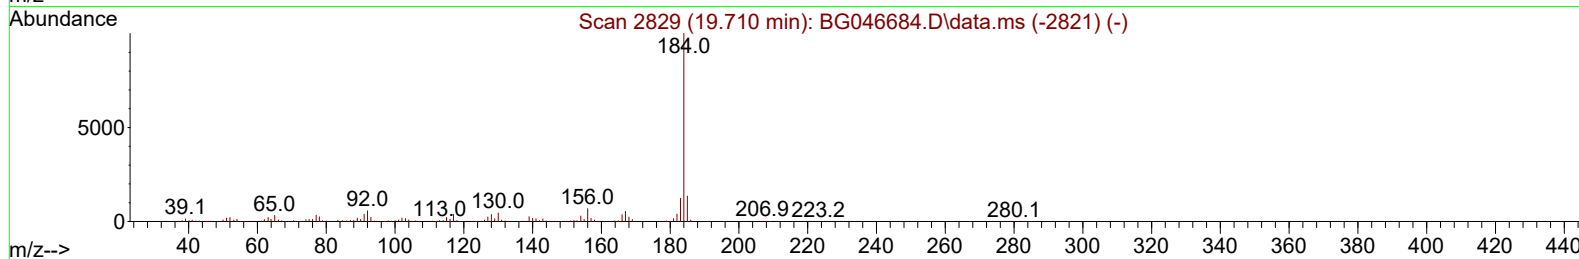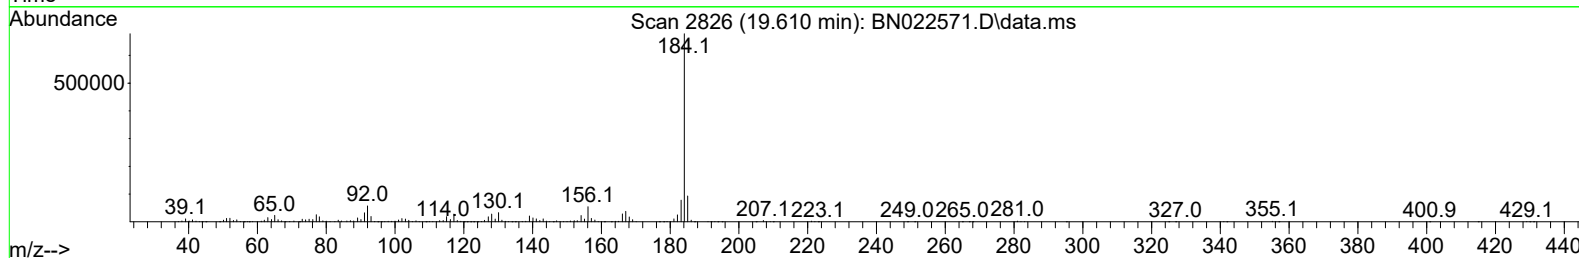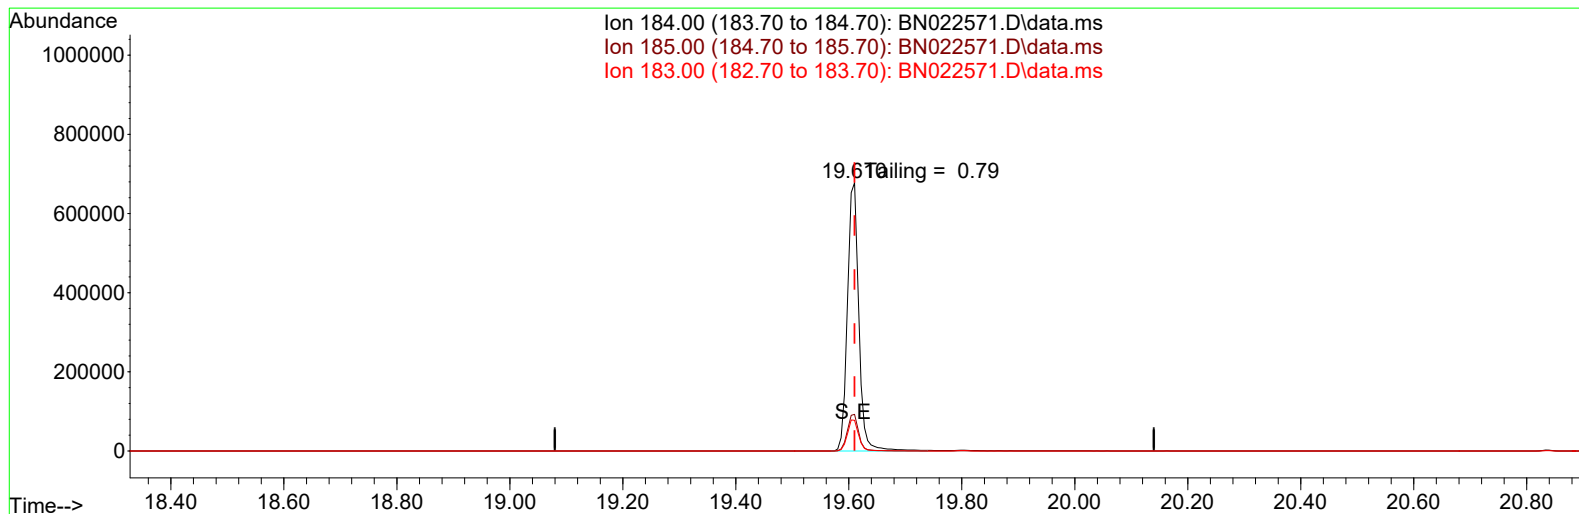

TIC: BN022571.D\data.ms

(77) Benzidine

19.610min (0.000) 0.00 ng

response 951680

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2022	BNA_N	<u>BN022571.D</u>
Compound Name	Response	Retention Time
DDT	526409	20.839
DDD	24705	20.398
DDE	1049	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25754	552163	4.66

Instrument :
BNA_N
ClientSampleId :
DFTPP