

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034935.D
 Acq On : 09 Nov 2024 11:03
 Operator : RC/JU
 Sample : P4744-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP63

Quant Time: Nov 09 22:51:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.571	152	2200	0.400	ng/ul	0.00
4) Naphthalene-d8	10.333	136	5806	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.208	164	4711	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.95
17) Chrysene-d12	21.145	240	12391	0.400	ng/ul	0.00
23) Perylene-d12	23.182	264	1121915	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	13115	6.265	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.934	152	3522	0.396	ng/ul	0.00
18) Fluoranthene-d10	18.986	212	15408	0.484	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.187	88	154	0.067	ng/ul#	80
12) Fluorene	15.207	166	1541	0.083	ng/ul#	14
20) Pyrene	19.353	202	1998	0.047	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034935.D
Acq On : 09 Nov 2024 11:03
Operator : RC/JU
Sample : P4744-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP63

Quant Time: Nov 09 22:51:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration




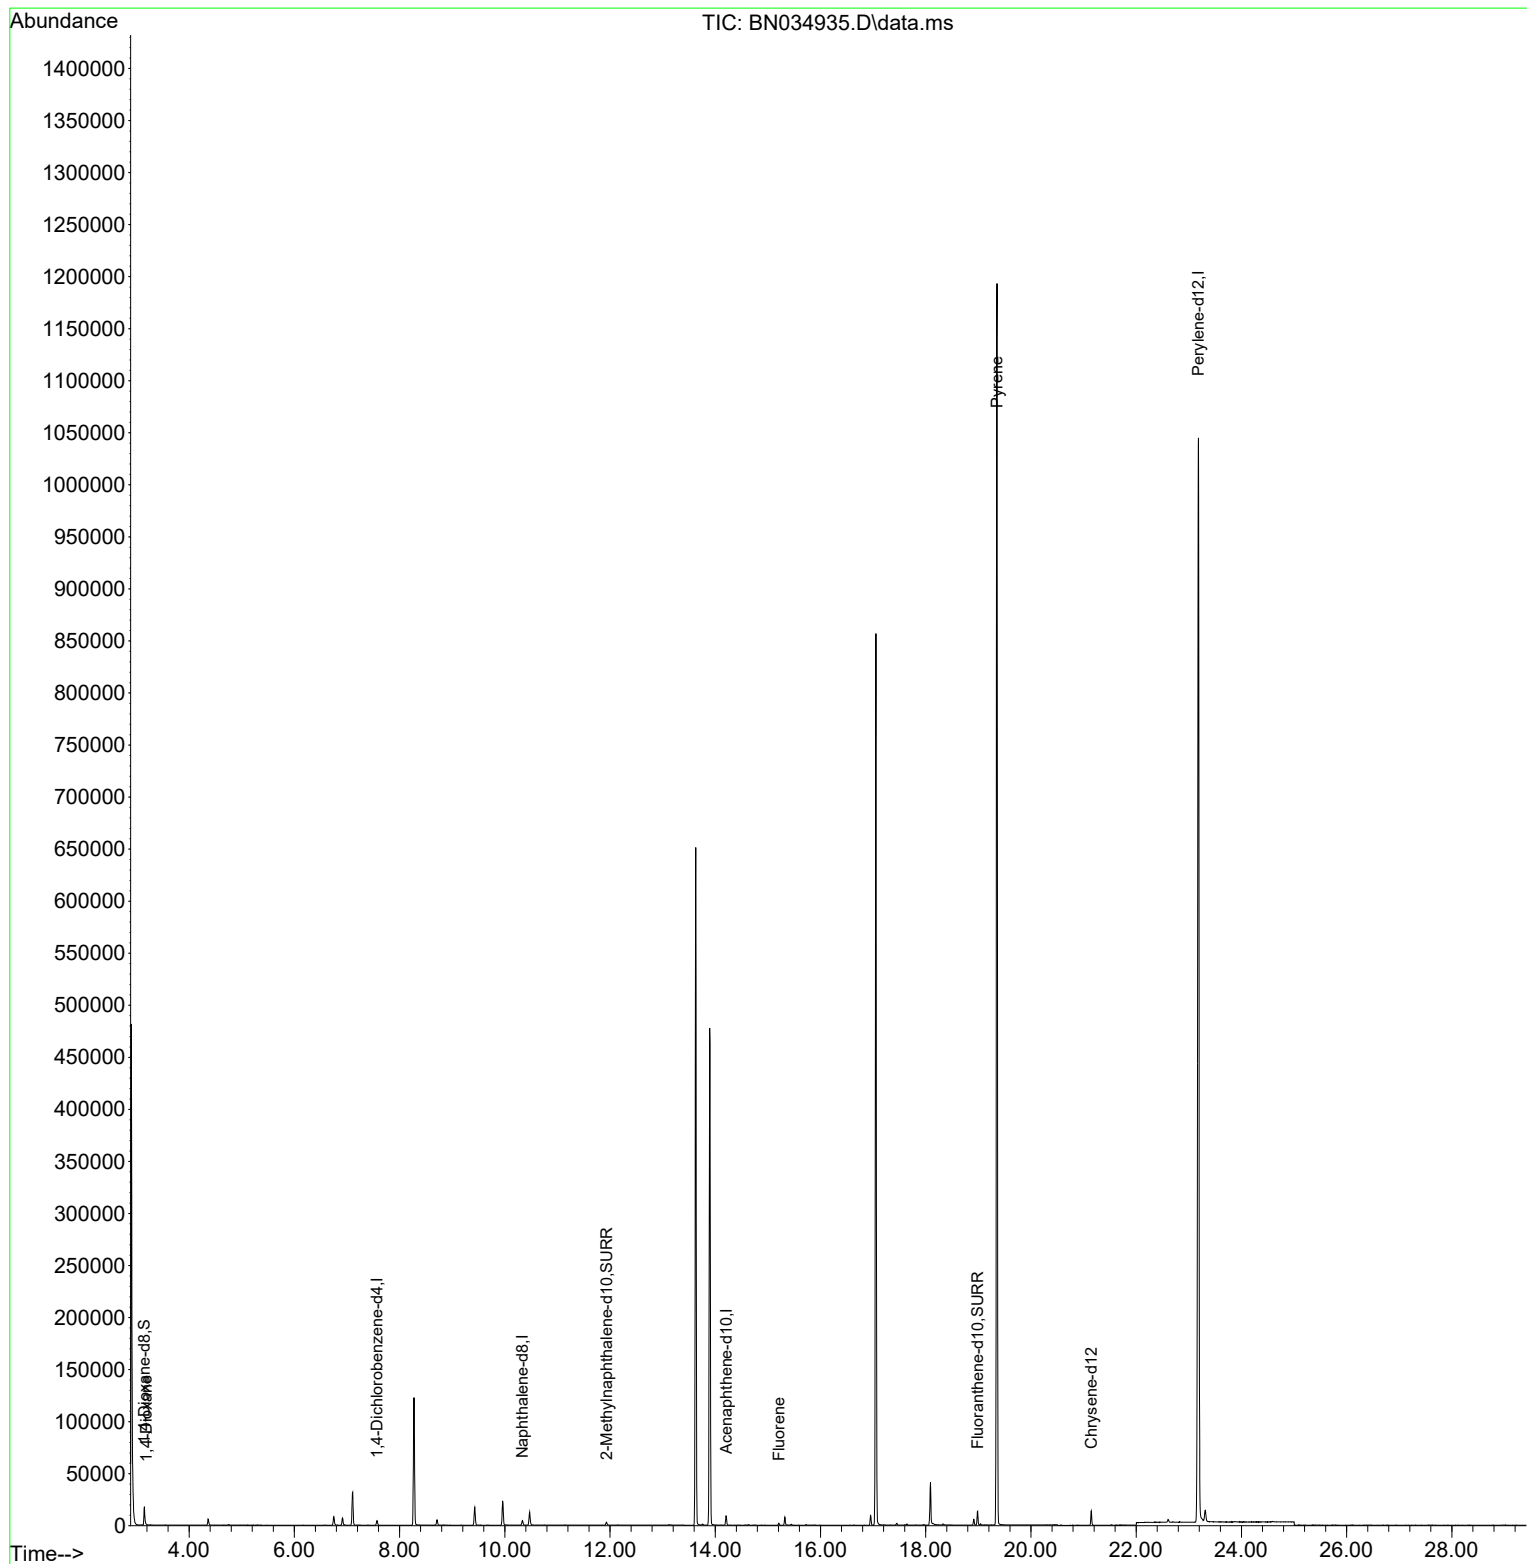


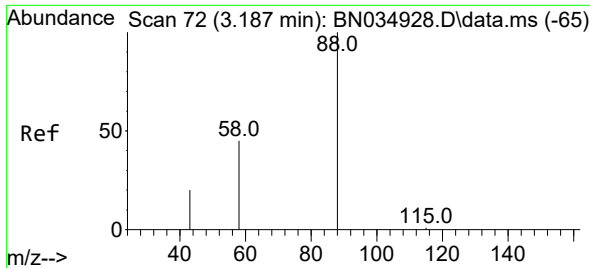

#2
 1,4-Dioxane
 Concen: 0.067 ng/ul
 RT: 3.187 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BN034935.D
 Acq: 09 Nov 2024 11:03




Instrument :
 BNA_N
 ClientSampleId :
 GCP63


Tgt Ion: 88 Resp: 154
 Ion Ratio Lower Upper
 88 100
 43 53.3 23.3 34.9#
 58 42.5 35.4 53.2

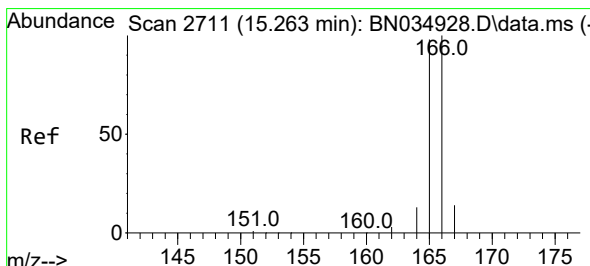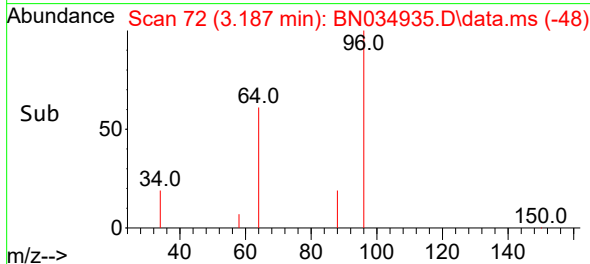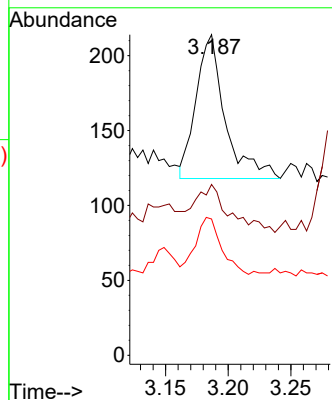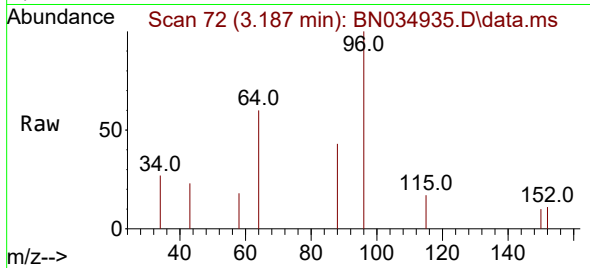

#12
 Fluorene
 Concen: 0.083 ng/ul
 RT: 15.207 min Scan# 2699
 Delta R.T. -0.055 min
 Lab File: BN034935.D
 Acq: 09 Nov 2024 11:03


Tgt Ion: 166 Resp: 1541
 Ion Ratio Lower Upper
 166 100
 165 8.2 79.0 118.4#
 167 35.6 11.8 17.6#

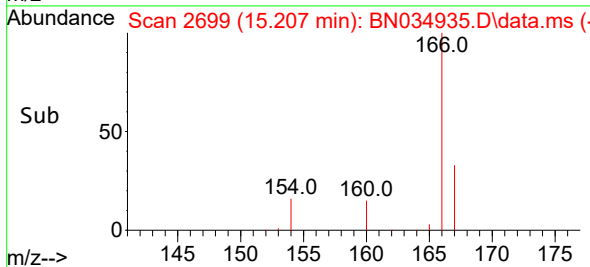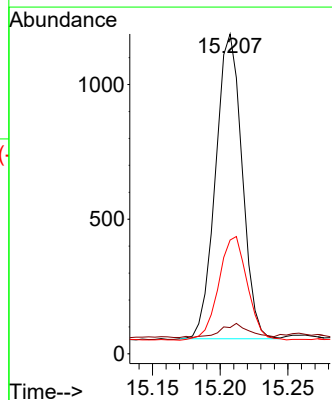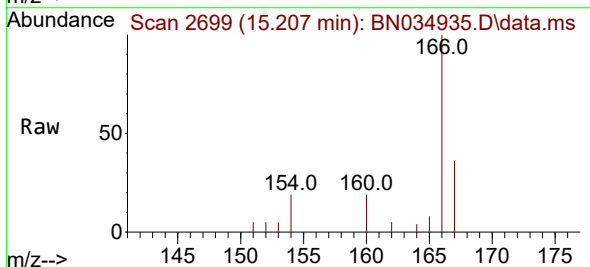

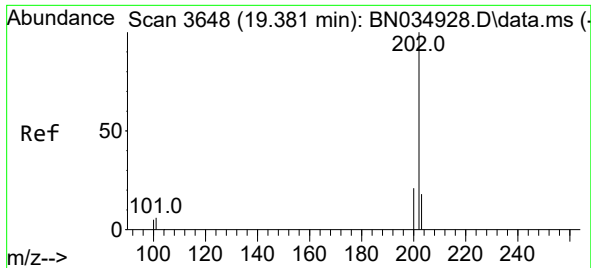

#20
 Pyrene
 Concen: 0.047 ng/ul
 RT: 19.353 min Scan# 30
 Delta R.T. -0.028 min
 Lab File: BN034935.D
 Acq: 09 Nov 2024 11:03

Instrument :
 BNA_N
 ClientSampleId :
 GCP63

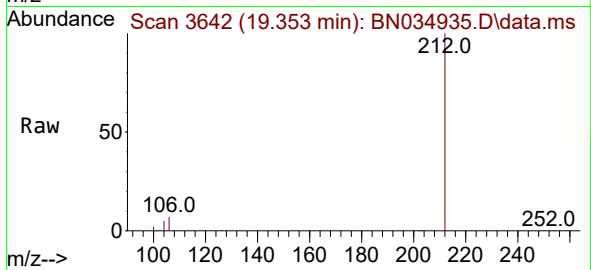

Tgt Ion:202 Resp: 1998
 Ion Ratio Lower Upper
 202 100
 101 146.4 5.0 7.4#
 100 1133.3 4.1 6.1#

