

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034940.D
 Acq On : 09 Nov 2024 14:02
 Operator : RC/JU
 Sample : P4744-14
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP68

Quant Time: Nov 09 22:52:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.570	152	3148	0.400	ng/ul	0.00
4) Naphthalene-d8	10.333	136	8424	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.208	164	6615	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.95
17) Chrysene-d12	21.145	240	16123	0.400	ng/ul	0.00
23) Perylene-d12	23.179	264	1179947	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.153	96	13238	4.419	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.934	152	4506	0.349	ng/ul	0.00
18) Fluoranthene-d10	18.986	212	19051	0.460	ng/ul	0.00
Target Compounds						
					Qvalue	
7) 2-Methylnaphthalene	12.005	142	2390	0.152	ng/ul	100
8) 1-Methylnaphthalene	12.225	142	1068	0.068	ng/ul	100
20) Pyrene	19.353	202	2529	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034940.D
Acq On : 09 Nov 2024 14:02
Operator : RC/JU
Sample : P4744-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP68

Quant Time: Nov 09 22:52:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration




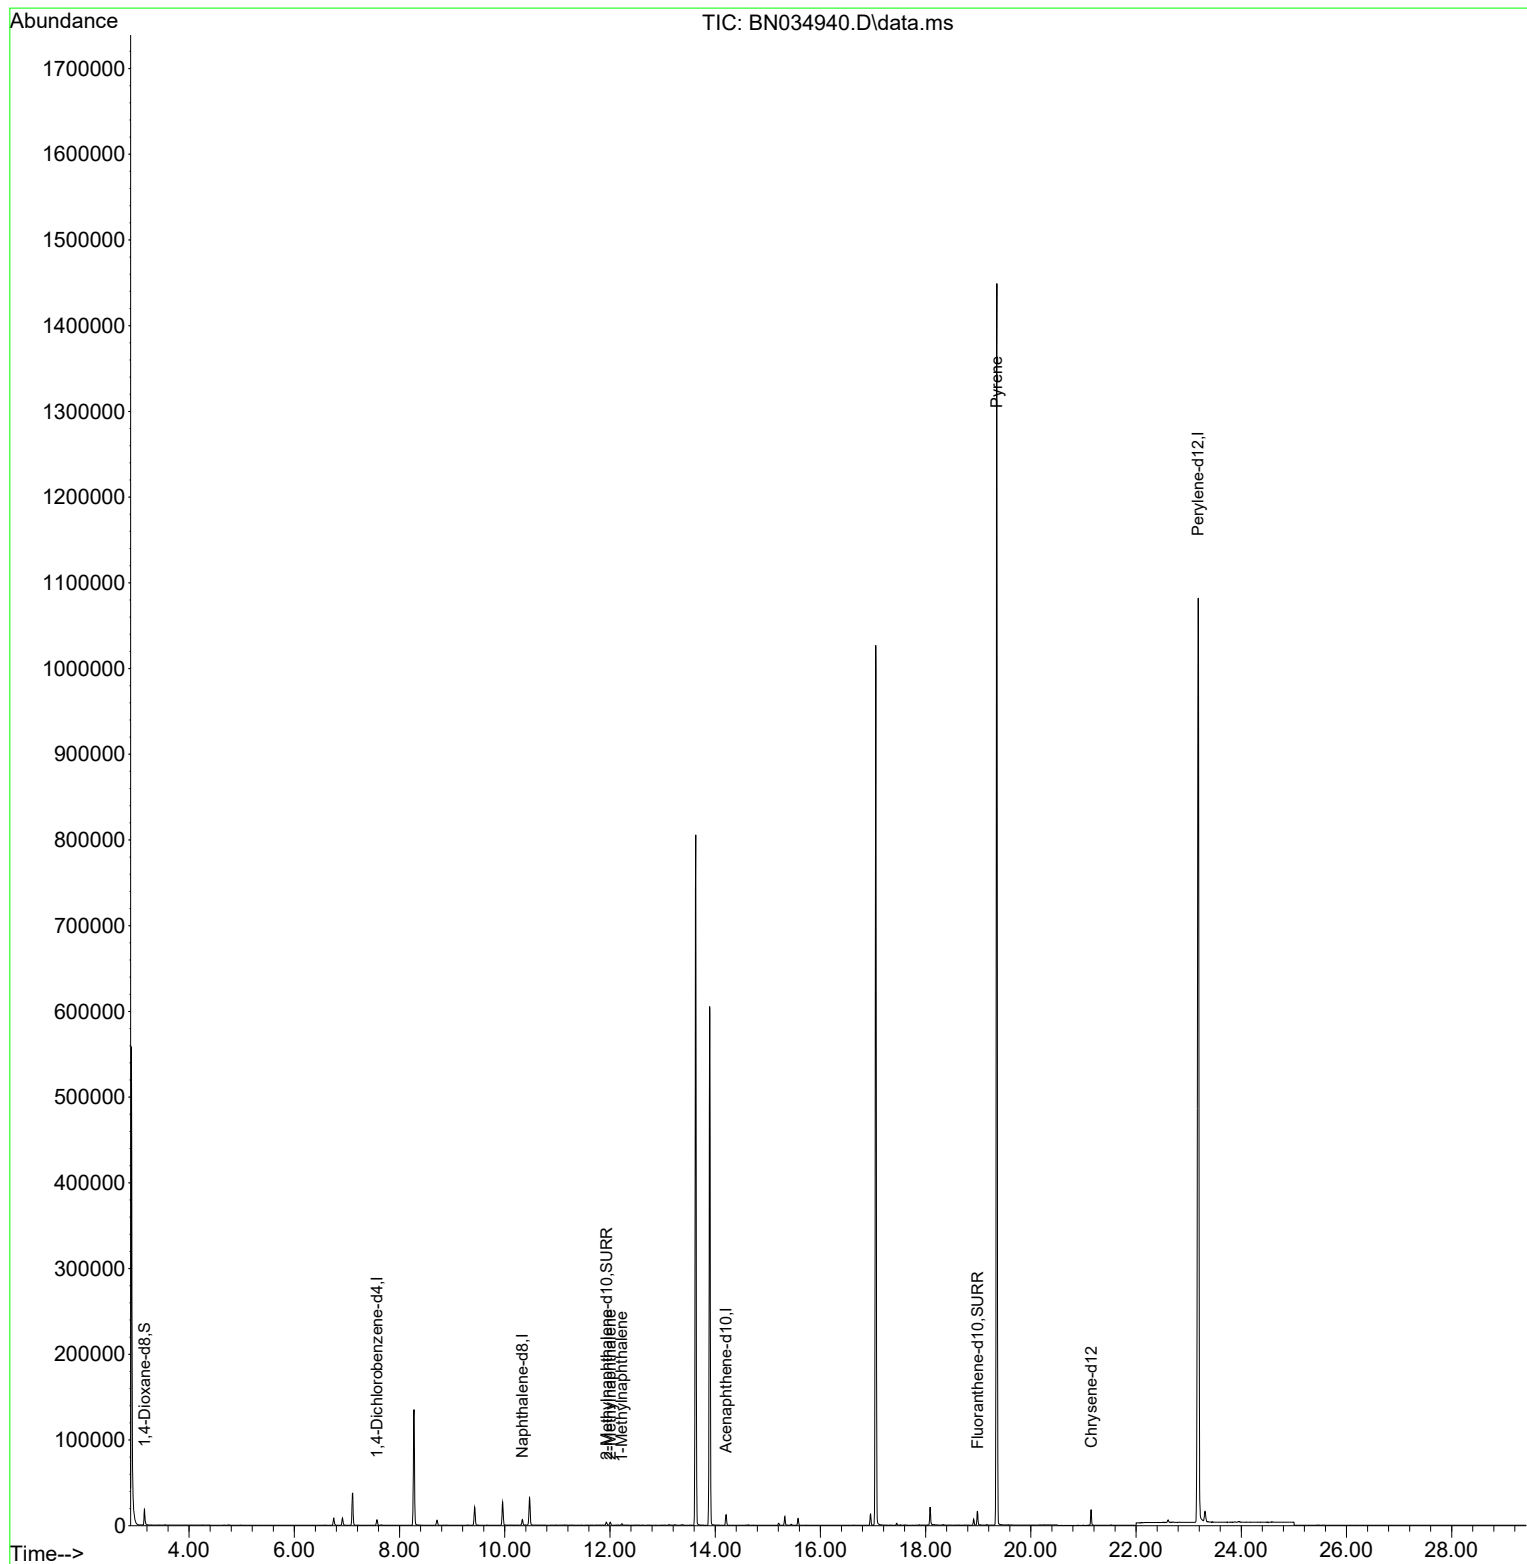


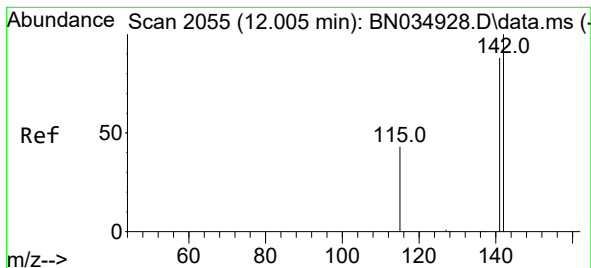

#7
2-Methylnaphthalene
Concen: 0.152 ng/ul
RT: 12.005 min Scan# 2055
Delta R.T. -0.006 min
Lab File: BN034940.D
Acq: 09 Nov 2024 14:02




Instrument :
BNA_N
ClientSampleId :
GCP68


Tgt Ion:142 Resp: 2390
Ion Ratio Lower Upper
142 100
141 88.8 70.8 106.2

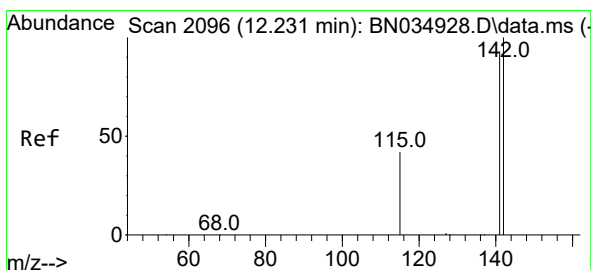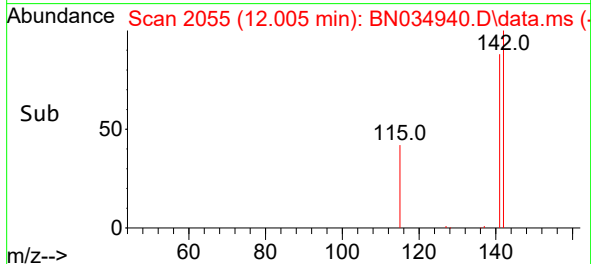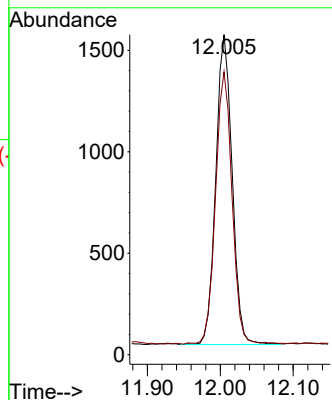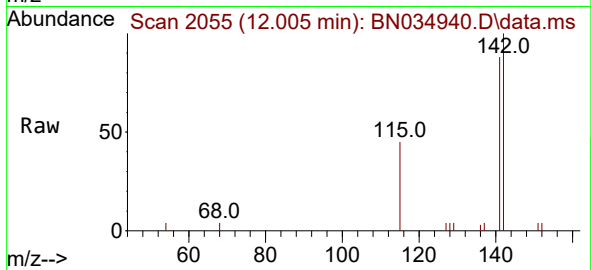

#8
1-Methylnaphthalene
Concen: 0.068 ng/ul
RT: 12.225 min Scan# 2095
Delta R.T. -0.006 min
Lab File: BN034940.D
Acq: 09 Nov 2024 14:02

Tgt Ion:142 Resp: 1068
Ion Ratio Lower Upper
142 100
141 92.9 74.6 111.8

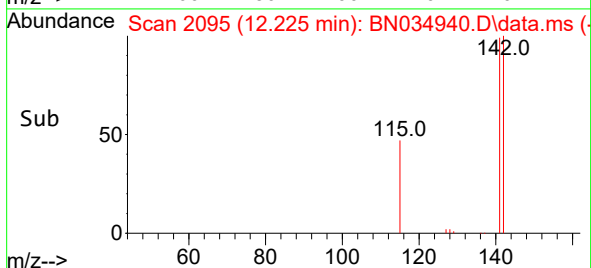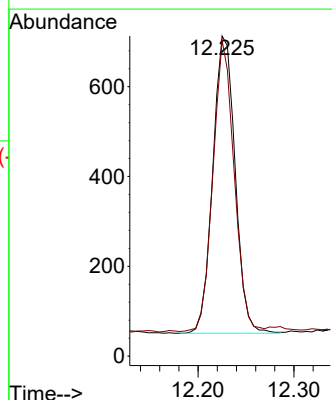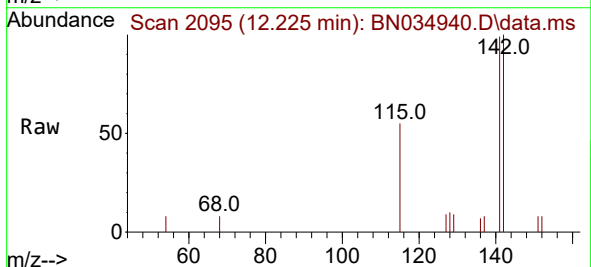

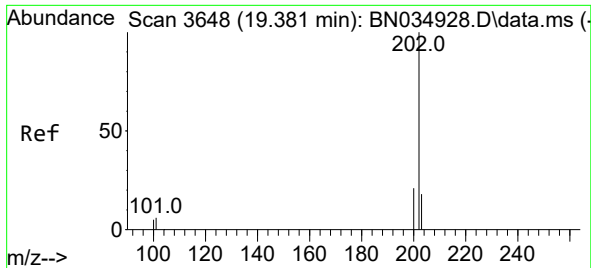

#20

Pyrene

Concen: 0.045 ng/ul

RT: 19.353 min Scan# 30

Delta R.T. -0.028 min

Lab File: BN034940.D


Acq: 09 Nov 2024 14:02

Instrument :

BNA_N

ClientSampleId :

GCP68

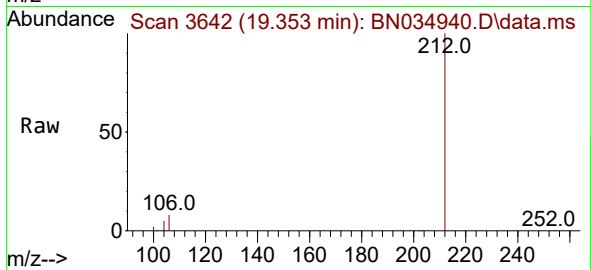

Tgt Ion:202 Resp: 2529

Ion Ratio Lower Upper

202 100

101 143.8 5.0 7.4#

100 1078.4 4.1 6.1#

