

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034943.D
 Acq On : 09 Nov 2024 15:50
 Operator : RC/JU
 Sample : P4715-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK4

Quant Time: Nov 09 22:52:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.570	152	2032	0.400	ng/ul	0.00
4) Naphthalene-d8	10.333	136	5386	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.208	164	4296	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.95
17) Chrysene-d12	21.148	240	12254	0.400	ng/ul	0.00
23) Perylene-d12	23.179	264	627992	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	9140	4.727	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.928	152	1665	0.202	ng/ul	0.00
18) Fluoranthene-d10	18.986	212	7516	0.239	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.014	202	2262	0.055	ng/ul#	85
20) Pyrene	19.376	202	2322	0.055	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034943.D
Acq On : 09 Nov 2024 15:50
Operator : RC/JU
Sample : P4715-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK4

Quant Time: Nov 09 22:52:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration




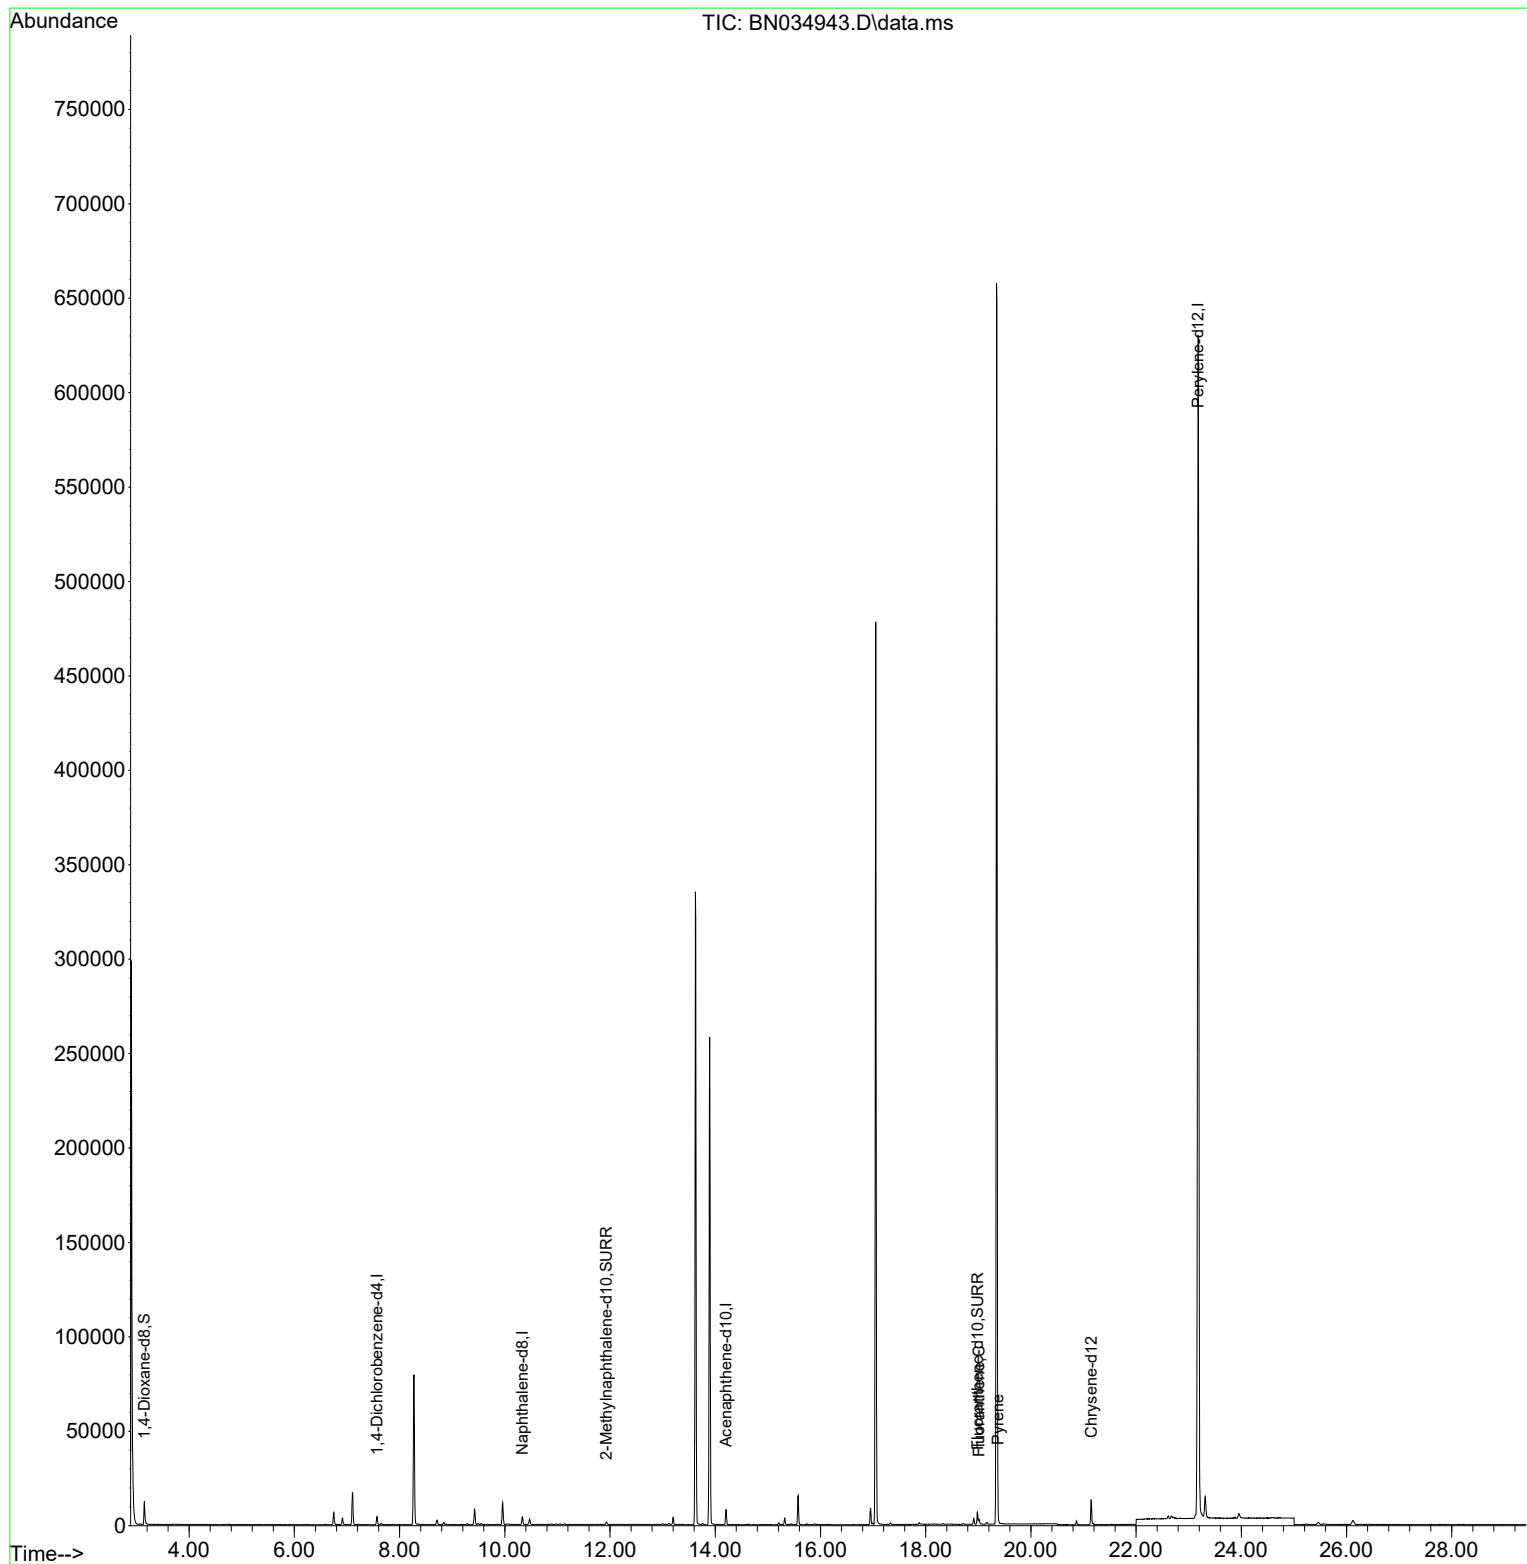


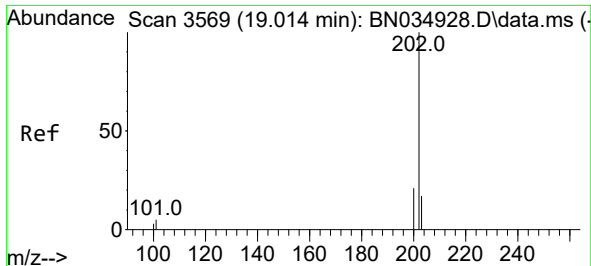

#19
Fluoranthene
Concen: 0.055 ng/ul
RT: 19.014 min Scan# 3569
Delta R.T. -0.005 min
Lab File: BN034943.D
Acq: 09 Nov 2024 15:50

Instrument :
BNA_N
ClientSampleId :
C0AK4

Tgt Ion:202 Resp: 2262
Ion Ratio Lower Upper
202 100
101 11.1 4.2 6.2#
100 7.4 3.2 4.8#

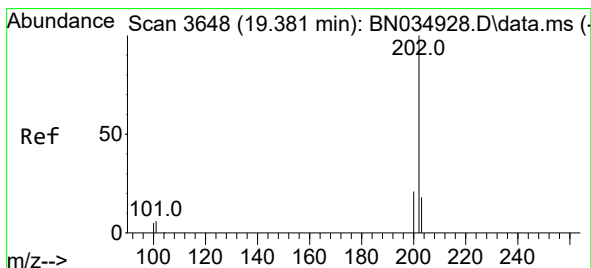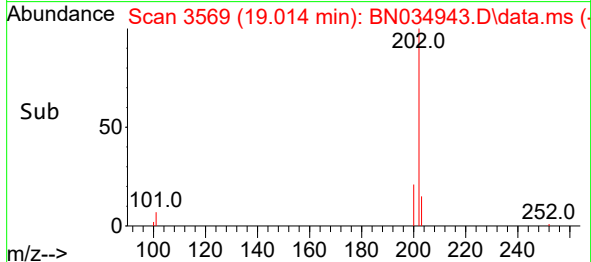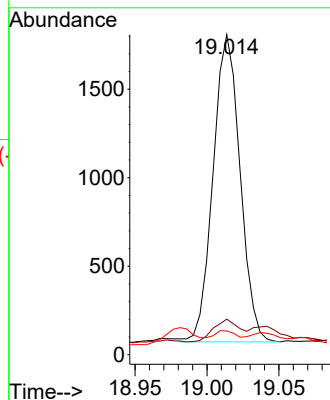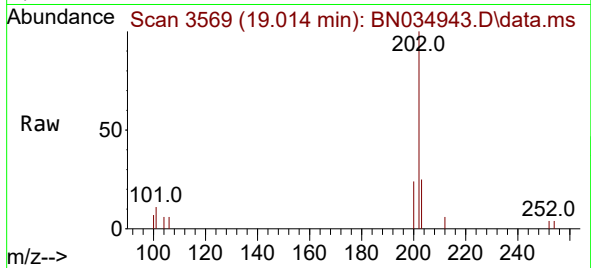

#20
Pyrene
Concen: 0.055 ng/ul
RT: 19.376 min Scan# 3647
Delta R.T. -0.005 min
Lab File: BN034943.D
Acq: 09 Nov 2024 15:50

Tgt Ion:202 Resp: 2322
Ion Ratio Lower Upper
202 100
101 11.0 5.0 7.4#
100 11.0 4.1 6.1#

