

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034946.D
 Acq On : 09 Nov 2024 18:13
 Operator : RC/JU
 Sample : PB164777BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK777

Quant Time: Nov 09 22:53:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.571	152	2557	0.400	ng/ul	0.00
4) Naphthalene-d8	10.333	136	6720	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.203	164	5398	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.95
17) Chrysene-d12	21.145	240	12965	0.400	ng/ul	0.00
23) Perylene-d12	23.179	264	869208	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	12476	5.128	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.928	152	3377	0.328	ng/ul	0.00
18) Fluoranthene-d10	18.981	212	11592	0.348	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.207	166	1314	0.062	ng/ul#	15
20) Pyrene	19.348	202	1564	0.035	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034946.D
Acq On : 09 Nov 2024 18:13
Operator : RC/JU
Sample : PB164777BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK777

Quant Time: Nov 09 22:53:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration




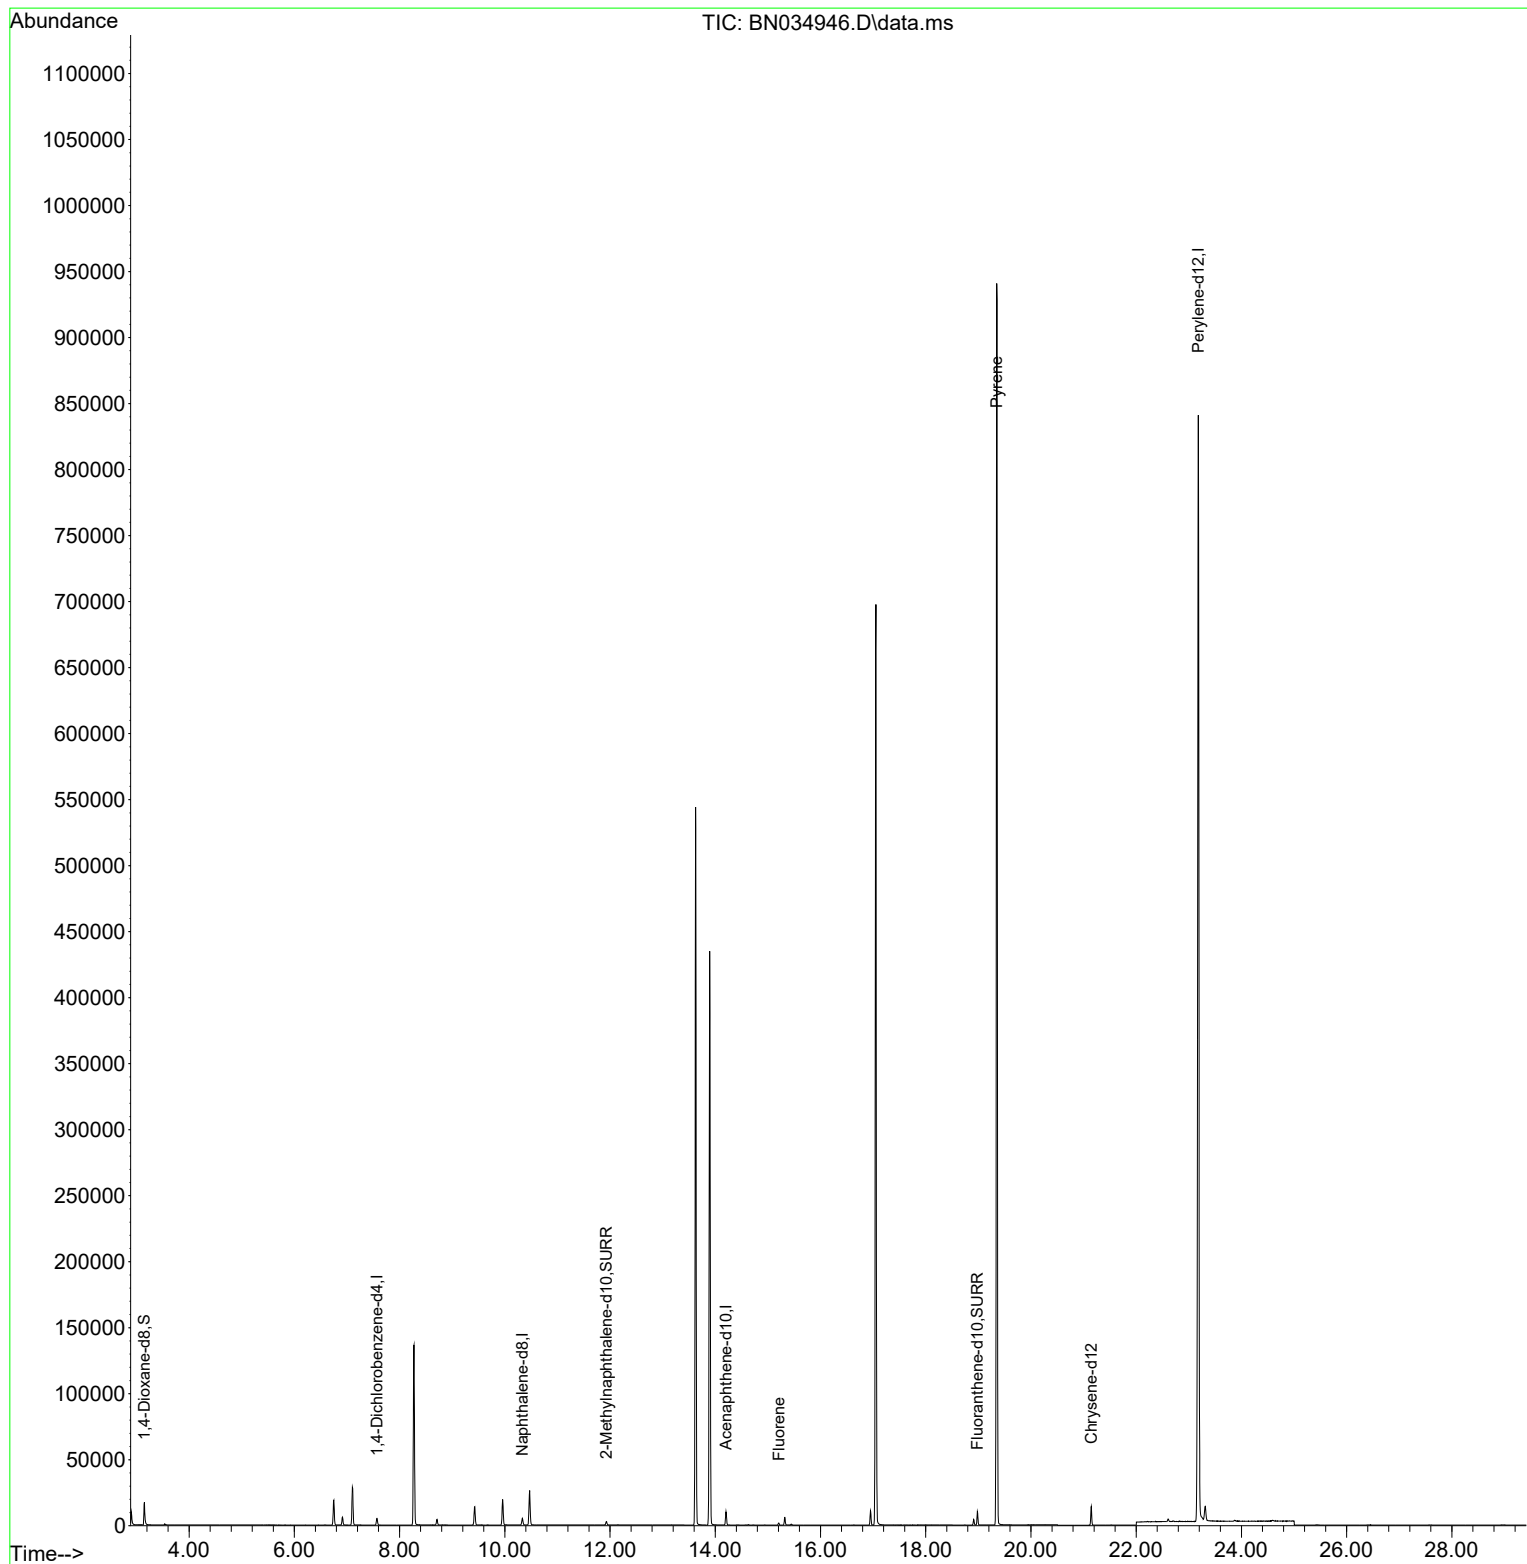


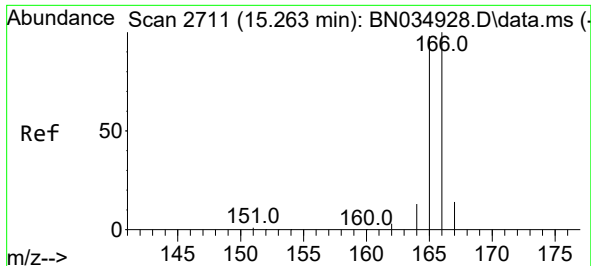

#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.207 min Scan# 20
Delta R.T. -0.055 min
Lab File: BN034946.D
Acq: 09 Nov 2024 18:13

Instrument :
BNA_N
ClientSampleId :
SBLK777

Tgt Ion:166 Resp: 1314
Ion Ratio Lower Upper
166 100
165 10.3 79.0 118.4#
167 37.4 11.8 17.6#

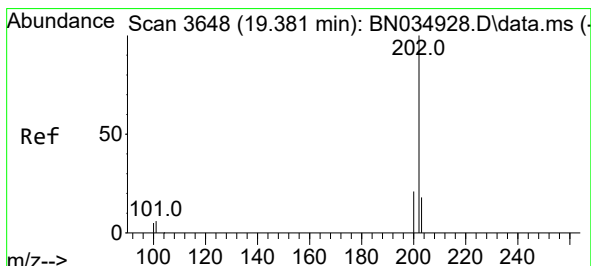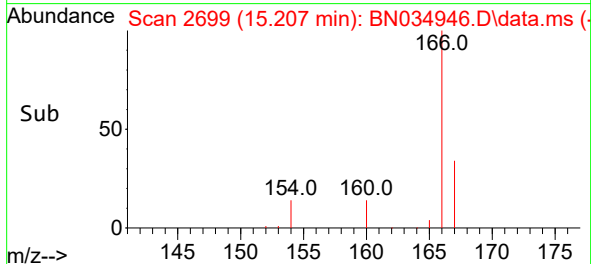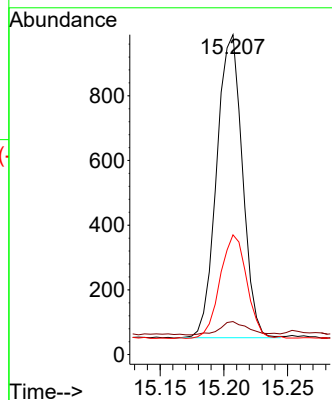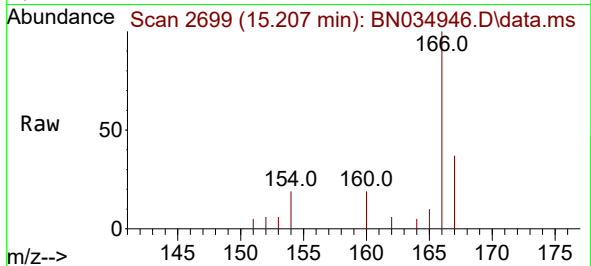

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.348 min Scan# 3641
Delta R.T. -0.032 min
Lab File: BN034946.D
Acq: 09 Nov 2024 18:13

Tgt Ion:202 Resp: 1564
Ion Ratio Lower Upper
202 100
101 156.7 5.0 7.4#
100 1256.7 4.1 6.1#

