

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034972.D
 Acq On : 10 Nov 2024 10:21
 Operator : RC/JU
 Sample : P4746-17
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP90

Quant Time: Nov 10 21:51:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.566	152	2689	0.400	ng/ul	0.00
4) Naphthalene-d8	10.328	136	6822	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.203	164	5134	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.95
17) Chrysene-d12	21.142	240	12047	0.400	ng/ul	0.00
23) Perylene-d12	23.176	264	1150803	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	13691	5.351	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.928	152	3650	0.349	ng/ul	0.00
18) Fluoranthene-d10	18.981	212	12814	0.414	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.187	88	164	0.058	ng/ul#	80
12) Fluorene	15.203	166	1564	0.077	ng/ul#	14
20) Pyrene	19.349	202	1823	0.044	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034972.D
Acq On : 10 Nov 2024 10:21
Operator : RC/JU
Sample : P4746-17
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP90

Quant Time: Nov 10 21:51:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration




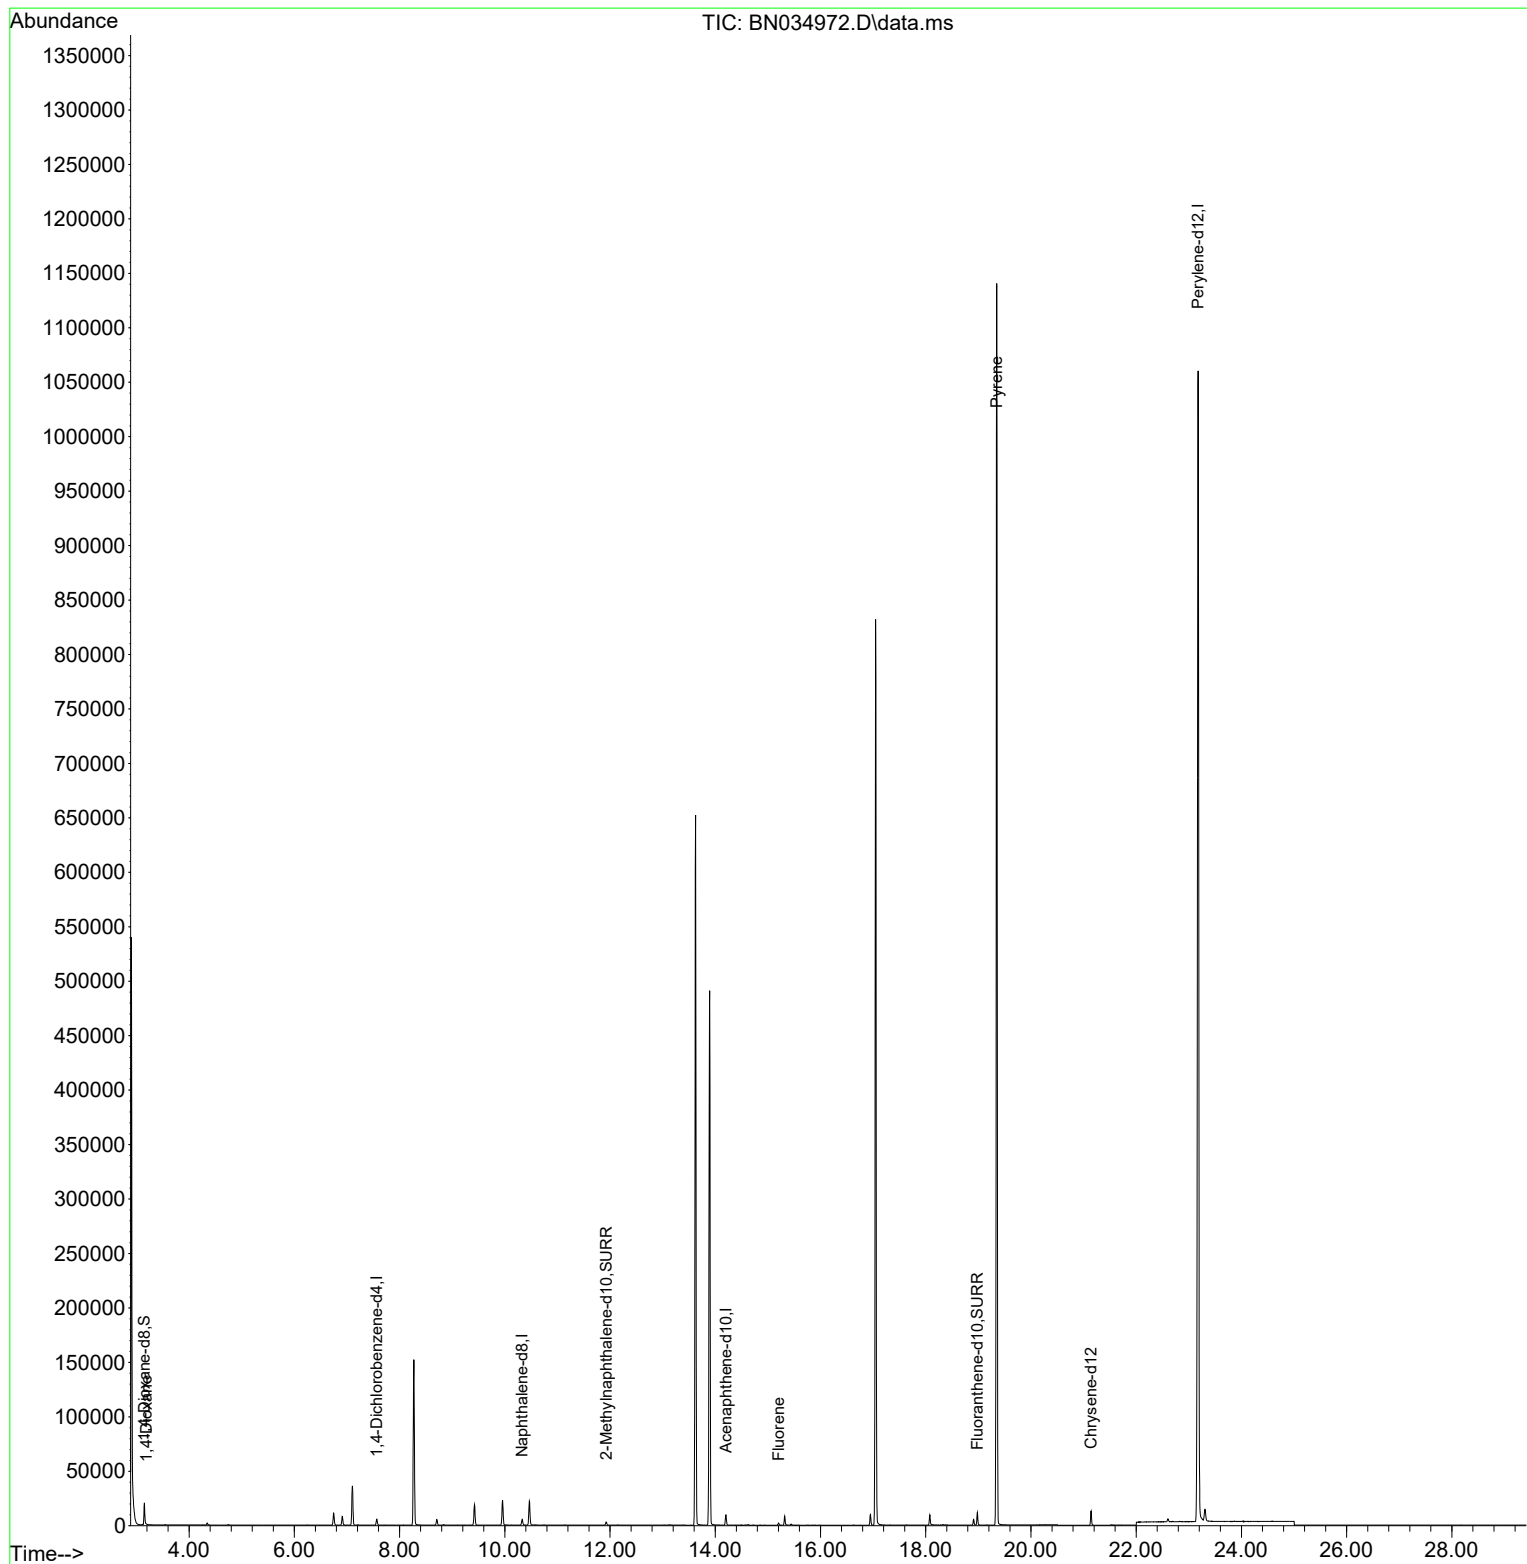


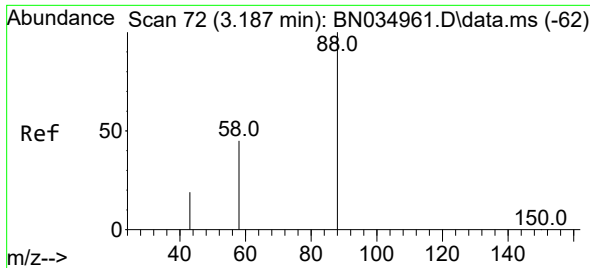

#2
 1,4-Dioxane
 Concen: 0.058 ng/ul
 RT: 3.187 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BN034972.D
 Acq: 10 Nov 2024 10:21




Instrument :
 BNA_N
 ClientSampleId :
 GCP90


Tgt Ion: 88 Resp: 164
 Ion Ratio Lower Upper
 88 100
 43 38.8 23.3 34.9#
 58 30.3 35.4 53.2#

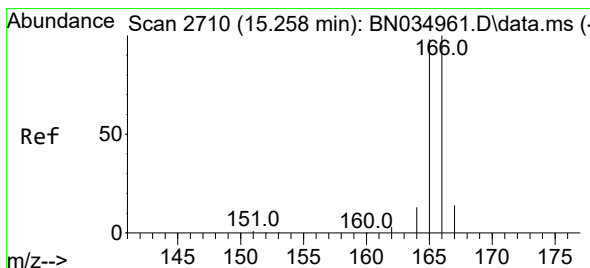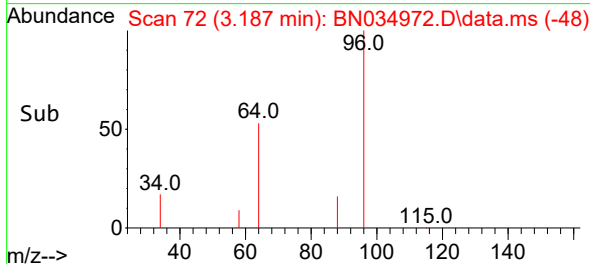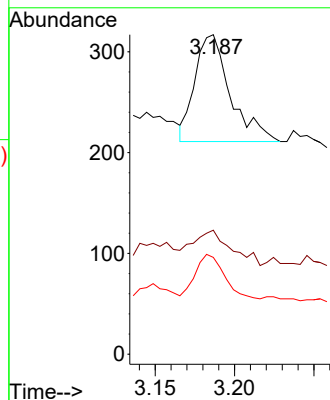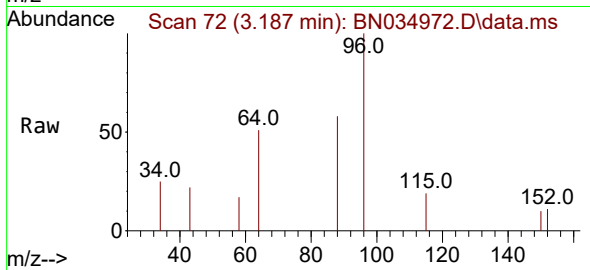

#12
 Fluorene
 Concen: 0.077 ng/ul
 RT: 15.203 min Scan# 2698
 Delta R.T. -0.060 min
 Lab File: BN034972.D
 Acq: 10 Nov 2024 10:21


Tgt Ion:166 Resp: 1564
 Ion Ratio Lower Upper
 166 100
 165 9.2 79.0 118.4#
 167 38.1 11.8 17.6#

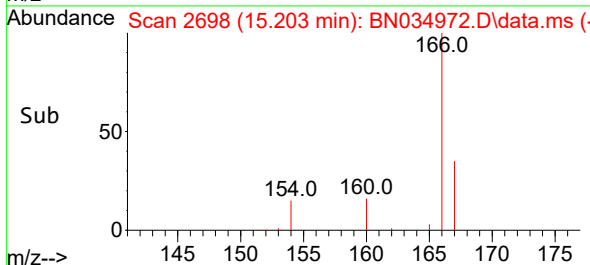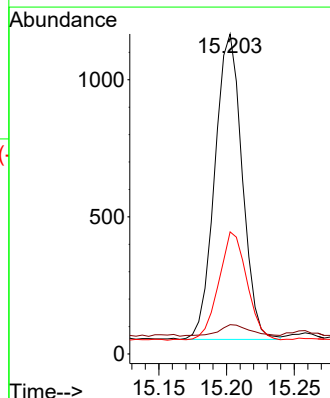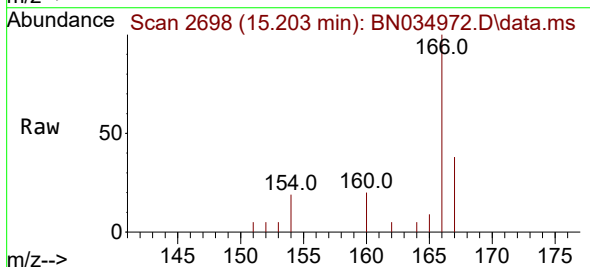

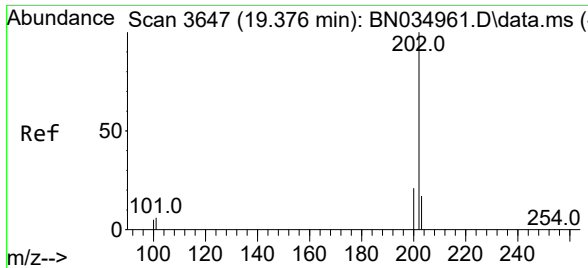

#20
 Pyrene
 Concen: 0.044 ng/ul
 RT: 19.349 min Scan# 30
 Delta R.T. -0.032 min
 Lab File: BN034972.D
 Acq: 10 Nov 2024 10:21

Instrument :
 BNA_N
 ClientSampleId :
 GCP90

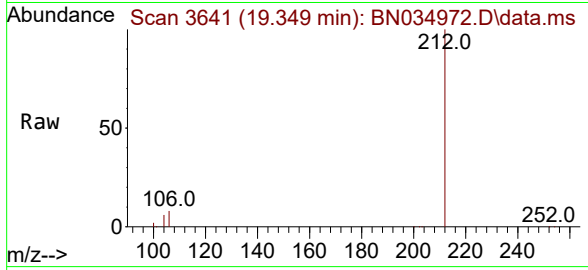

Tgt Ion:202 Resp: 1823
 Ion Ratio Lower Upper
 202 100
 101 145.0 5.0 7.4#
 100 1123.0 4.1 6.1#

