

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034978.D
 Acq On : 10 Nov 2024 14:31
 Operator : RC/JU
 Sample : PB164814BL
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK814

Quant Time: Nov 10 21:52:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.566	152	2251	0.400	ng/ul	0.00
4) Naphthalene-d8	10.328	136	5599	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.203	164	4223	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.95
17) Chrysene-d12	21.142	240	9531	0.400	ng/ul	0.00
23) Perylene-d12	23.174	264	871464	0.400	ng/ul	#-0.14
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	14624	6.828	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.928	152	3464	0.404	ng/ul	0.00
18) Fluoranthene-d10	18.981	212	10533	0.430	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.349	202	1417	0.043	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034978.D
Acq On : 10 Nov 2024 14:31
Operator : RC/JU
Sample : PB164814BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK814


Quant Time: Nov 10 21:52:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

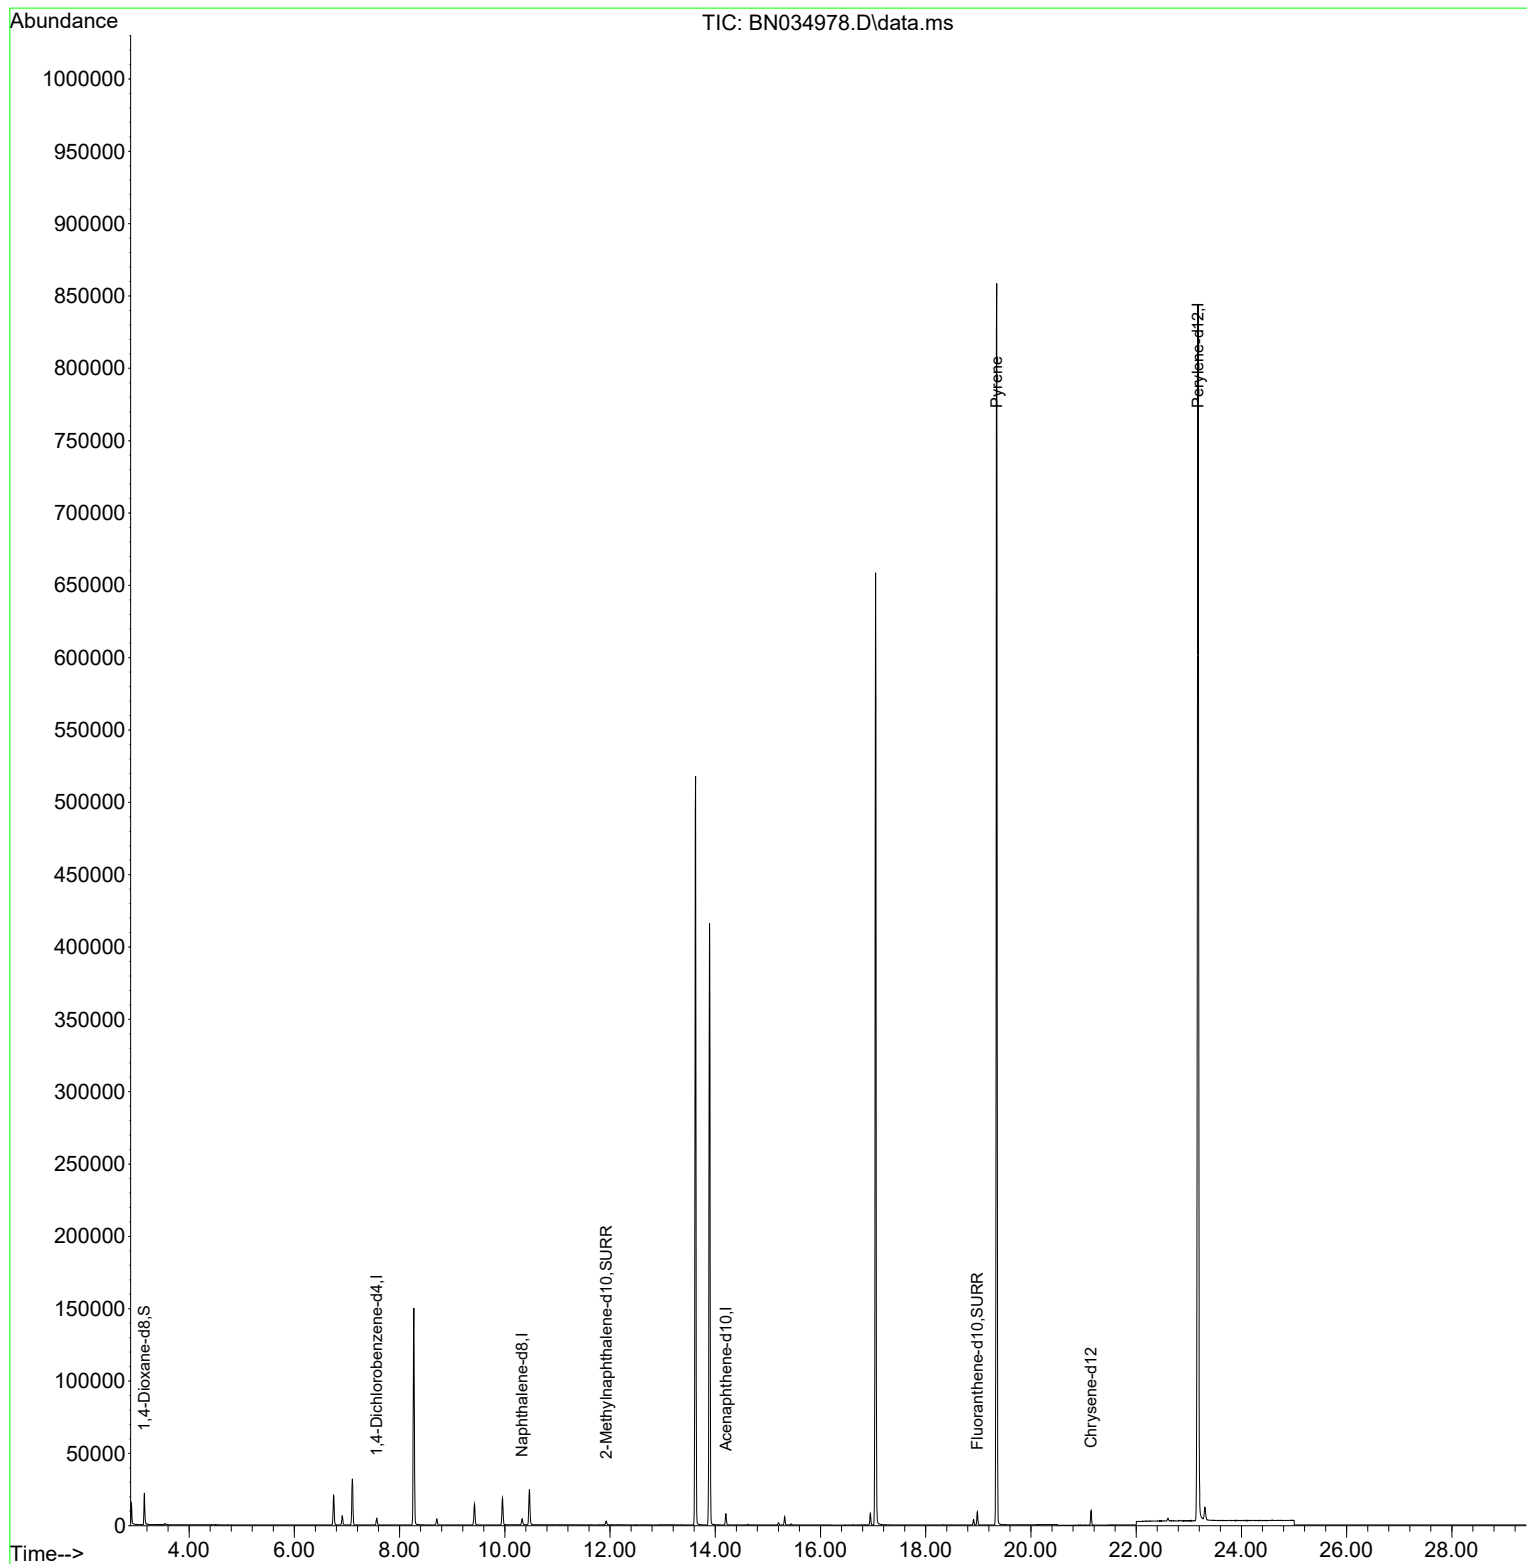

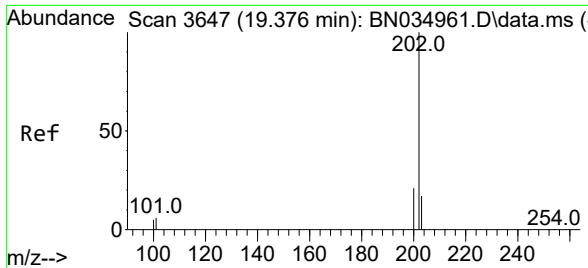

#20
 Pyrene
 Concen: 0.043 ng/ul
 RT: 19.349 min Scan# 30
 Delta R.T. -0.032 min
 Lab File: BN034978.D
 Acq: 10 Nov 2024 14:31

Instrument :
 BNA_N
 ClientSampleId :
 SBLK814

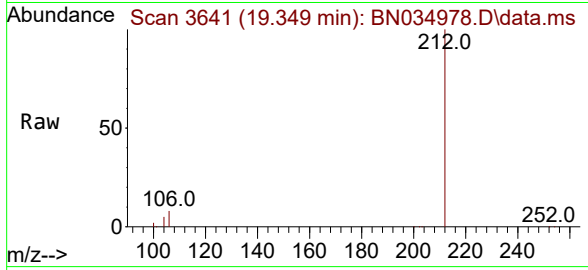

Tgt Ion:202 Resp: 1417
 Ion Ratio Lower Upper
 202 100
 101 140.2 5.0 7.4#
 100 1058.3 4.1 6.1#

