

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034982.D
Acq On : 10 Nov 2024 16:54
Operator : RC/JU
Sample : P4746-07
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP82

Quant Time: Nov 10 21:52:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.566	152	2746	0.400	ng/ul	0.00
4) Naphthalene-d8	10.328	136	6976	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.203	164	5229	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.95
17) Chrysene-d12	21.140	240	11293	0.400	ng/ul	# 0.00
23) Perylene-d12	23.176	264	1086831	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	13792	5.278	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.923	152	4100	0.384	ng/ul	-0.01
18) Fluoranthene-d10	18.981	212	13810	0.476	ng/ul	0.00
Target Compounds					Qvalue	
20) Pyrene	19.349	202	1737	0.044	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034982.D
Acq On : 10 Nov 2024 16:54
Operator : RC/JU
Sample : P4746-07
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP82


Quant Time: Nov 10 21:52:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

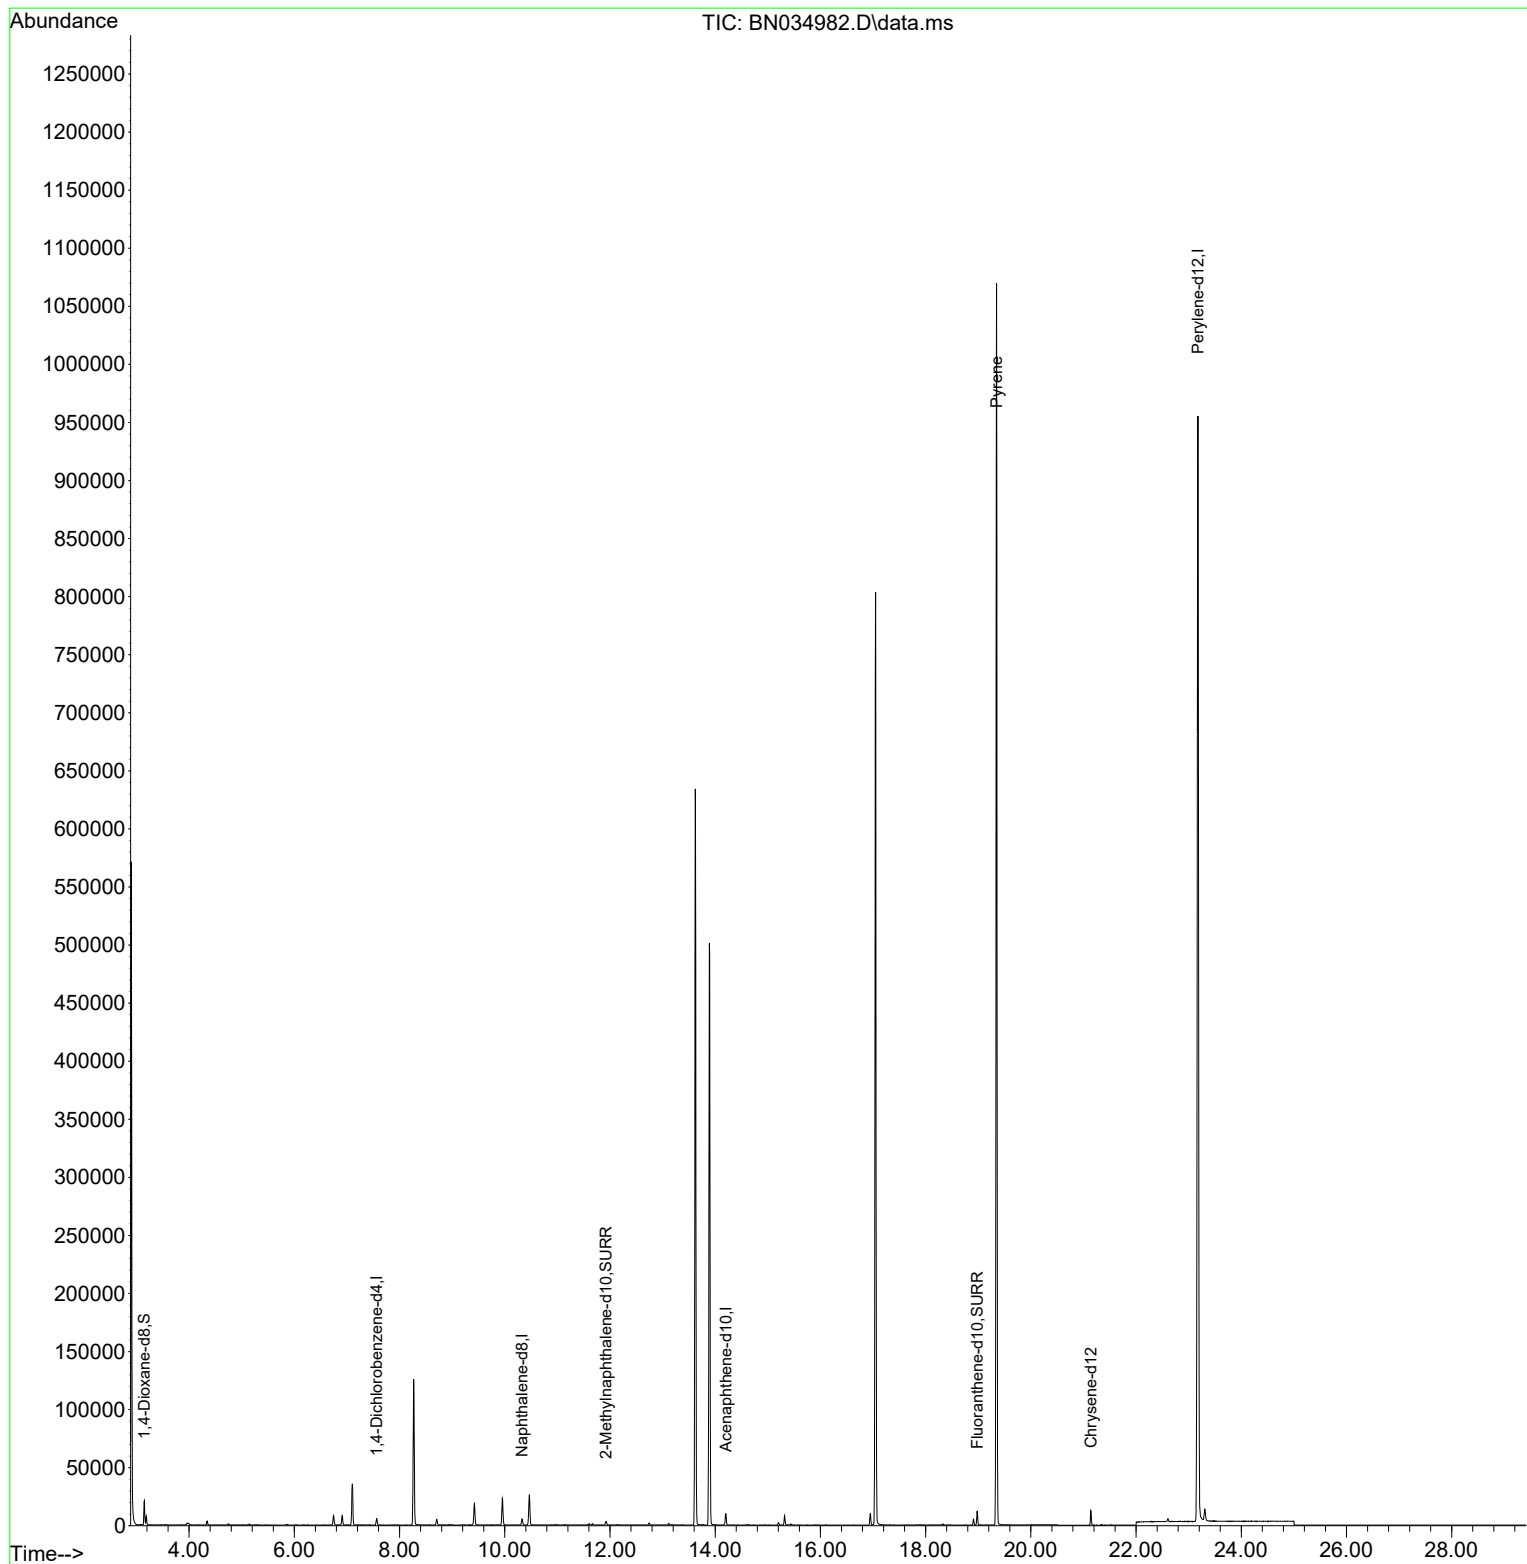

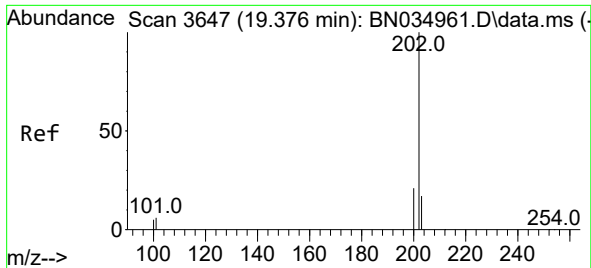

#20
 Pyrene
 Concen: 0.044 ng/ul
 RT: 19.349 min Scan# 30
 Delta R.T. -0.032 min
 Lab File: BN034982.D
 Acq: 10 Nov 2024 16:54

Instrument :
 BNA_N
 ClientSampleId :
 GCP82

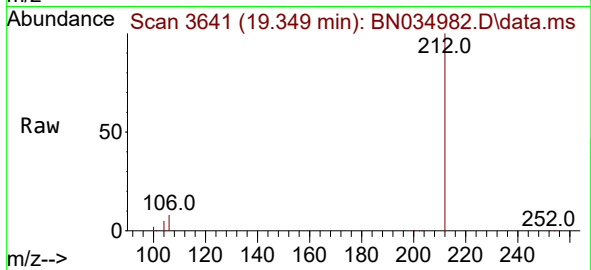

Tgt Ion:202 Resp: 1737
 Ion Ratio Lower Upper
 202 100
 101 141.0 5.0 7.4#
 100 1064.2 4.1 6.1#

