




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034942.D
 Acq On : 09 Nov 2024 15:14
 Operator : RC/JU
 Sample : P4746-22DL 5X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP95DL

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:52:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

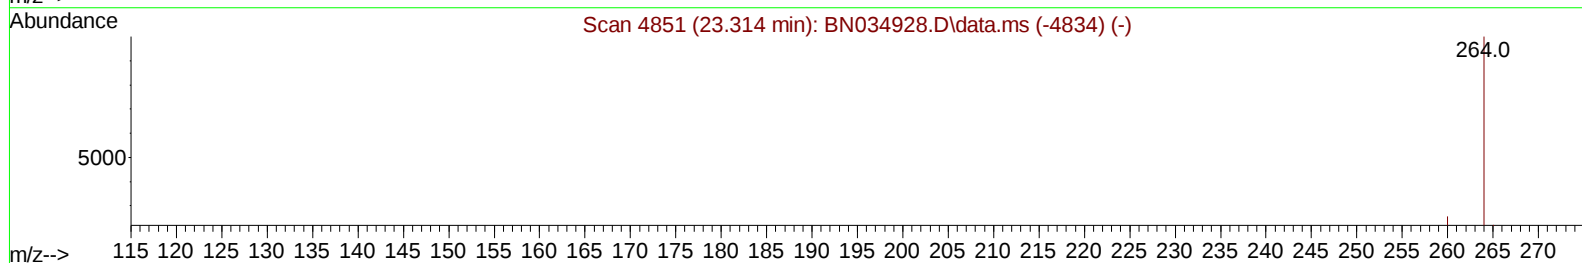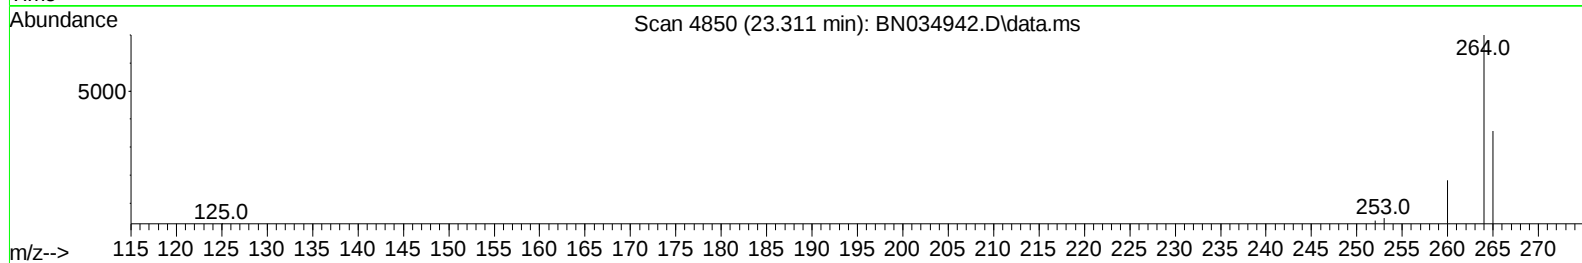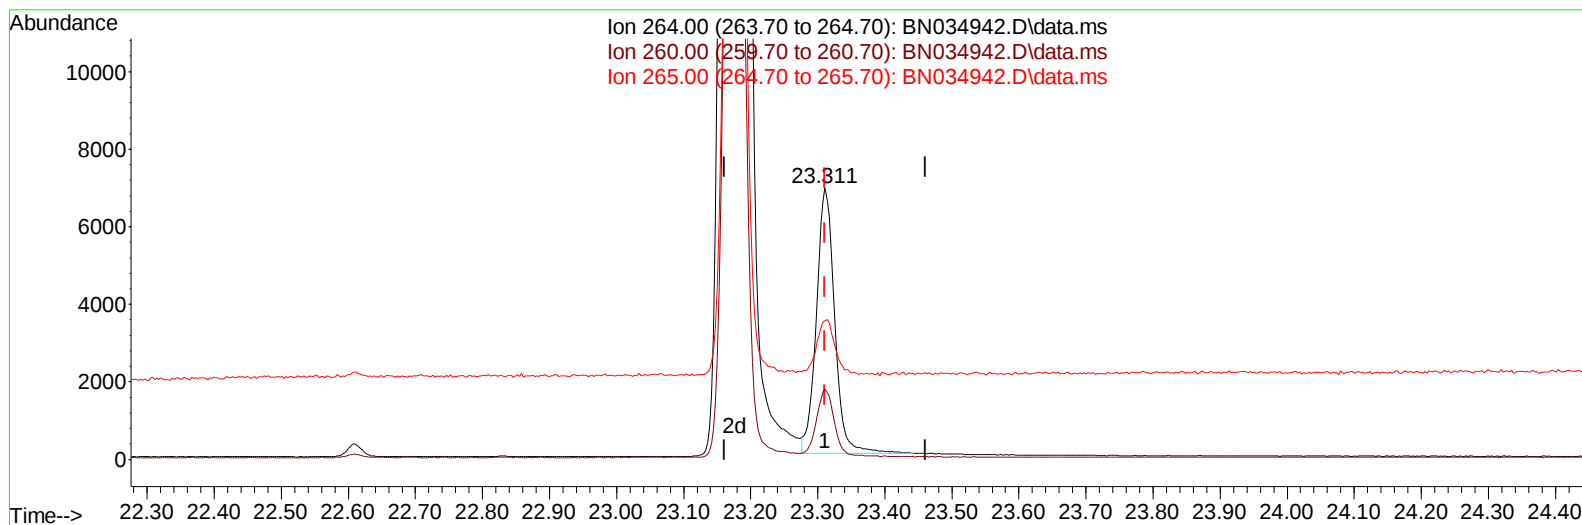

TIC: BN034942.D\data.ms

(23) Perylene-d12 (I)

23.311min (+ 0.000) 0.40 ng/ul

response 12791

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	25.85
265.00	52.80	51.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034942.D
Acq On : 09 Nov 2024 15:14
Operator : RC/JU
Sample : P4746-22DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP95DL

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:52:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024

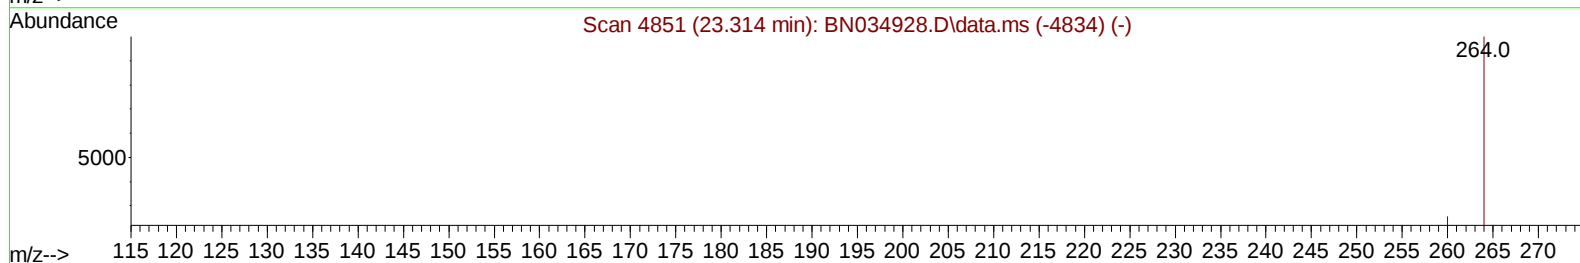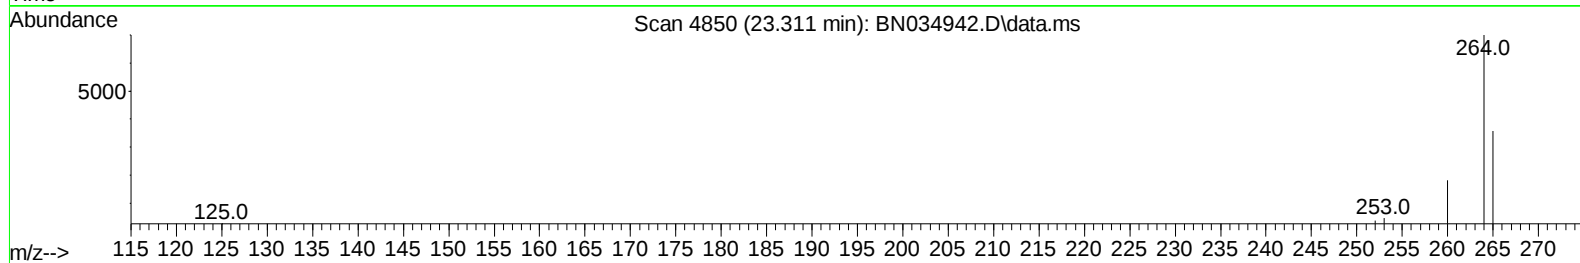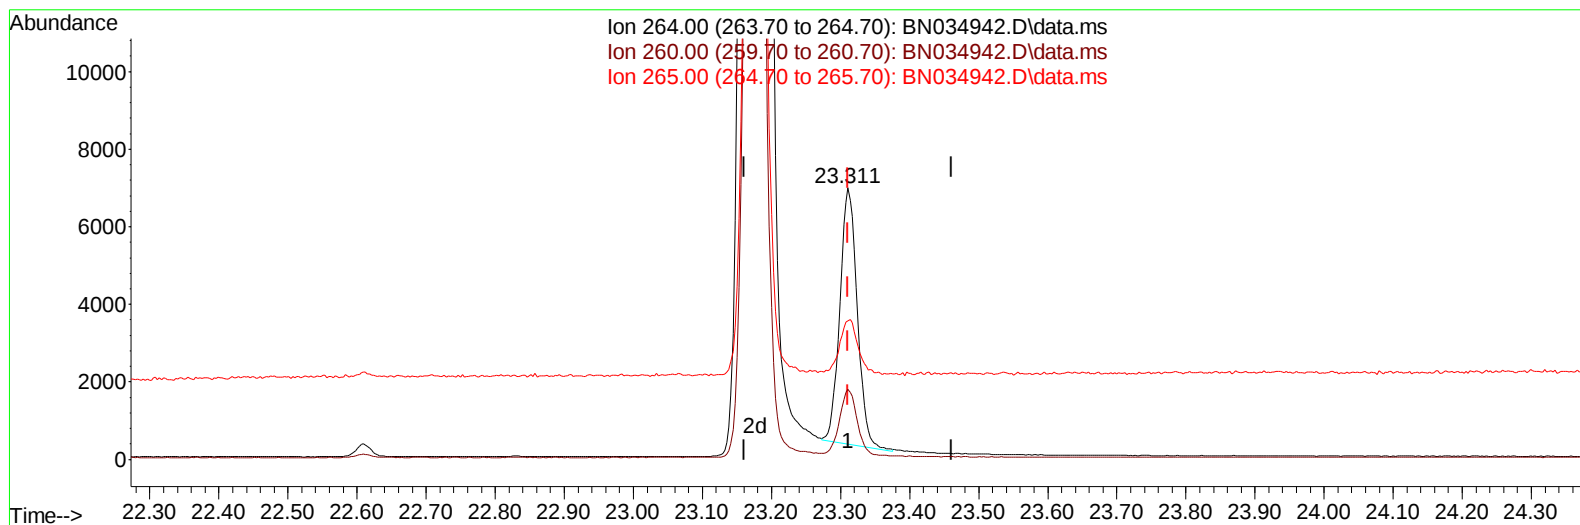

TIC: BN034942.D\data.ms

(23) Perylene-d12 (I)

23.311min (+ 0.000) 0.40 ng/ul m

response 11530

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	25.85
265.00	52.80	51.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034942.D
 Acq On : 09 Nov 2024 15:14
 Operator : RC/JU
 Sample : P4746-22DL 5X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP95DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

Quant Time: Nov 09 22:52:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.571	152		2405	0.400	ng/ul	0.00
4) Naphthalene-d8	10.333	136		6187	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.203	164		4866	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.949	188		11872	0.400	ng/ul	0.00
17) Chrysene-d12	21.145	240		11693	0.400	ng/ul	0.00
23) Perylene-d12	23.311	264		11530m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.149	96		4164	1.820	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.928	152		806	0.085	ng/ul	0.00
18) Fluoranthene-d10	18.981	212		2767	0.092	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.182	88		1828	0.729	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034942.D
Acq On : 09 Nov 2024 15:14
Operator : RC/JU
Sample : P4746-22DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP95DL

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:52:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024

