




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034949.D
Acq On : 09 Nov 2024 20:01
Operator : RC/JU
Sample : P4744-17
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP72

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:53:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024

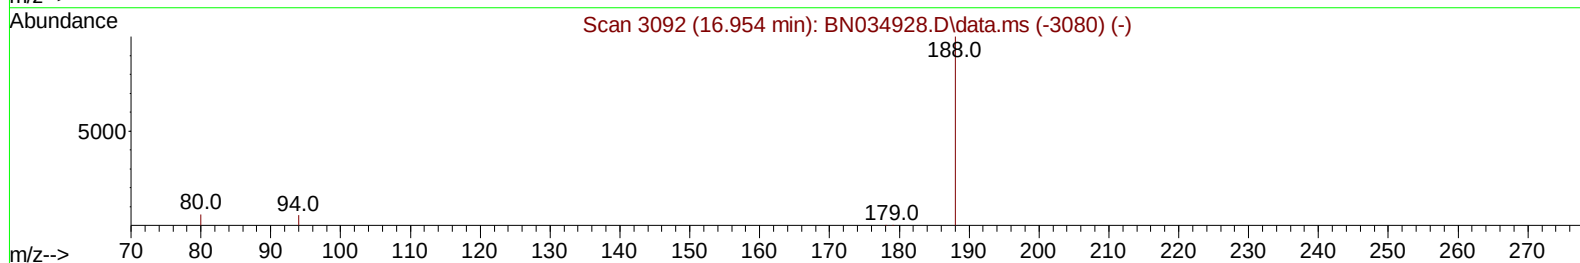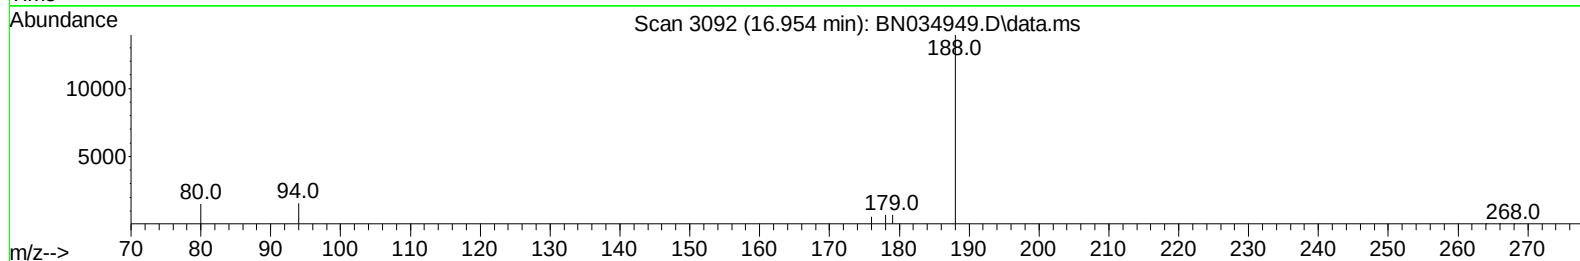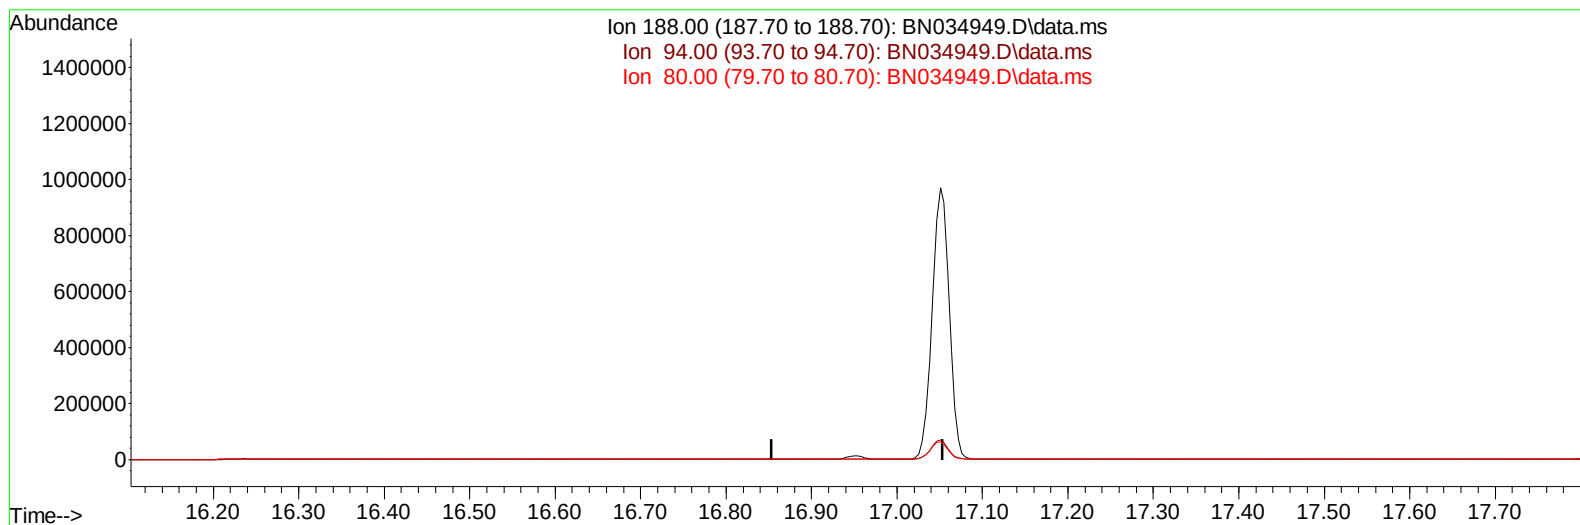

TIC: BN034949.D\data.ms

(13) Phenanthrene-d10 (I)

16.954min (-16.954) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.10	0.00#
80.00	7.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034949.D
Acq On : 09 Nov 2024 20:01
Operator : RC/JU
Sample : P4744-17
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP72

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:53:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024

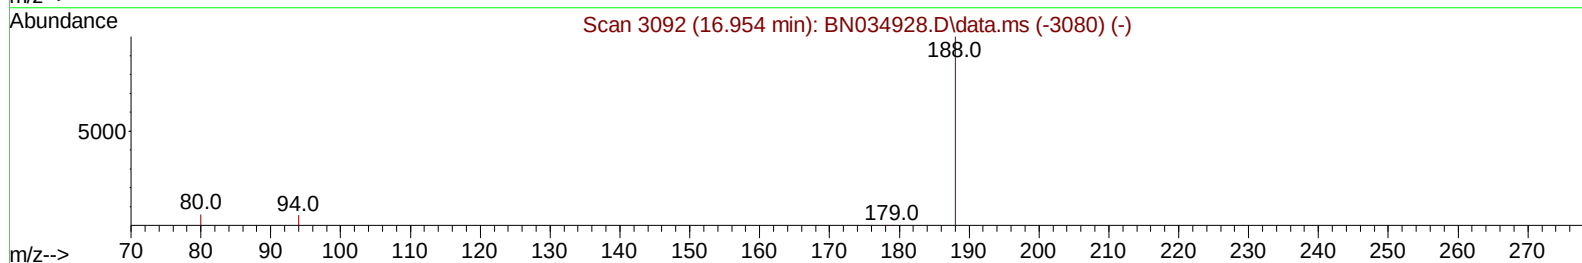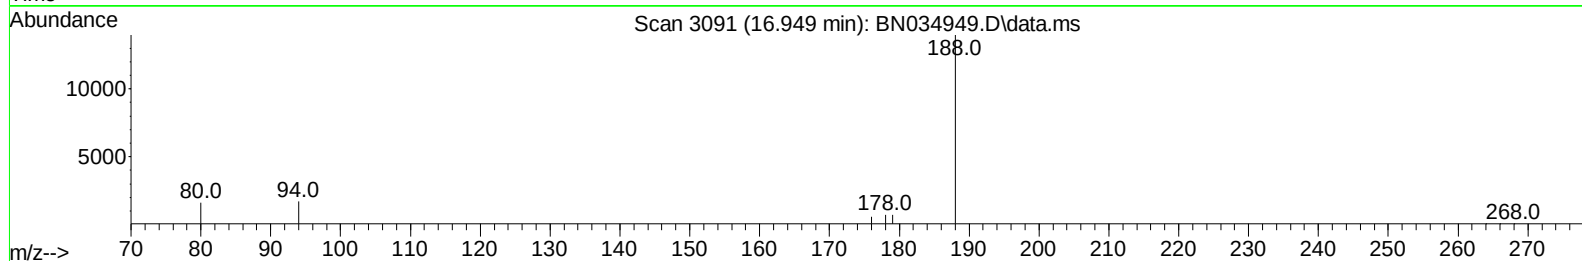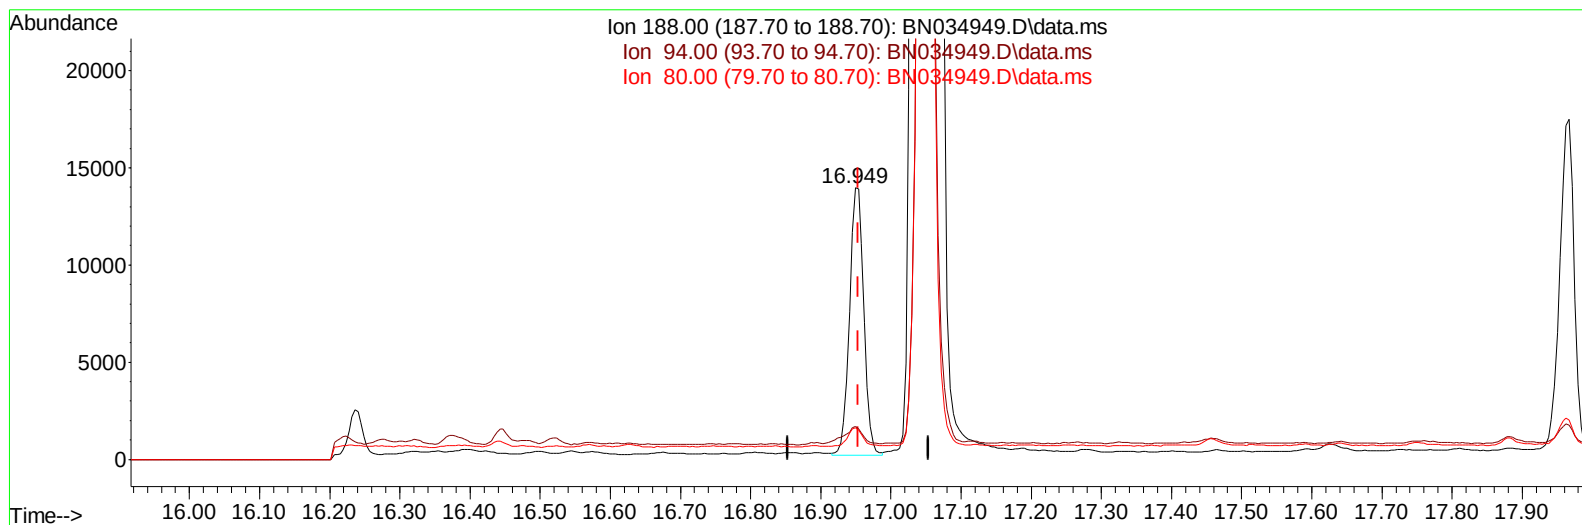

TIC: BN034949.D\data.ms

(13) Phenanthrene-d10 (I)

16.949min (-0.004) 0.40 ng/ul m

response 19339

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.10	12.12#
80.00	7.00	11.66#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034949.D
Acq On : 09 Nov 2024 20:01
Operator : RC/JU
Sample : P4744-17
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP72

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:53:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024

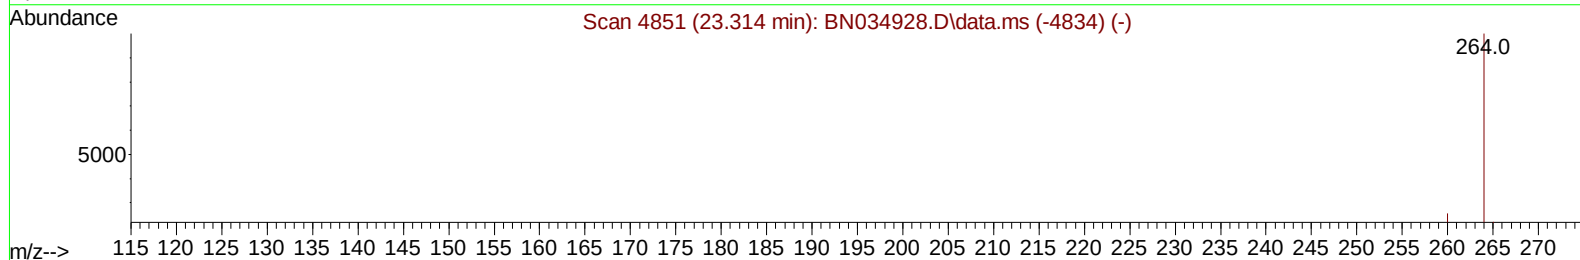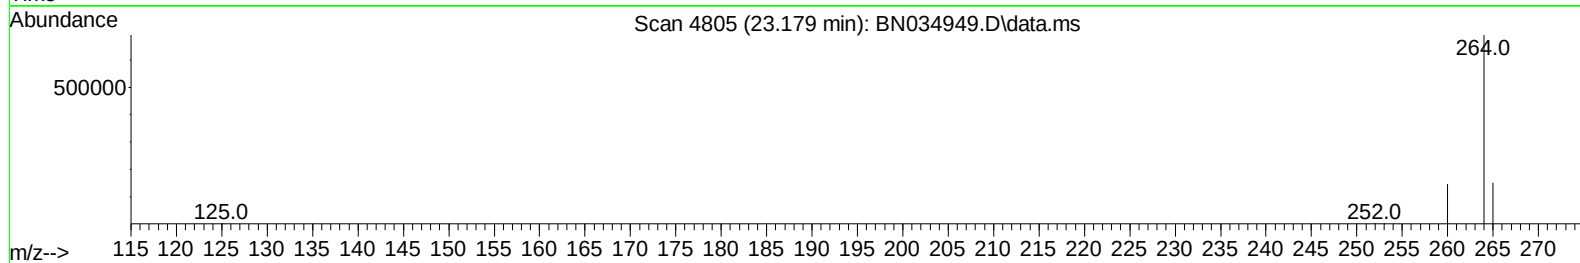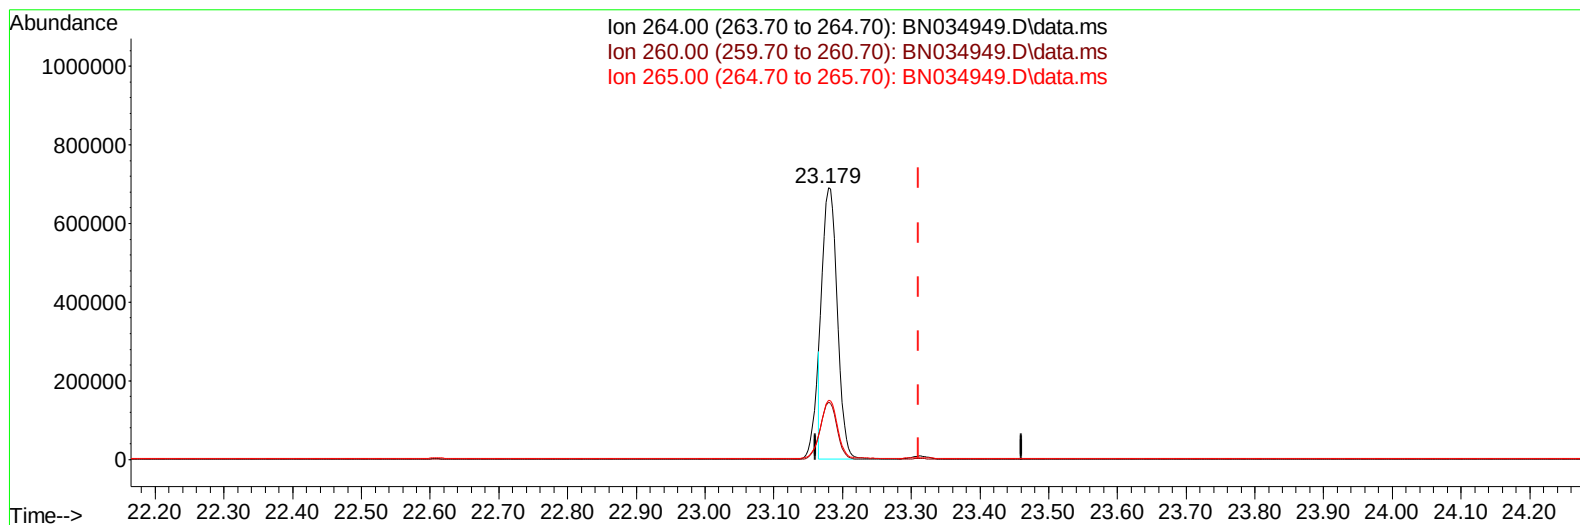

TIC: BN034949.D\data.ms

(23) Perylene-d12 (I)

23.179min (-0.132) 0.40 ng/u1

response 1049681

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	21.19
265.00	52.80	21.87#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034949.D
Acq On : 09 Nov 2024 20:01
Operator : RC/JU
Sample : P4744-17
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP72

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:53:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024

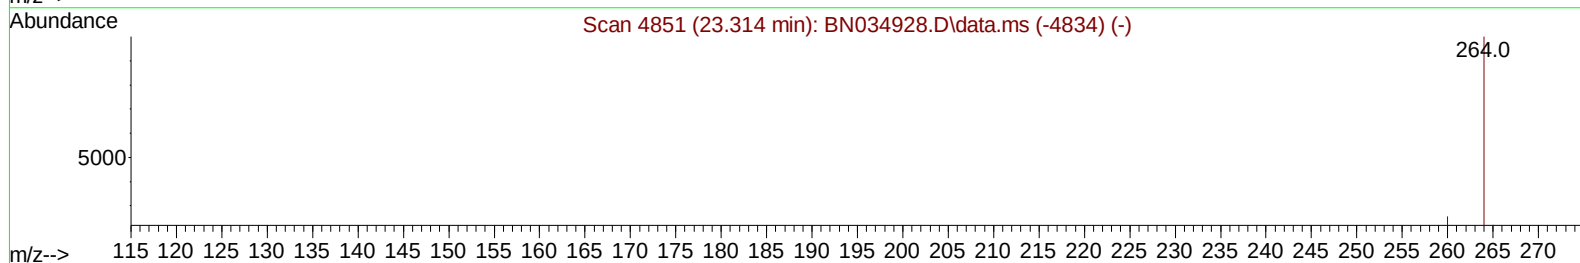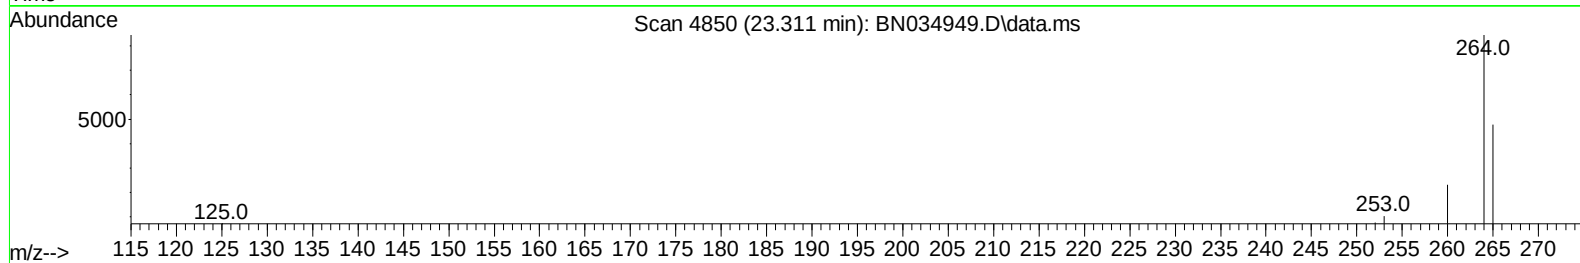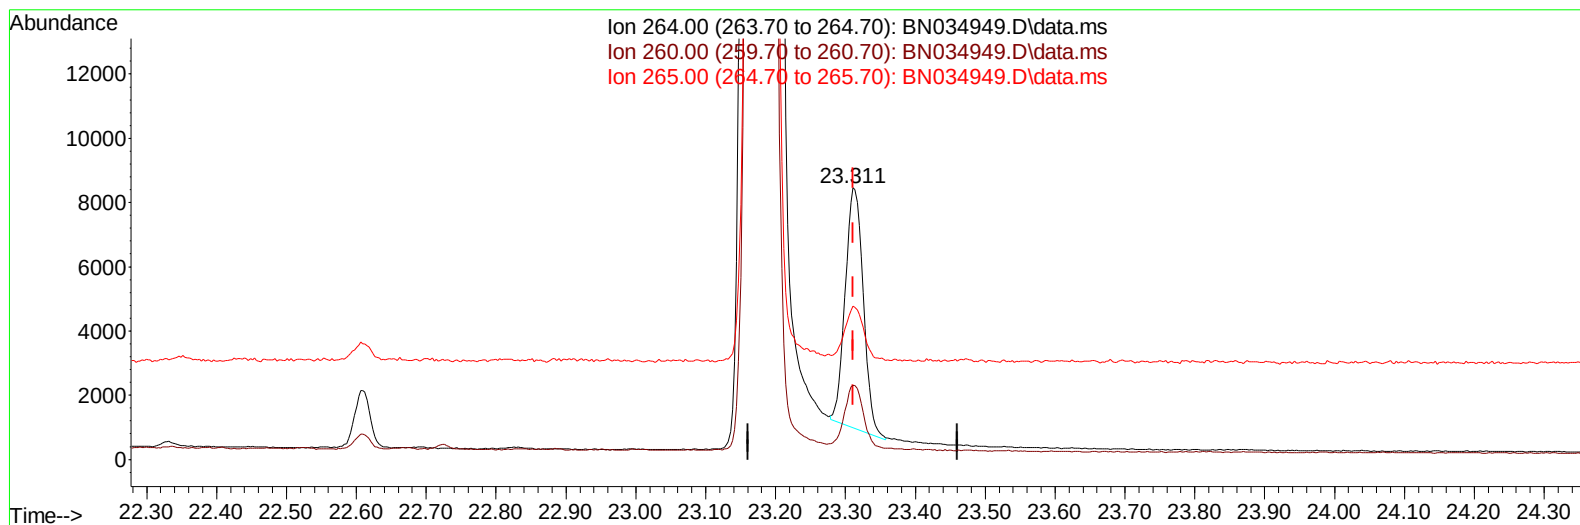

TIC: BN034949.D\data.ms

(23) Perylene-d12 (I)

23.311min (-0.000) 0.40 ng/ul m

response 13474

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	27.25
265.00	52.80	56.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034949.D
 Acq On : 09 Nov 2024 20:01
 Operator : RC/JU
 Sample : P4744-17
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP72

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

Quant Time: Nov 09 22:53:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.571	152	3308	0.400	ng/ul	0.00
4) Naphthalene-d8	10.333	136	8998	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.203	164	8220	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.949	188	19339m	0.400	ng/ul	0.00
17) Chrysene-d12	21.145	240	16887	0.400	ng/ul	# 0.00
23) Perylene-d12	23.311	264	13474m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	13035	4.141	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.928	152	5469	0.397	ng/ul	0.00
18) Fluoranthene-d10	18.981	212	22237	0.513	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034949.D
Acq On : 09 Nov 2024 20:01
Operator : RC/JU
Sample : P4744-17
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP72

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:53:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024

