




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110924\  
Data File : BN034986.D  
Acq On : 10 Nov 2024 19:18  
Operator : RC/JU  
Sample : P4744-16  
Misc :  
ALS Vial : 80 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
GCP71

Manual IntegrationsAPPROVED

Quant Time: Nov 10 21:53:22 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN110924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 09 00:09:12 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024  
Supervised By :mohammad ahmed 11/12/2024

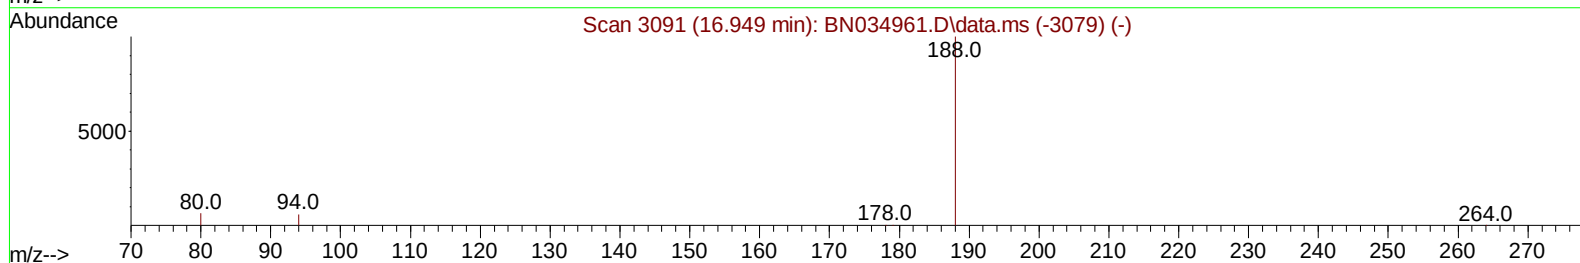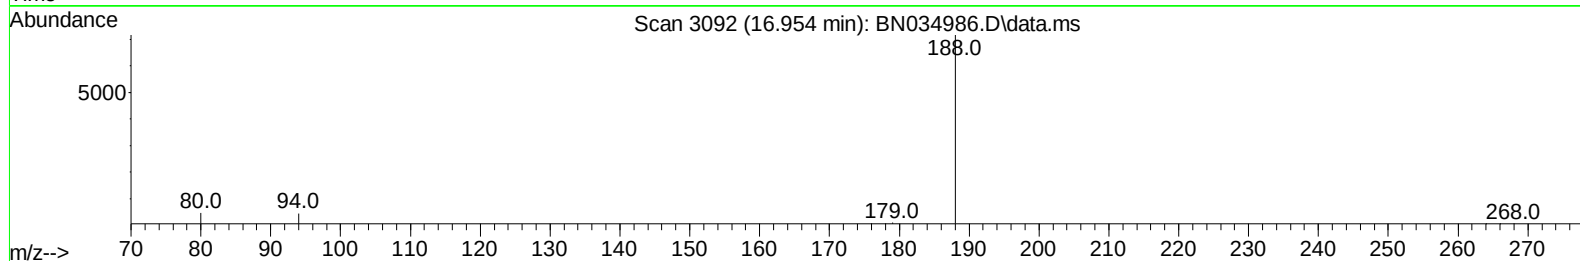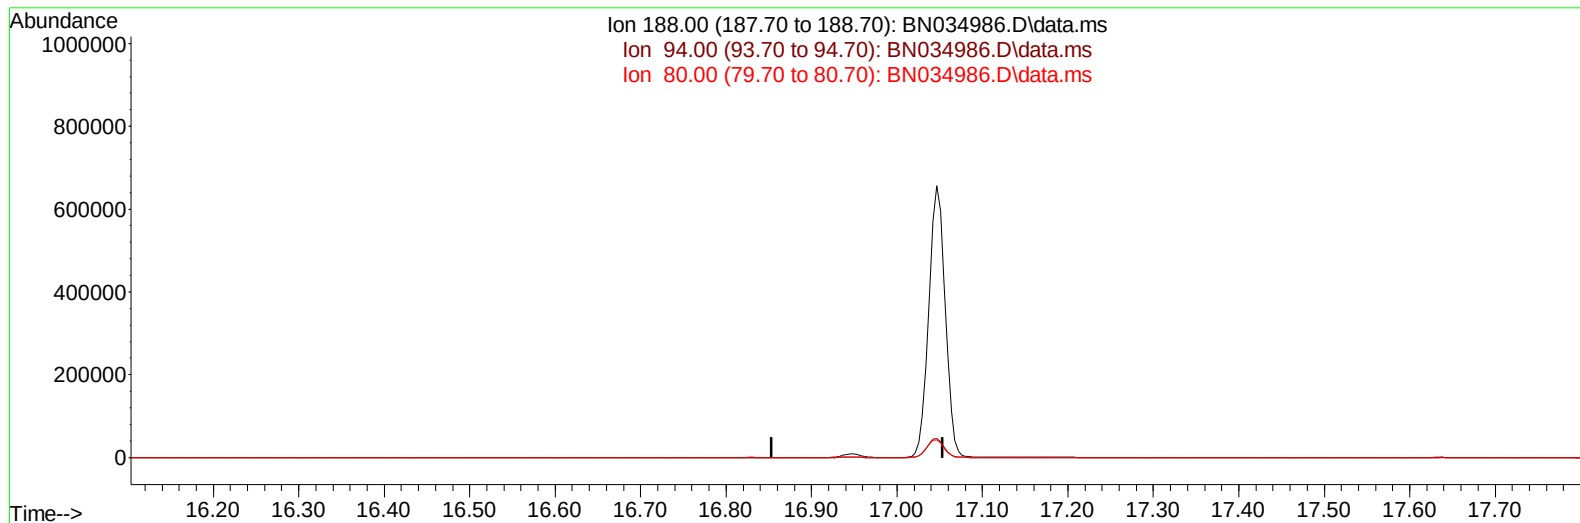

TIC: BN034986.D\data.ms

(13) Phenanthrene-d10 (I)

16.954min (-16.954) 0.00 ng/u1

response 0

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 188.00 | 100.00 | 0.00  |
| 94.00  | 6.10   | 0.00# |
| 80.00  | 7.00   | 0.00# |
| 0.00   | 0.00   | 0.00  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110924\  
Data File : BN034986.D  
Acq On : 10 Nov 2024 19:18  
Operator : RC/JU  
Sample : P4744-16  
Misc :  
ALS Vial : 80 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
GCP71

Manual IntegrationsAPPROVED

Quant Time: Nov 10 21:53:22 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN110924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 09 00:09:12 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024  
Supervised By :mohammad ahmed 11/12/2024

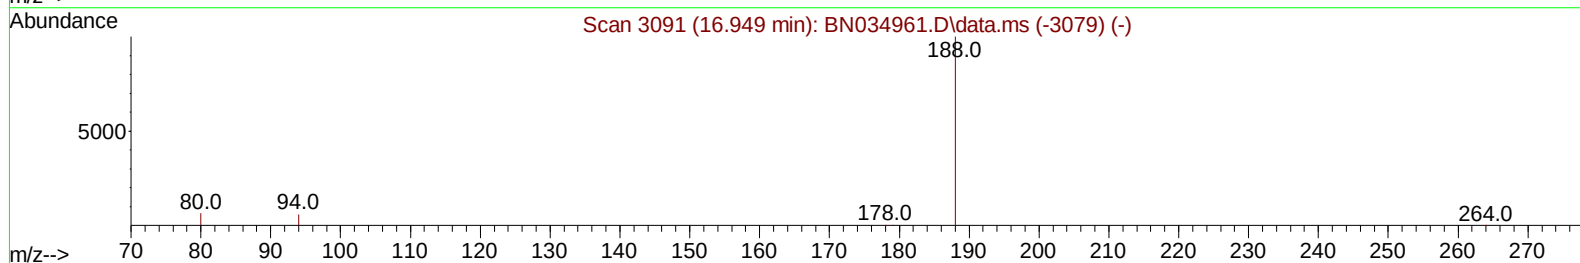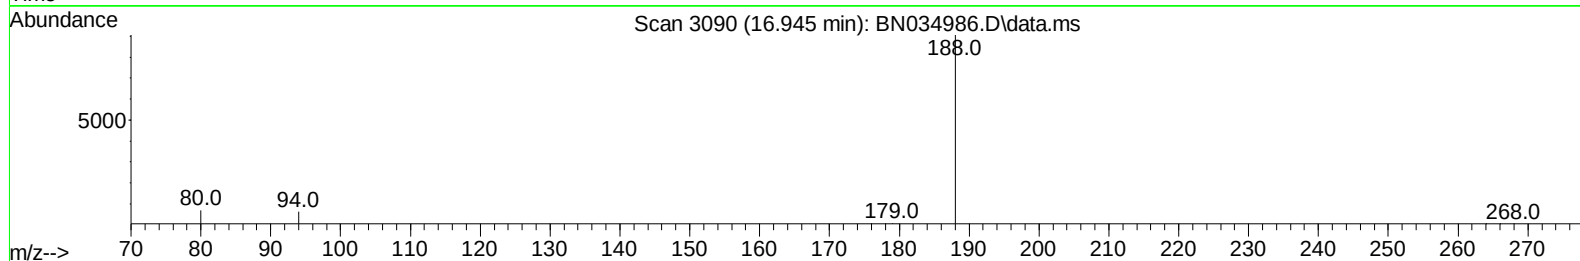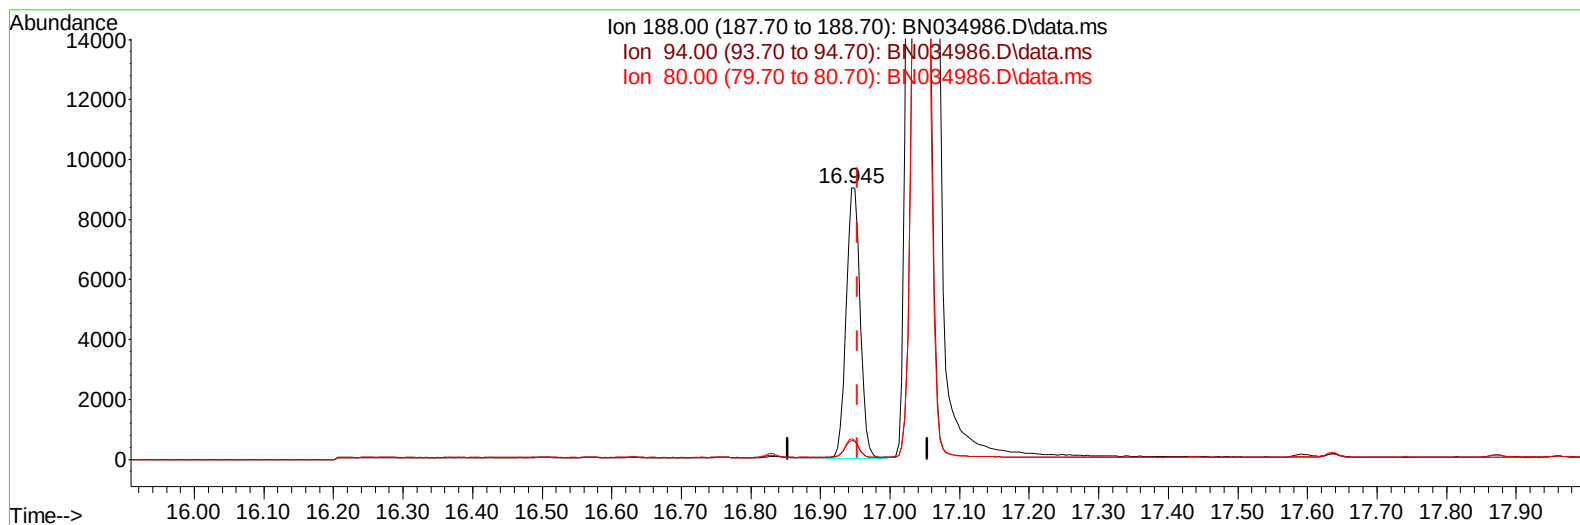

TIC: BN034986.D\data.ms

**(13) Phenanthrene-d10 (I)**

**16.945min (-0.008) 0.40 ng/ul m**

**response 12554**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 6.10   | 6.98   |
| 80.00  | 7.00   | 7.71   |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110924\  
Data File : BN034986.D  
Acq On : 10 Nov 2024 19:18  
Operator : RC/JU  
Sample : P4744-16  
Misc :  
ALS Vial : 80 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
GCP71

## Manual IntegrationsAPPROVED

Quant Time: Nov 10 21:53:22 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN110924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 09 00:09:12 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024  
Supervised By :mohammad ahmed 11/12/2024

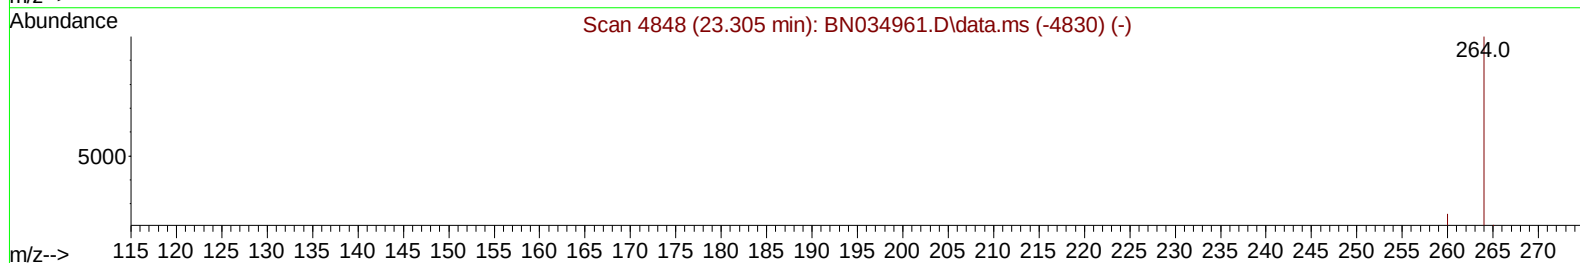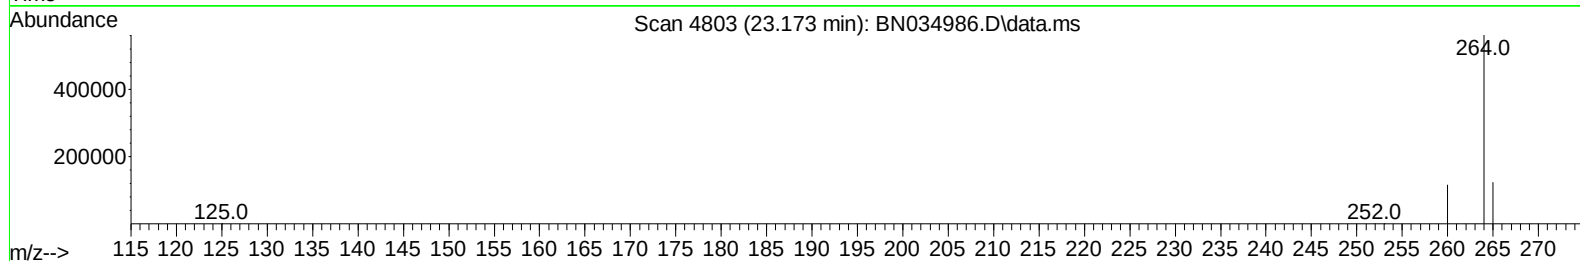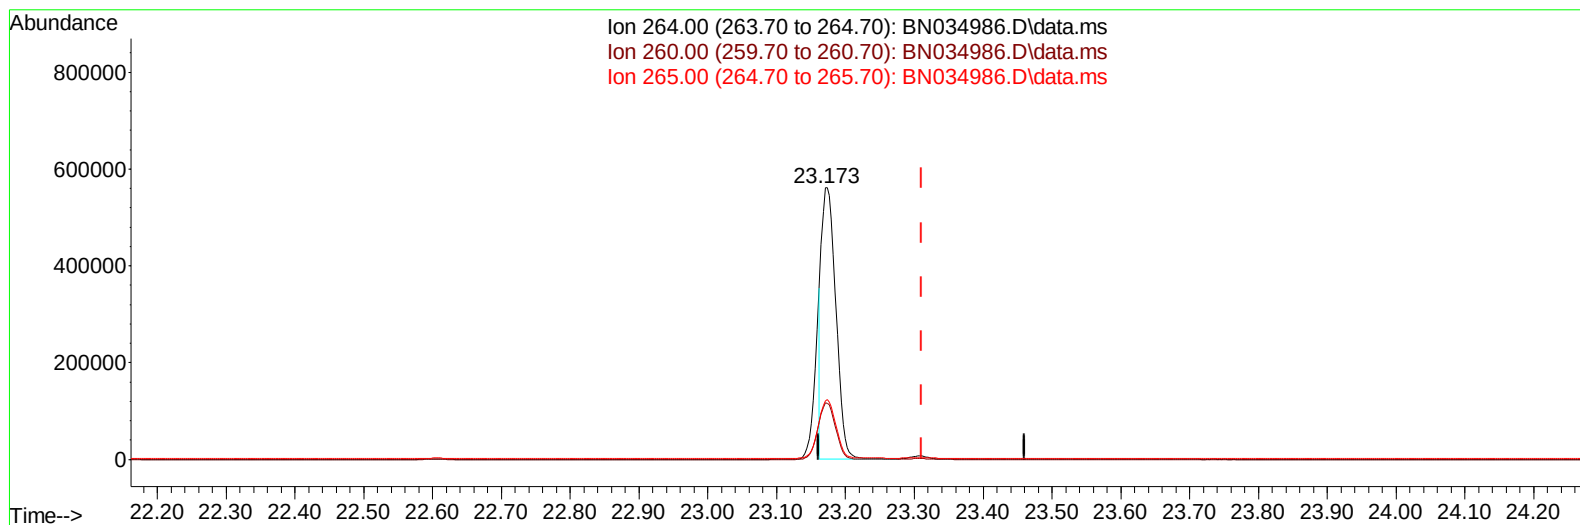

TIC: BN034986.D\data.ms

## (23) Perylene-d12 (I)

23.173min (-0.137) 0.40 ng/u1

response 811190

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 26.40  | 20.67# |
| 265.00 | 52.80  | 21.99# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110924\  
Data File : BN034986.D  
Acq On : 10 Nov 2024 19:18  
Operator : RC/JU  
Sample : P4744-16  
Misc :  
ALS Vial : 80 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
GCP71

Manual IntegrationsAPPROVED

Quant Time: Nov 10 21:53:22 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN110924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 09 00:09:12 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024  
Supervised By :mohammad ahmed 11/12/2024

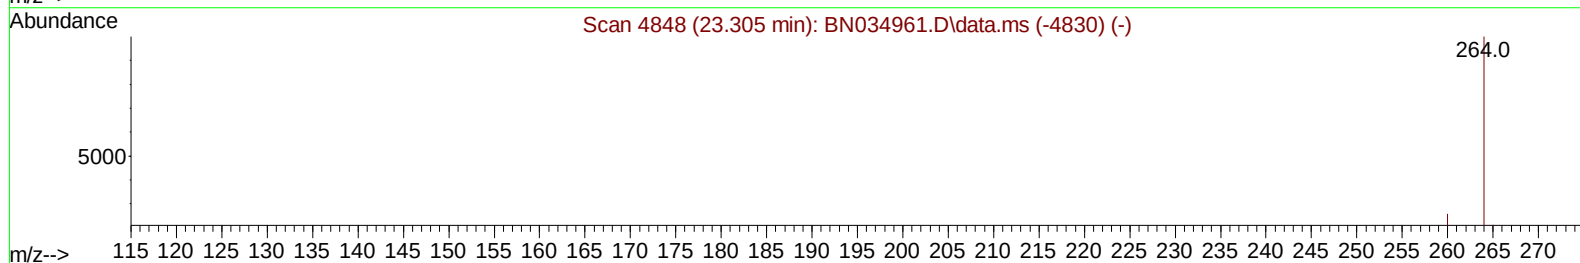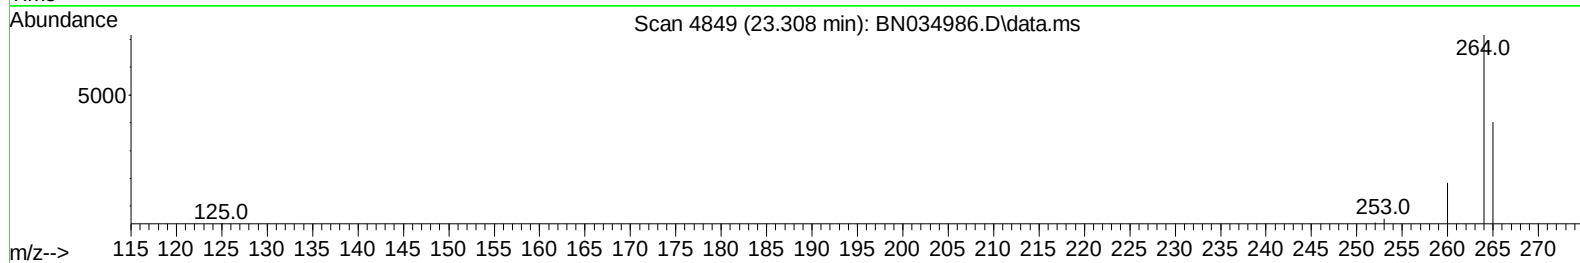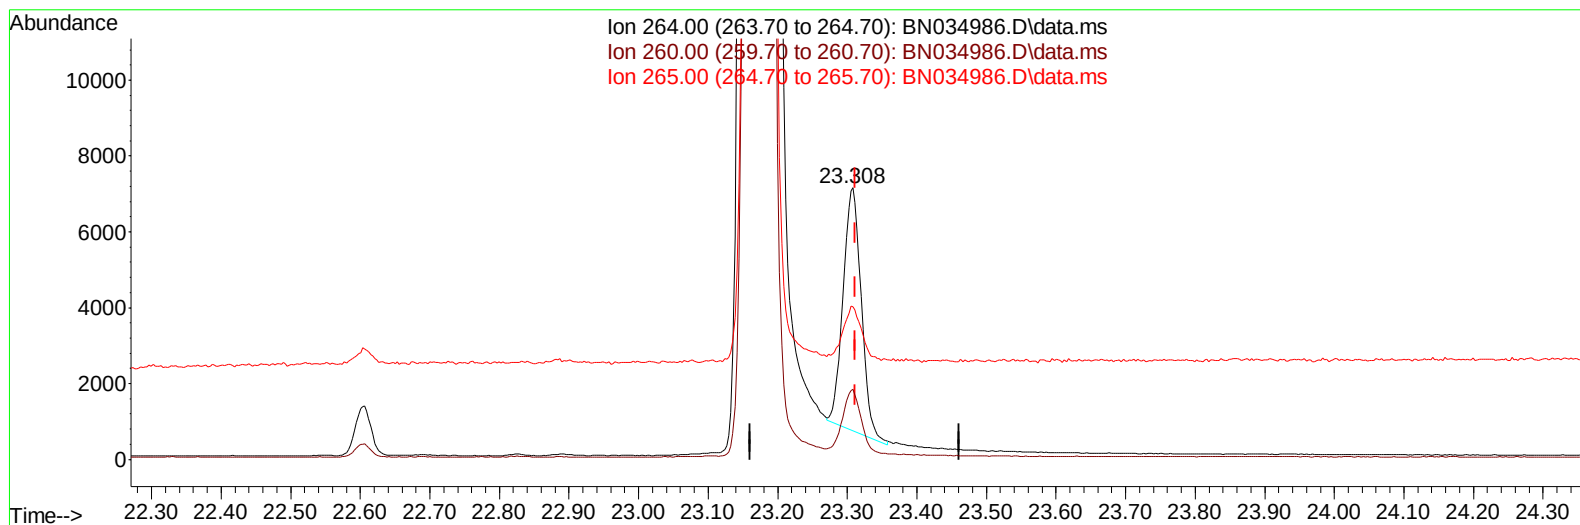

TIC: BN034986.D\data.ms

(23) Perylene-d12 (I)

23.308min (-0.003) 0.40 ng/ul m

response 11581

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 26.40  | 25.82  |
| 265.00 | 52.80  | 56.20  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110924\  
 Data File : BN034986.D  
 Acq On : 10 Nov 2024 19:18  
 Operator : RC/JU  
 Sample : P4744-16  
 Misc :  
 ALS Vial : 80 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 GCP71

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/10/2024  
 Supervised By :mohammad ahmed 11/12/2024

Quant Time: Nov 10 21:53:22 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN110924.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Nov 09 00:09:12 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | Q   | Ion | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|-----|-----|----------|-------|--------|----------|
| -----                       |        |     |     |          |       |        |          |
| Internal Standards          |        |     |     |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.566  | 152 |     | 3110     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.328 | 136 |     | 7657     | 0.400 | ng/ul  | -0.01    |
| 9) Acenaphthene-d10         | 14.199 | 164 |     | 5591     | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 16.945 | 188 |     | 12554m   | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.142 | 240 |     | 11579    | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.308 | 264 |     | 11581m   | 0.400 | ng/ul  | 0.00     |
|                             |        |     |     |          |       |        |          |
| System Monitoring Compounds |        |     |     |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.149  | 96  |     | 13200    | 4.461 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 11.923 | 152 |     | 3920     | 0.334 | ng/ul  | -0.01    |
| 18) Fluoranthene-d10        | 18.981 | 212 |     | 13162    | 0.443 | ng/ul  | 0.00     |
|                             |        |     |     |          |       |        |          |
| Target Compounds            |        |     |     |          |       |        | Qvalue   |
| 2) 1,4-Dioxane              | 3.182  | 88  |     | 314      | 0.097 | ng/ul# | 85       |
| -----                       |        |     |     |          |       |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110924\  
Data File : BN034986.D  
Acq On : 10 Nov 2024 19:18  
Operator : RC/JU  
Sample : P4744-16  
Misc :  
ALS Vial : 80 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
GCP71

Manual IntegrationsAPPROVED

Quant Time: Nov 10 21:53:22 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN110924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Nov 09 00:09:12 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024  
Supervised By :mohammad ahmed 11/12/2024

