

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034925.D
 Acq On : 09 Nov 2024 04:29
 Operator : RC/JU
 Sample : P4744-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP57

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

Quant Time: Nov 09 04:52:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.571	152	2486	0.400	ng/ul	0.00
4) Naphthalene-d8	10.339	136	6673	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.208	164	5352	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.954	188	13444m	0.400	ng/ul	0.00
17) Chrysene-d12	21.145	240	13612	0.400	ng/ul	0.00
23) Perylene-d12	23.314	264	13209m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	12166	5.143	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.934	152	3896	0.381	ng/ul	0.00
18) Fluoranthene-d10	18.986	212	16536	0.473	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.187	88	383	0.148	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034925.D
Acq On : 09 Nov 2024 04:29
Operator : RC/JU
Sample : P4744-03
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCP57

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024


Quant Time: Nov 09 04:52:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

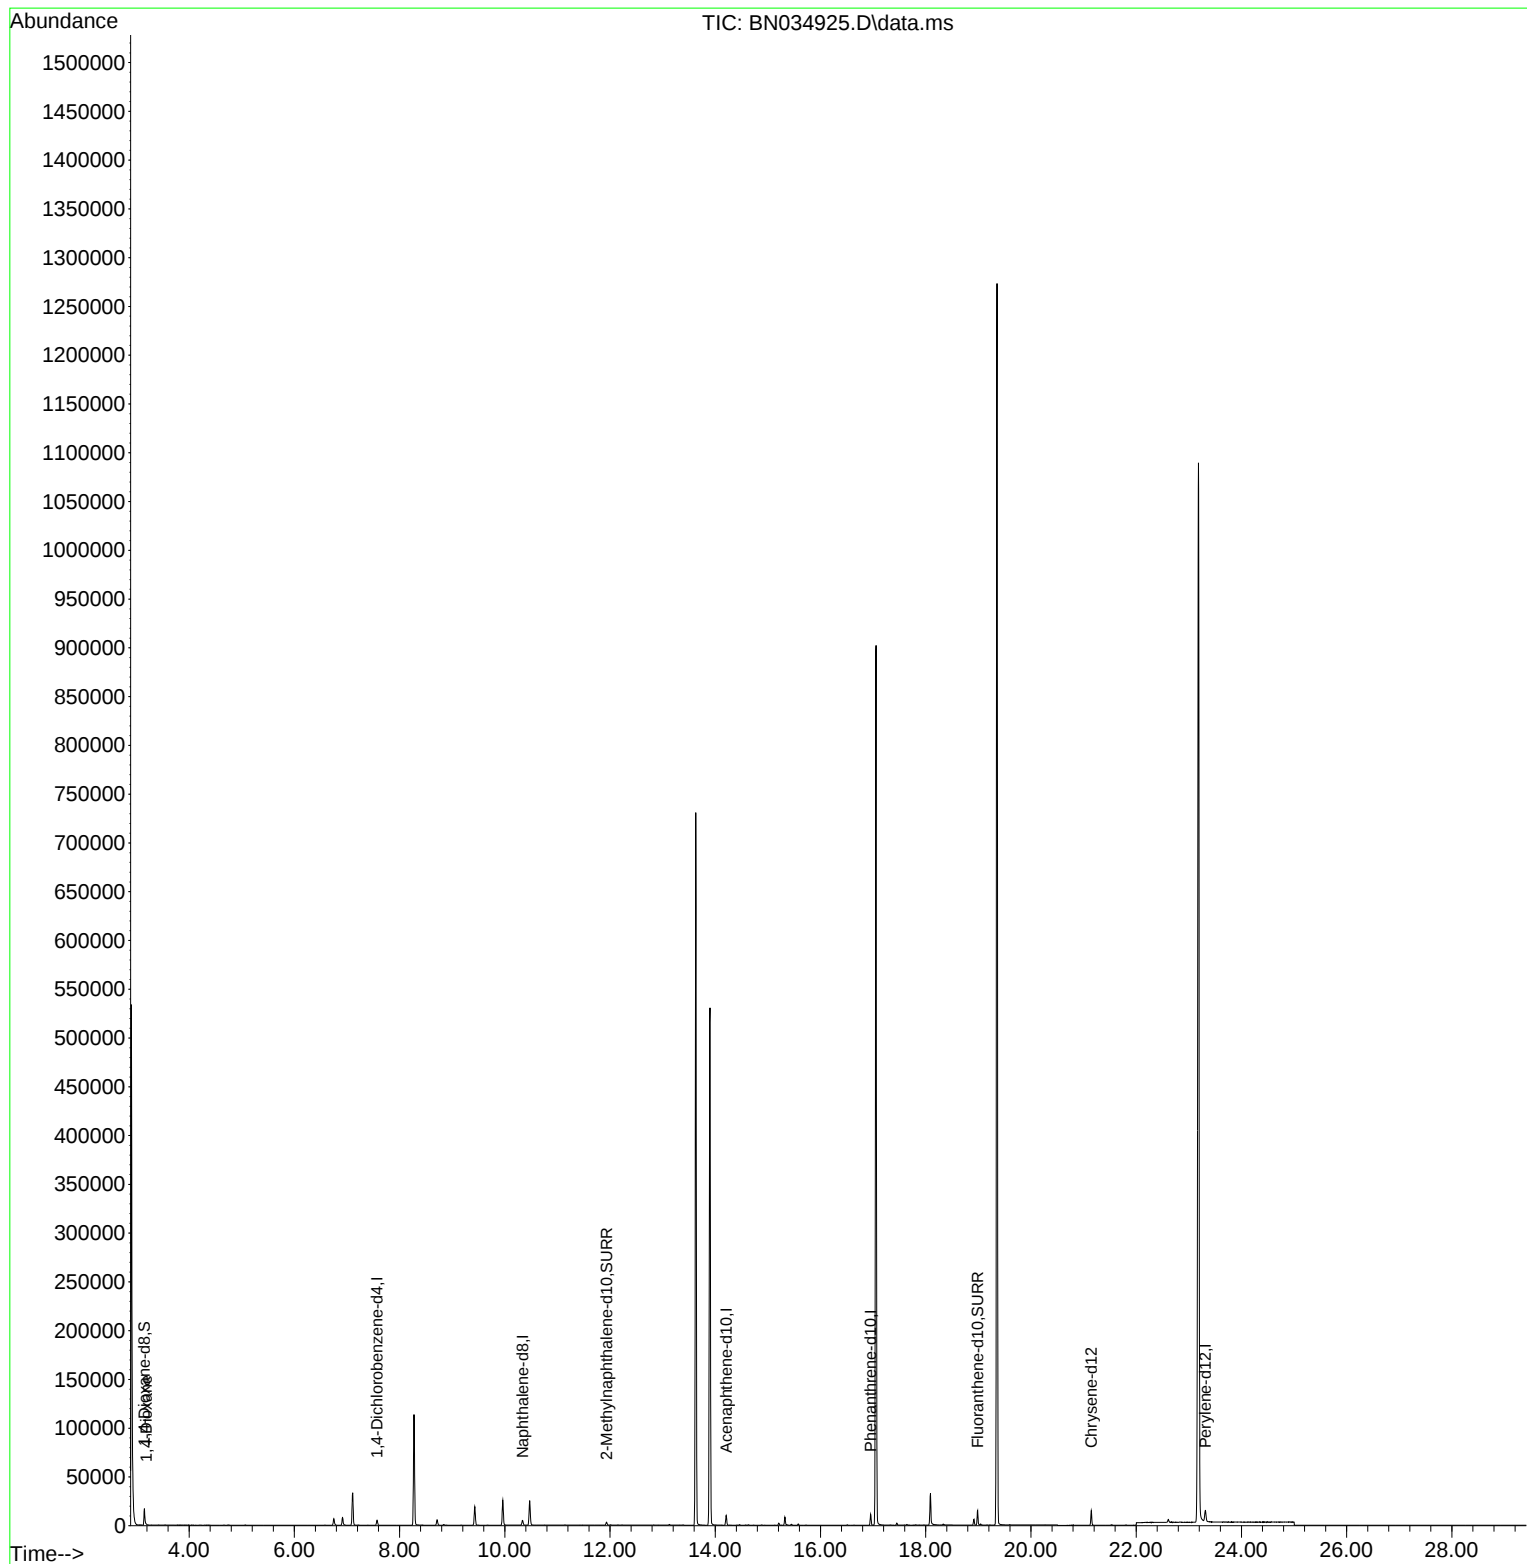

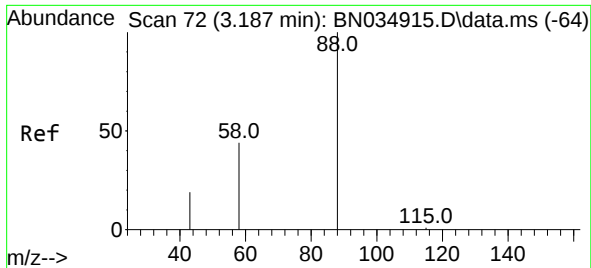

#2
 1,4-Dioxane
 Concen: 0.148 ng/ul
 RT: 3.187 min Scan# 72
 Delta R.T. 0.000 min
 Lab File: BN034925.D
 Acq: 09 Nov 2024 04:29

Instrument :
 BNA_N
 ClientSampleId :
 GCP57

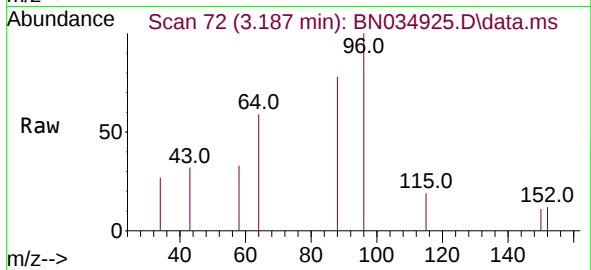

Tgt Ion: 88 Resp: 38
 Ion Ratio Lower Upper
 88 100
 43 41.1 23.3 53.2
 58 42.4 35.4 53.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

