

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034967.D
 Acq On : 10 Nov 2024 07:23
 Operator : RC/JU
 Sample : P4746-09MS
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP83MS

Quant Time: Nov 10 21:50:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.566	152	2663	0.400	ng/ul	0.00
4) Naphthalene-d8	10.328	136	6503	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.203	164	4592	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.949	188	10769	0.400	ng/ul	0.00
17) Chrysene-d12	21.142	240	10827	0.400	ng/ul	0.00
23) Perylene-d12	23.305	264	11594	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.153	96	643	0.254	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.928	152	3339	0.335	ng/ul	0.00
18) Fluoranthene-d10	18.981	212	12004	0.432	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.182	88	2033	0.732	ng/ul	95
5) Naphthalene	10.377	128	5641	0.347	ng/ul	99
7) 2-Methylnaphthalene	12.000	142	4057	0.334	ng/ul	99
8) 1-Methylnaphthalene	12.225	142	4090	0.335	ng/ul	100
10) Acenaphthylene	13.916	152	6587	0.351	ng/ul	99
11) Acenaphthene	14.263	153	5020	0.353	ng/ul	99
12) Fluorene	15.258	166	6290	0.348	ng/ul	98
14) Pentachlorophenol	16.603	266	2150	0.864	ng/ul	98
15) Phenanthrene	16.987	178	11073	0.385	ng/ul	99
16) Anthracene	17.080	178	10048	0.372	ng/ul	99
19) Fluoranthene	19.009	202	14484	0.400	ng/ul#	96
20) Pyrene	19.372	202	15031	0.401	ng/ul#	96
21) Benzo(a)anthracene	21.125	228	14845	0.379	ng/ul	99
22) Chrysene	21.177	228	15273	0.382	ng/ul	99
24) Benzo(b)fluoranthene	22.662	252	15285	0.375	ng/ul	97
25) Benzo(k)fluoranthene	22.706	252	16104	0.377	ng/ul	99
26) Benzo(a)pyrene	23.211	252	13479	0.370	ng/ul#	98
27) Indeno(1,2,3-cd)pyrene	25.456	276	18383	0.413	ng/ul	94
28) Dibenzo(a,h)anthracene	25.473	278	14452	0.416	ng/ul	99
29) Benzo(g,h,i)perylene	26.110	276	14238	0.418	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034967.D
Acq On : 10 Nov 2024 07:23
Operator : RC/JU
Sample : P4746-09MS
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCP83MS

Quant Time: Nov 10 21:50:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration




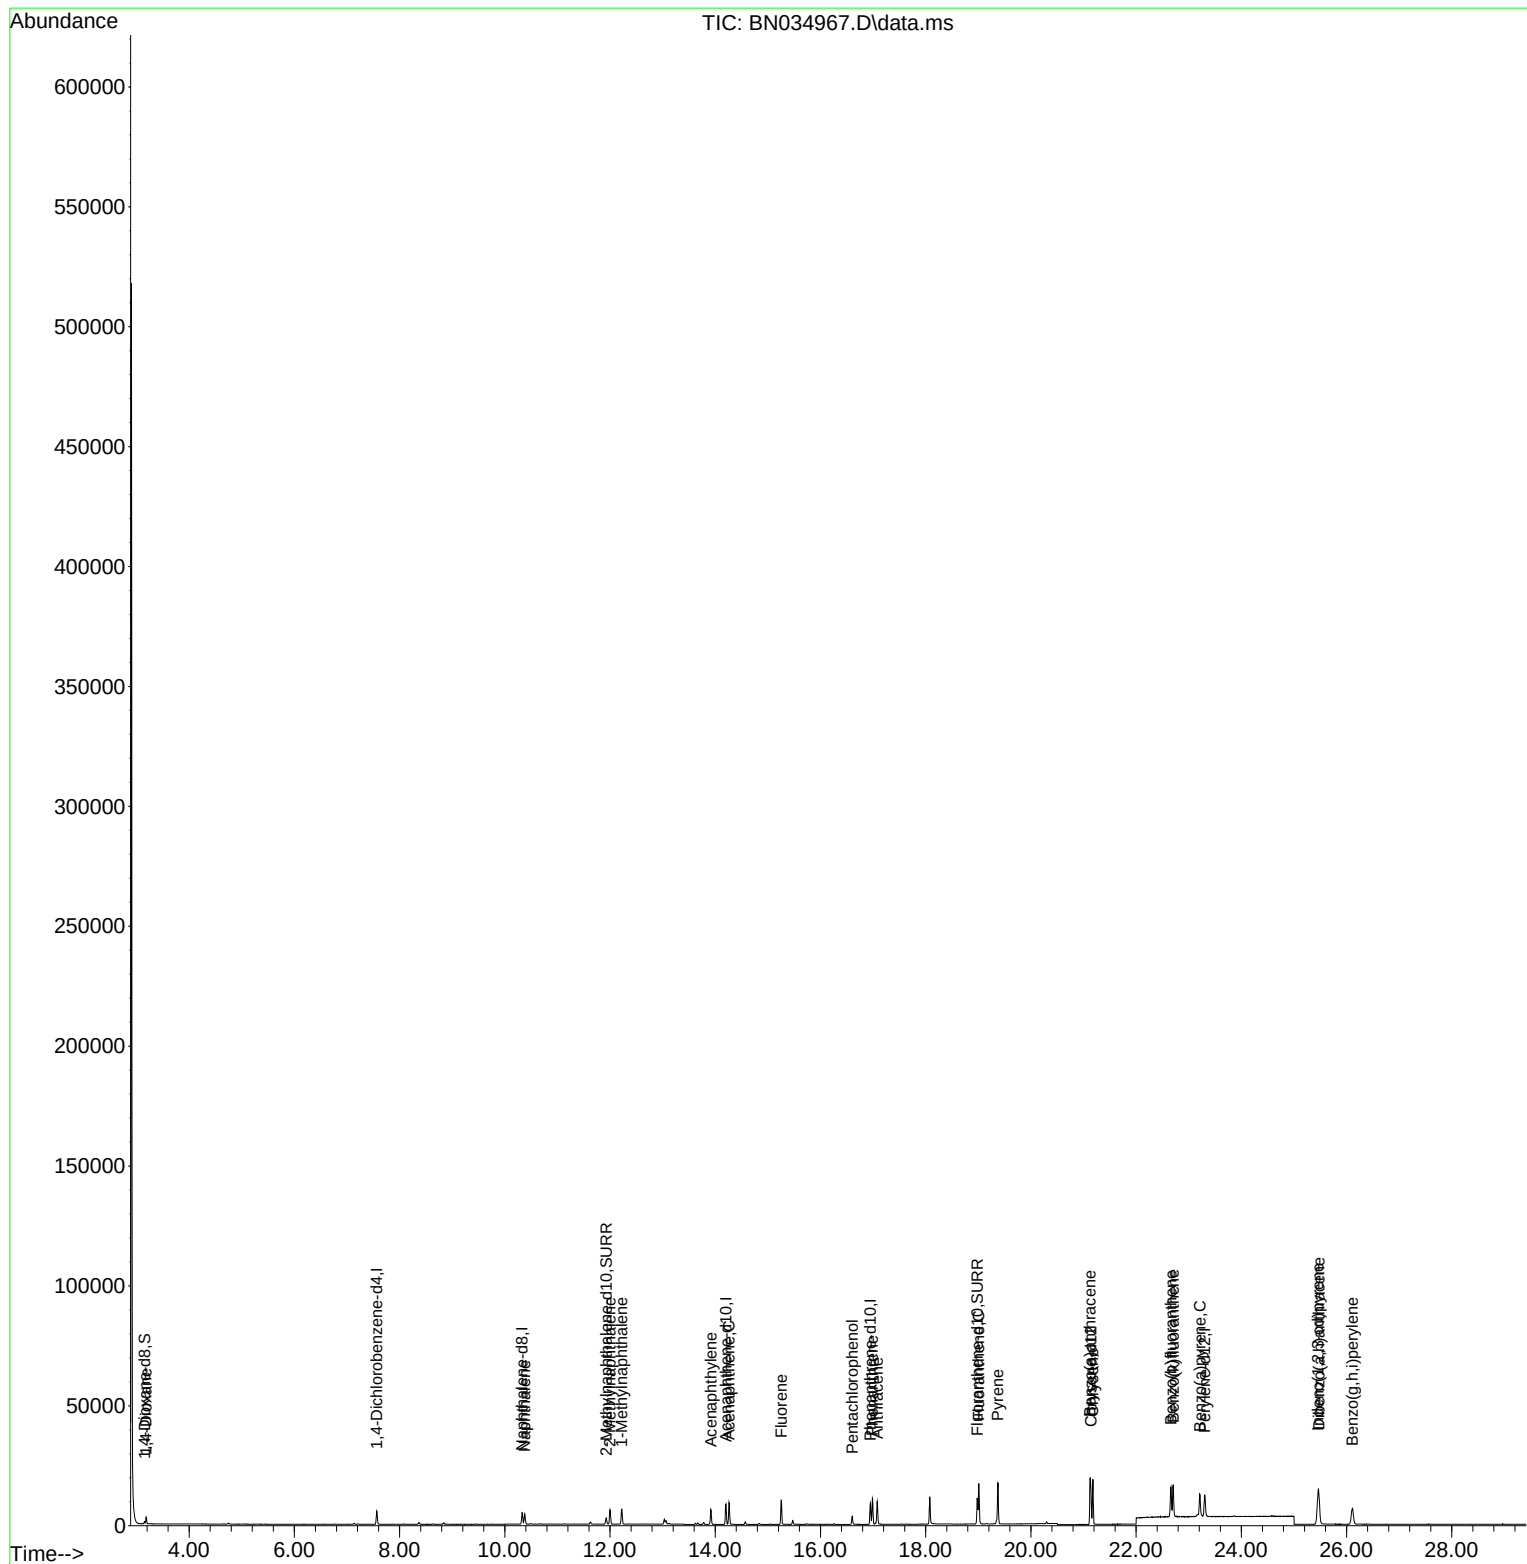


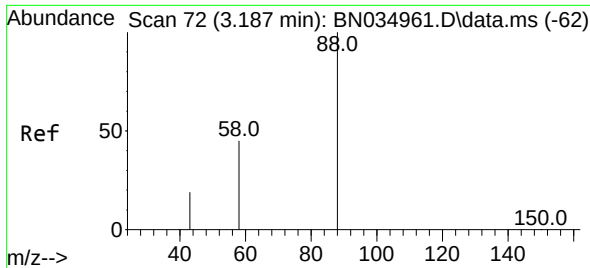

#2
 1,4-Dioxane
 Concen: 0.732 ng/ul
 RT: 3.182 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BN034967.D
 Acq: 10 Nov 2024 07:23




Instrument :
 BNA_N
 ClientSampleId :
 GCP83MS


Tgt Ion: 88	Resp: 2033
Ion Ratio	Lower Upper
88 100	
43 23.3	23.3 34.9
58 45.4	35.4 53.2

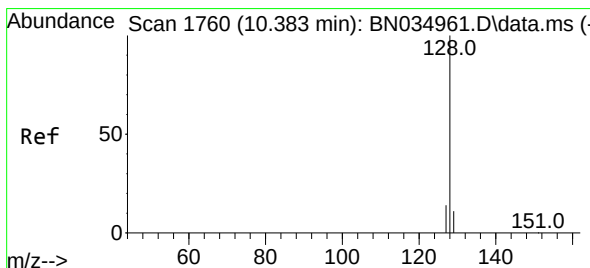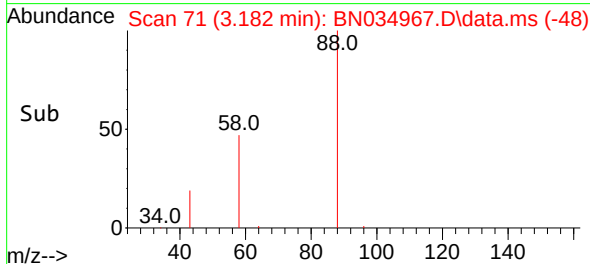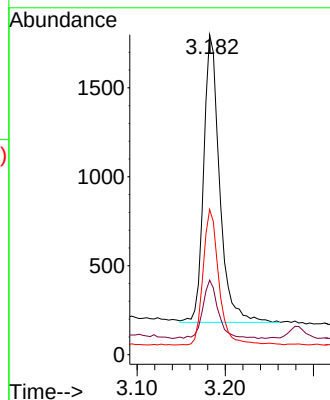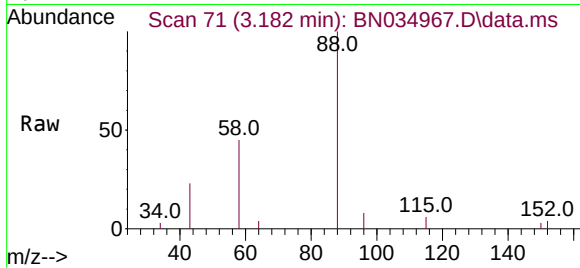

#5
 Naphthalene
 Concen: 0.347 ng/ul
 RT: 10.377 min Scan# 1759
 Delta R.T. -0.011 min
 Lab File: BN034967.D
 Acq: 10 Nov 2024 07:23

Tgt	Ion:128	Resp:	5641
Ion	Ratio	Lower	Upper
128	100		
129	12.4	10.1	15.1
127	14.5	12.1	18.1

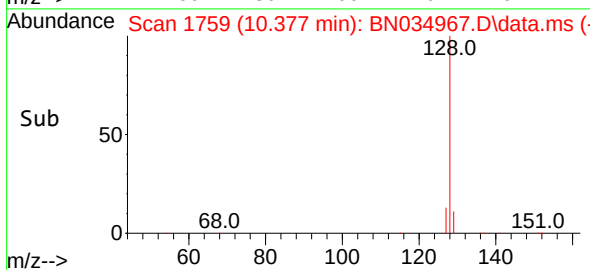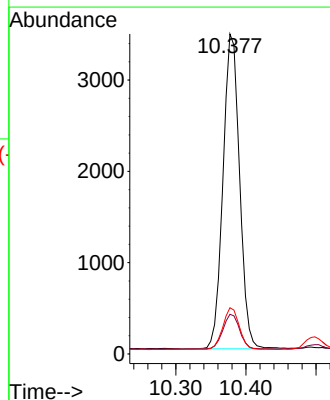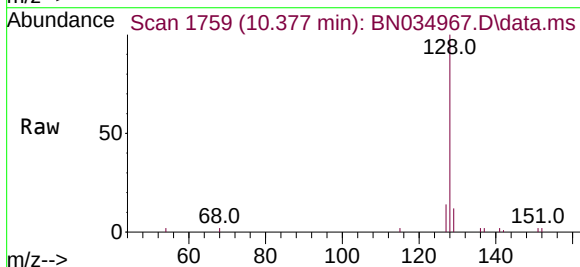



#7

2-Methylnaphthalene

Concen: 0.334 ng/ul

RT: 12.000 min Scan# 2054

Delta R.T. -0.011 min

Lab File: BN034967.D

Acq: 10 Nov 2024 07:23

Instrument :

BNA_N

ClientSampleId :





GCP83MS

Tgt Ion:142 Resp: 4057

Ion Ratio Lower Upper

142 100

141 89.3 70.8 106.2

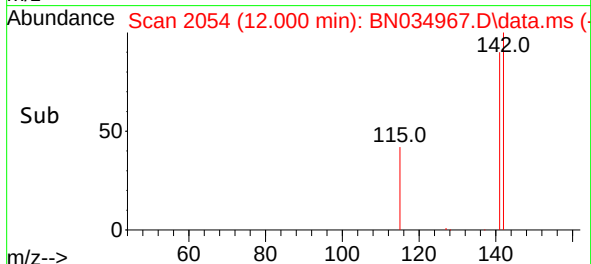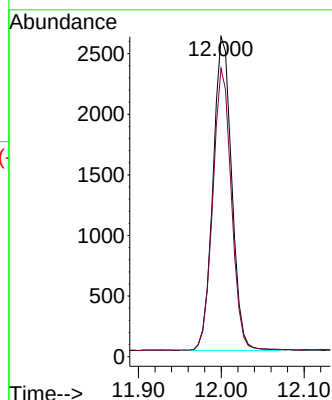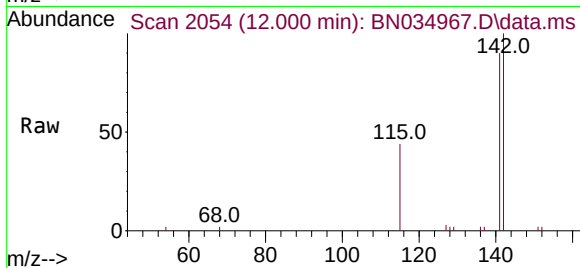

#8

1-Methylnaphthalene

Concen: 0.335 ng/ul

RT: 12.225 min Scan# 2095

Delta R.T. -0.006 min

Lab File: BN034967.D




Acq: 10 Nov 2024 07:23


Tgt Ion:142 Resp: 4090

Ion Ratio Lower Upper

142 100

141 93.0 74.6 111.8


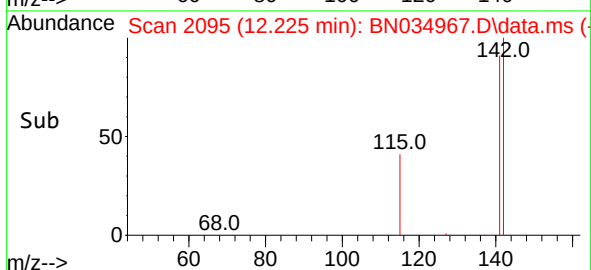
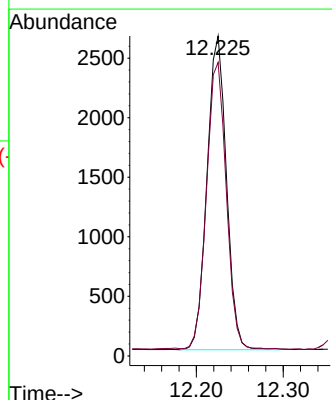
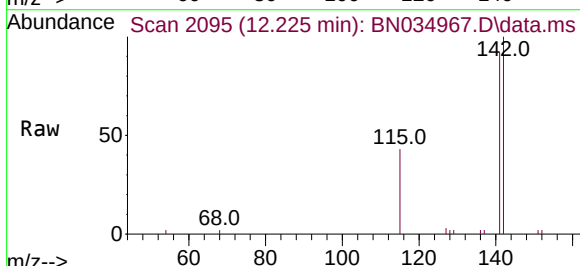


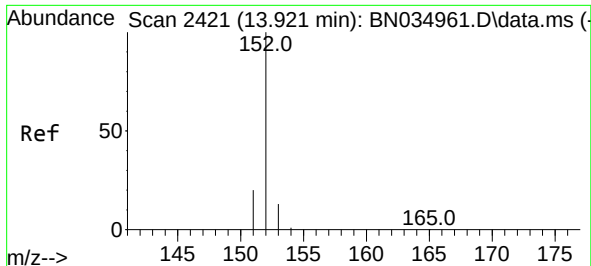

#10
Acenaphthylene
Concen: 0.351 ng/ul
RT: 13.916 min Scan# 2420
Delta R.T. -0.009 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23




Instrument :
BNA_N
ClientSampleId :
GCP83MS


Tgt Ion:152 Resp: 6587
Ion Ratio Lower Upper
152 100
151 21.3 16.6 24.8
153 14.4 11.0 16.6

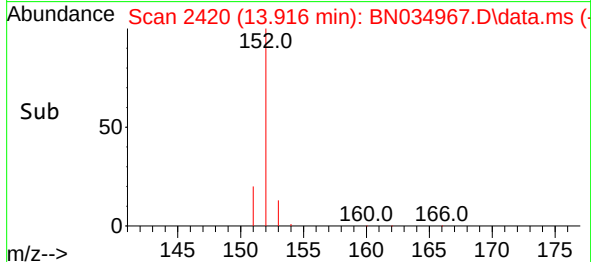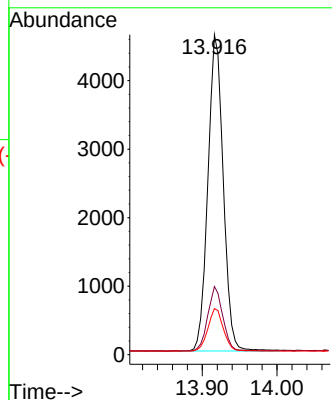

#11
Acenaphthene
Concen: 0.353 ng/ul
RT: 14.263 min Scan# 2495
Delta R.T. -0.009 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Tgt Ion:153 Resp: 5020
Ion Ratio Lower Upper
153 100
152 50.7 41.5 62.3
154 88.9 70.9 106.3


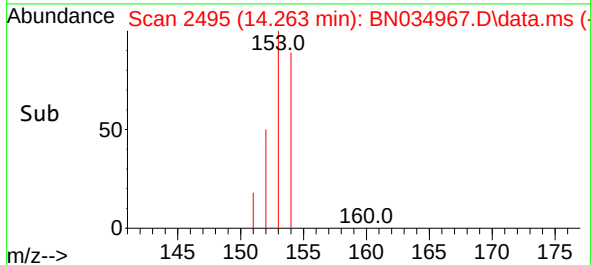
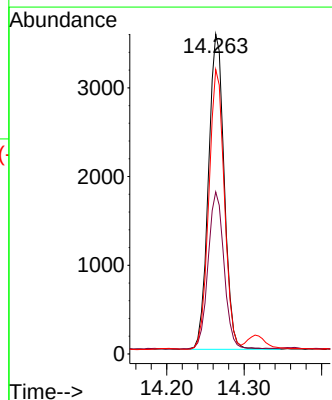
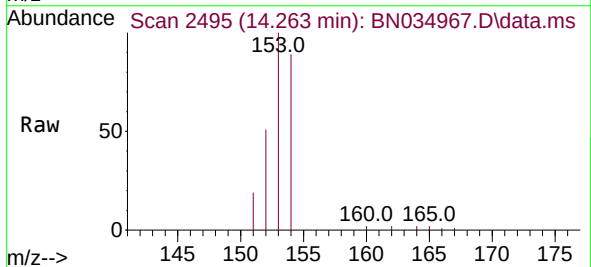


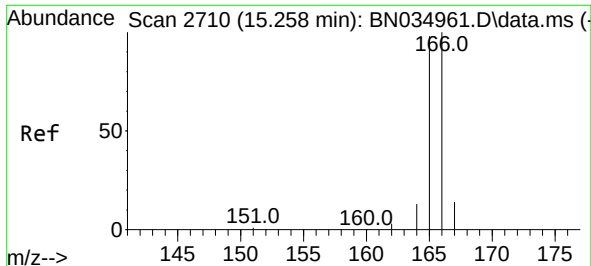

#12
Fluorene
Concen: 0.348 ng/ul
RT: 15.258 min Scan# 2710
Delta R.T. -0.005 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23




Instrument :
BNA_N
ClientSampleId :
GCP83MS


Tgt Ion:166 Resp: 6290
Ion Ratio Lower Upper
166 100
165 96.6 79.0 118.4
167 14.2 11.8 17.6

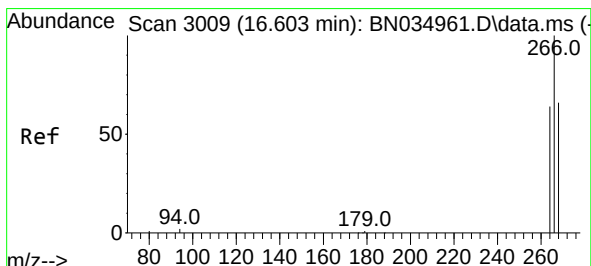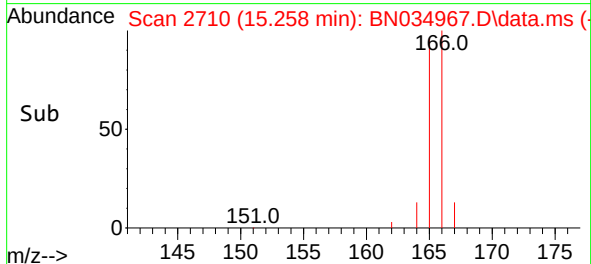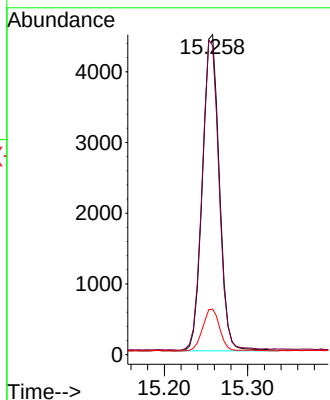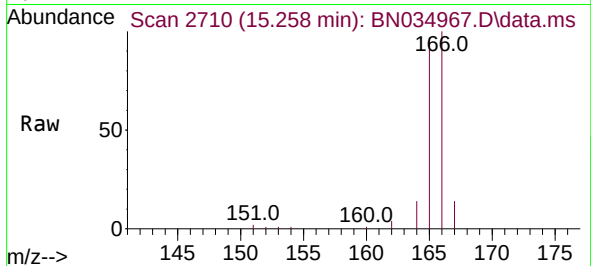

#14
Pentachlorophenol
Concen: 0.864 ng/ul
RT: 16.603 min Scan# 3009
Delta R.T. -0.004 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Tgt Ion:266 Resp: 2150
Ion Ratio Lower Upper
266 100
264 63.2 50.2 75.2
268 62.7 48.4 72.6


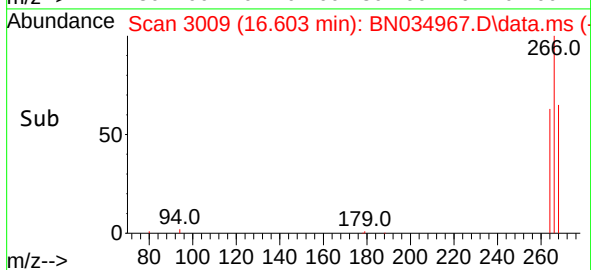
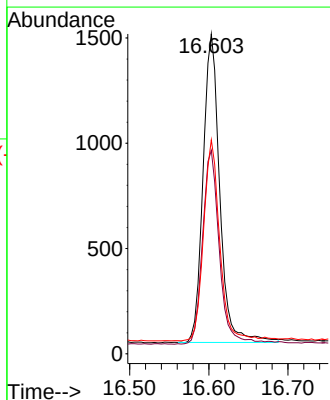
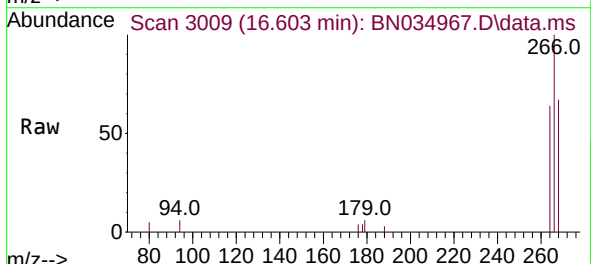


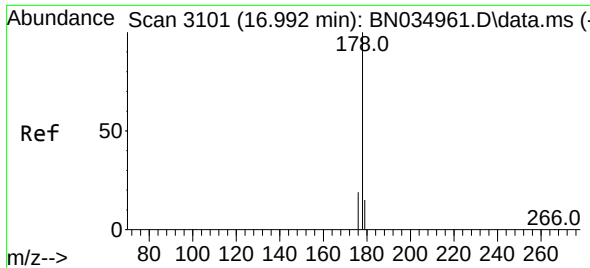

#15
Phenanthrene
Concen: 0.385 ng/ul
RT: 16.987 min Scan# 3100
Delta R.T. -0.009 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23




Instrument :
BNA_N
ClientSampleId :
GCP83MS


Tgt Ion:	178	Resp:	11073
Ion	Ratio	Lower	Upper
178	100		
179	16.0	13.4	20.2
176	20.0	15.8	23.6

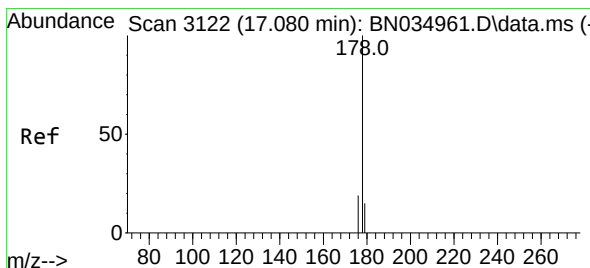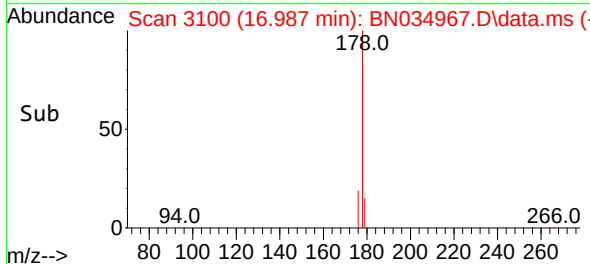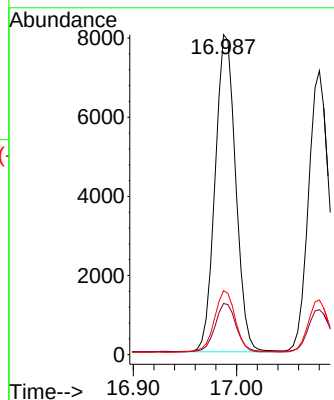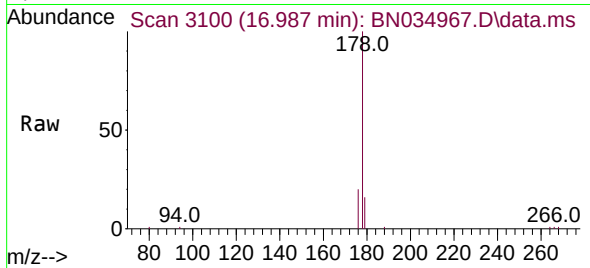

#16
Anthracene
Concen: 0.372 ng/ul
RT: 17.080 min Scan# 3122
Delta R.T. -0.004 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Tgt Ion:	178	Resp:	10048
Ion	Ratio	Lower	Upper
178	100		
179	15.8	13.3	19.9
176	19.3	15.8	23.8


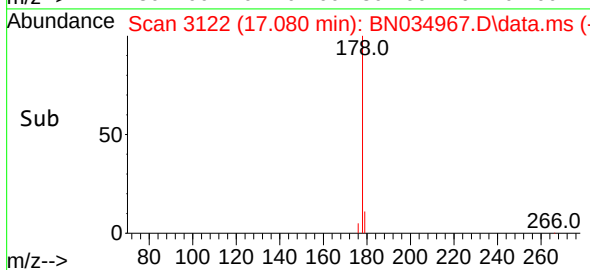
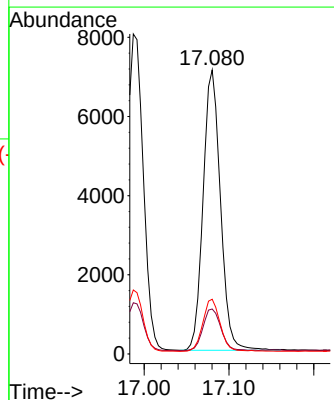
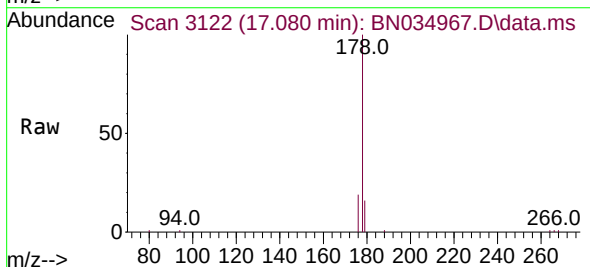


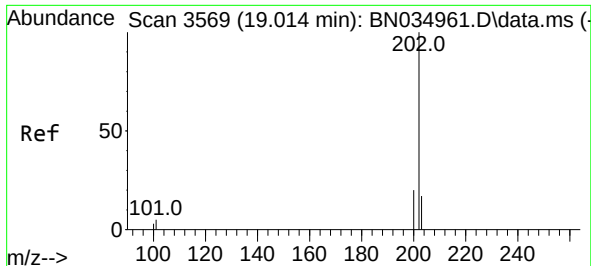

#19
Fluoranthene
Concen: 0.400 ng/u1
RT: 19.009 min Scan# 3568
Delta R.T. -0.009 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23




Instrument :
BNA_N
ClientSampleId :
GCP83MS


Tgt Ion:202 Resp: 14484
Ion Ratio Lower Upper
202 100
101 6.7 4.2 6.2#
100 5.2 3.2 4.8#

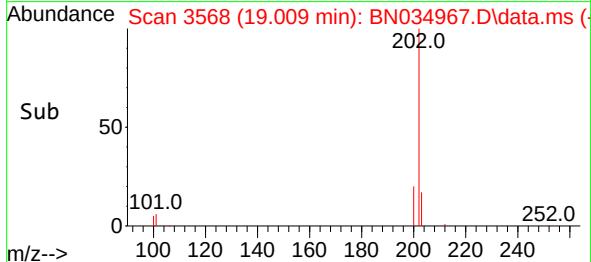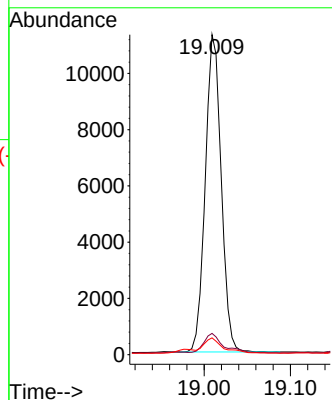

#20
Pyrene
Concen: 0.401 ng/u1
RT: 19.372 min Scan# 3646
Delta R.T. -0.009 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Tgt Ion:202 Resp: 15031
Ion Ratio Lower Upper
202 100
101 7.8 5.0 7.4#
100 6.3 4.1 6.1#


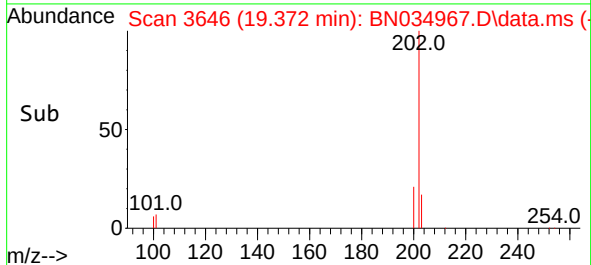
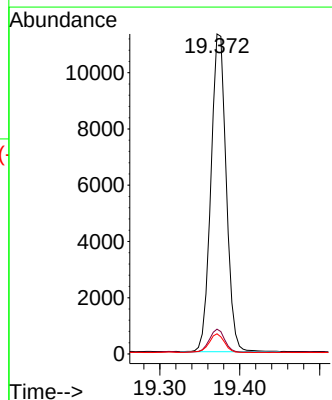
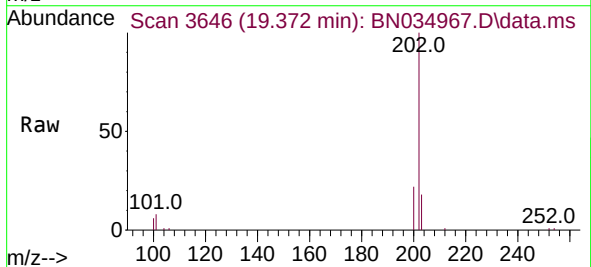


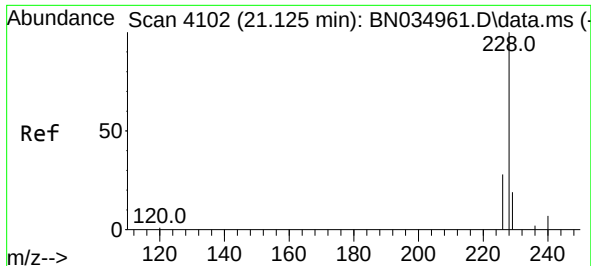

#21
Benzo(a)anthracene
Concen: 0.379 ng/ul
RT: 21.125 min Scan# 4102
Delta R.T. -0.006 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23




Instrument :
BNA_N
ClientSampleId :
GCP83MS


Tgt Ion:228 Resp: 14845
Ion Ratio Lower Upper
228 100
229 19.5 15.8 23.8
226 27.5 22.2 33.2

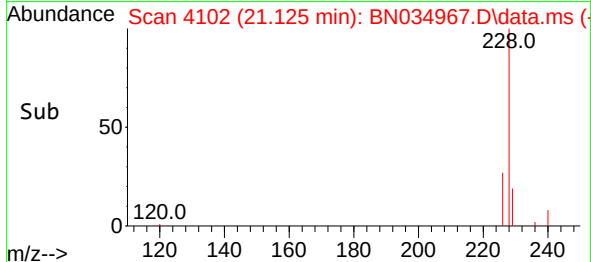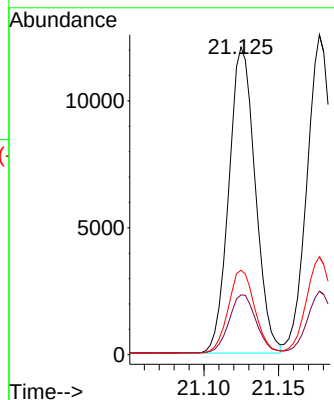

#22
Chrysene
Concen: 0.382 ng/ul
RT: 21.177 min Scan# 4120
Delta R.T. -0.006 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23


Tgt Ion:228 Resp: 15273
Ion Ratio Lower Upper
228 100
226 30.6 24.2 36.4
229 19.9 15.4 23.2

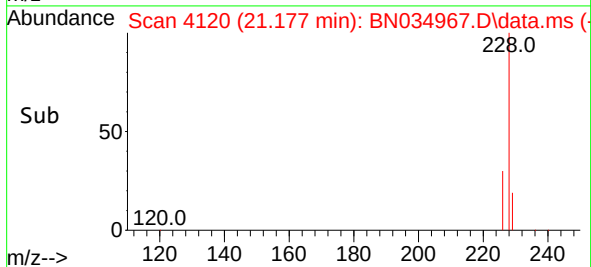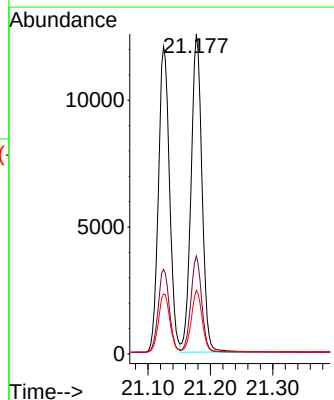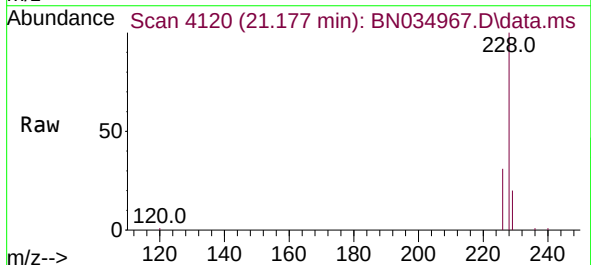


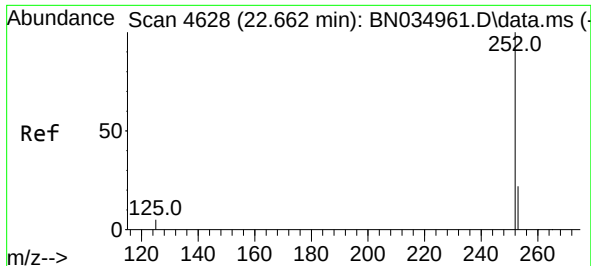


#24
Benzo(b)fluoranthene
Concen: 0.375 ng/ul
RT: 22.662 min Scan# 4628
Delta R.T. -0.009 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Instrument :
BNA_N
ClientSampleId :
GCP83MS







Tgt Ion:252 Resp: 15285
Ion Ratio Lower Upper
252 100
253 26.1 0.0 50.0
125 8.8 0.0 14.0

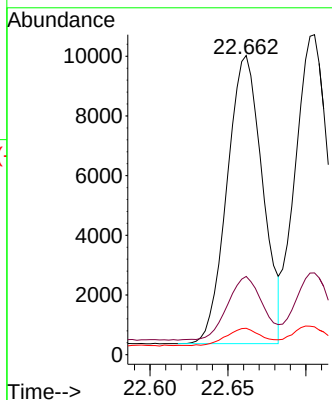

#25
Benzo(k)fluoranthene
Concen: 0.377 ng/ul
RT: 22.706 min Scan# 4643
Delta R.T. -0.006 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Tgt Ion:252 Resp: 16104
Ion Ratio Lower Upper
252 100
253 25.5 20.2 30.4
125 8.7 5.8 8.8


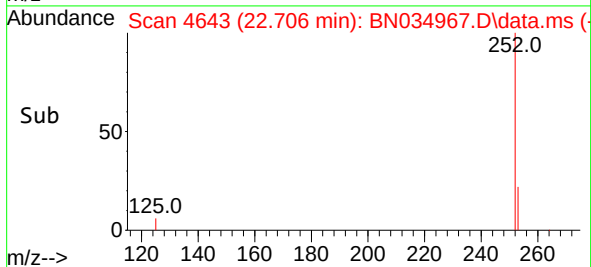
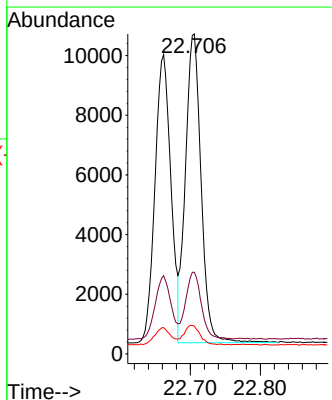
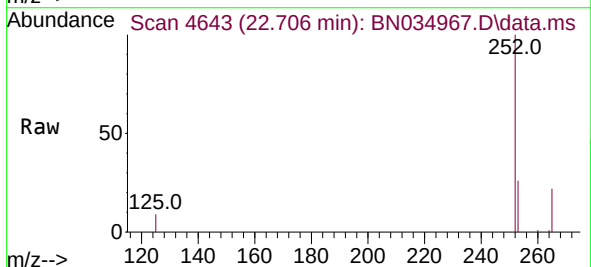


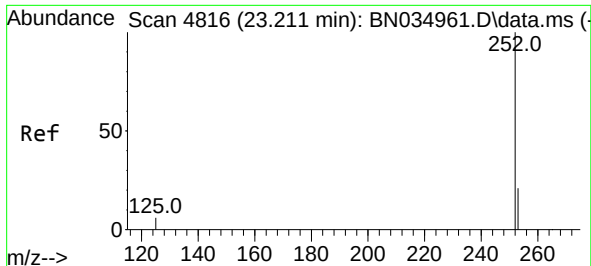

#26
Benzo(a)pyrene
Concen: 0.370 ng/ul
RT: 23.211 min Scan# 4816
Delta R.T. -0.006 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23




Instrument :
BNA_N
ClientSampleId :
GCP83MS


Tgt Ion:252 Resp: 13479
Ion Ratio Lower Upper
252 100
253 26.9 21.2 31.8
125 10.1 6.3 9.5#

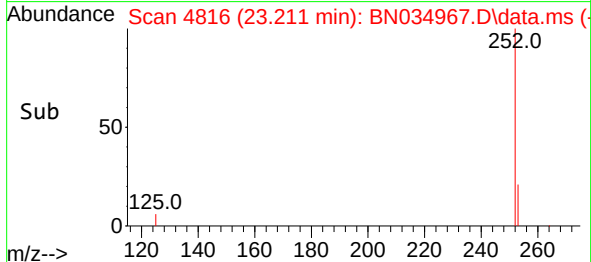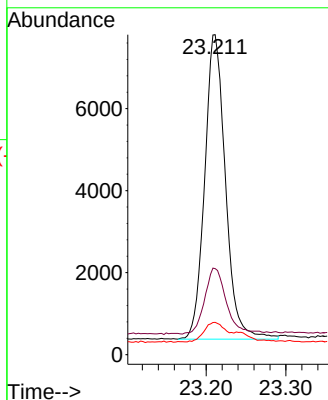

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.413 ng/ul
RT: 25.456 min Scan# 5564
Delta R.T. -0.013 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Tgt Ion:276 Resp: 18383
Ion Ratio Lower Upper
276 100
138 16.1 10.8 16.2
227 0.3 0.2 0.4


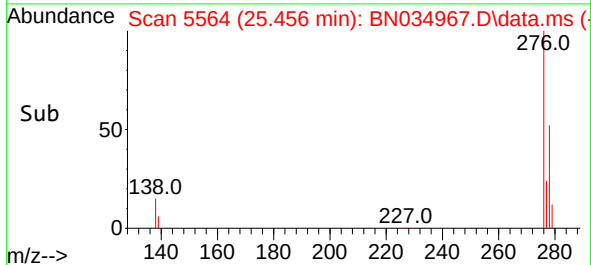
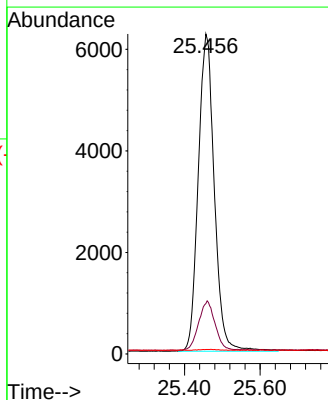
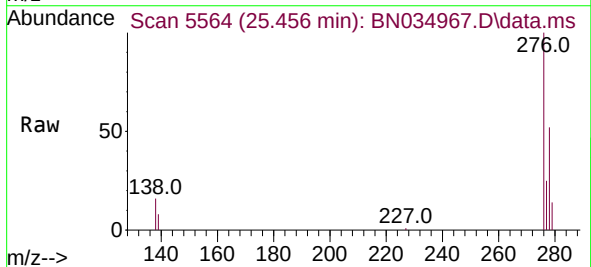


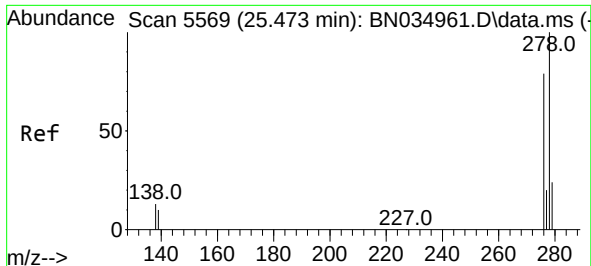

#28
Dibenzo(a,h)anthracene
Concen: 0.416 ng/ul
RT: 25.473 min Scan# 51
Delta R.T. -0.013 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Instrument :
BNA_N
ClientSampleId :
GCP83MS

Tgt Ion:278 Resp: 14452
Ion Ratio Lower Upper
278 100
139 12.3 8.4 12.6
279 27.0 21.5 32.3

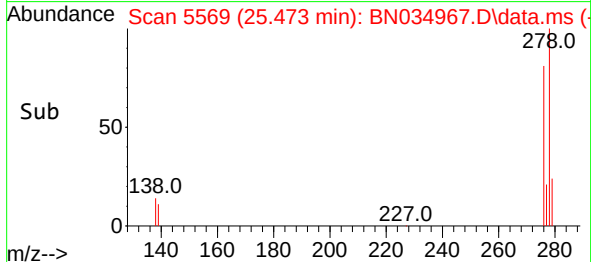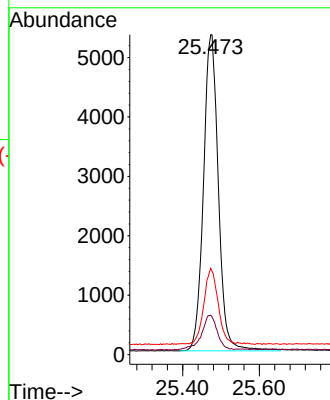

#29
Benzo(g,h,i)perylene
Concen: 0.418 ng/ul
RT: 26.110 min Scan# 5759
Delta R.T. -0.017 min
Lab File: BN034967.D
Acq: 10 Nov 2024 07:23

Tgt Ion:276 Resp: 14238
Ion Ratio Lower Upper
276 100
138 15.3 10.3 15.5
277 25.1 20.2 30.2

