

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034983.D
 Acq On : 10 Nov 2024 17:30
 Operator : RC/JU
 Sample : P4746-11
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP84

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

Quant Time: Nov 10 21:53:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.566	152	2696	0.400	ng/ul	0.00
4) Naphthalene-d8	10.328	136	6866	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.199	164	5046	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.945	188	11837m	0.400	ng/ul	0.00
17) Chrysene-d12	21.142	240	11500	0.400	ng/ul	# 0.00
23) Perylene-d12	23.308	264	11366m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	13497	5.261	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.923	152	3347	0.318	ng/ul	-0.01
18) Fluoranthene-d10	18.981	212	12100	0.410	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.187	88	286	0.102	ng/ul#	Qvalue 84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034983.D
Acq On : 10 Nov 2024 17:30
Operator : RC/JU
Sample : P4746-11
Misc :
ALS Vial : 77 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCP84

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024


Quant Time: Nov 10 21:53:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

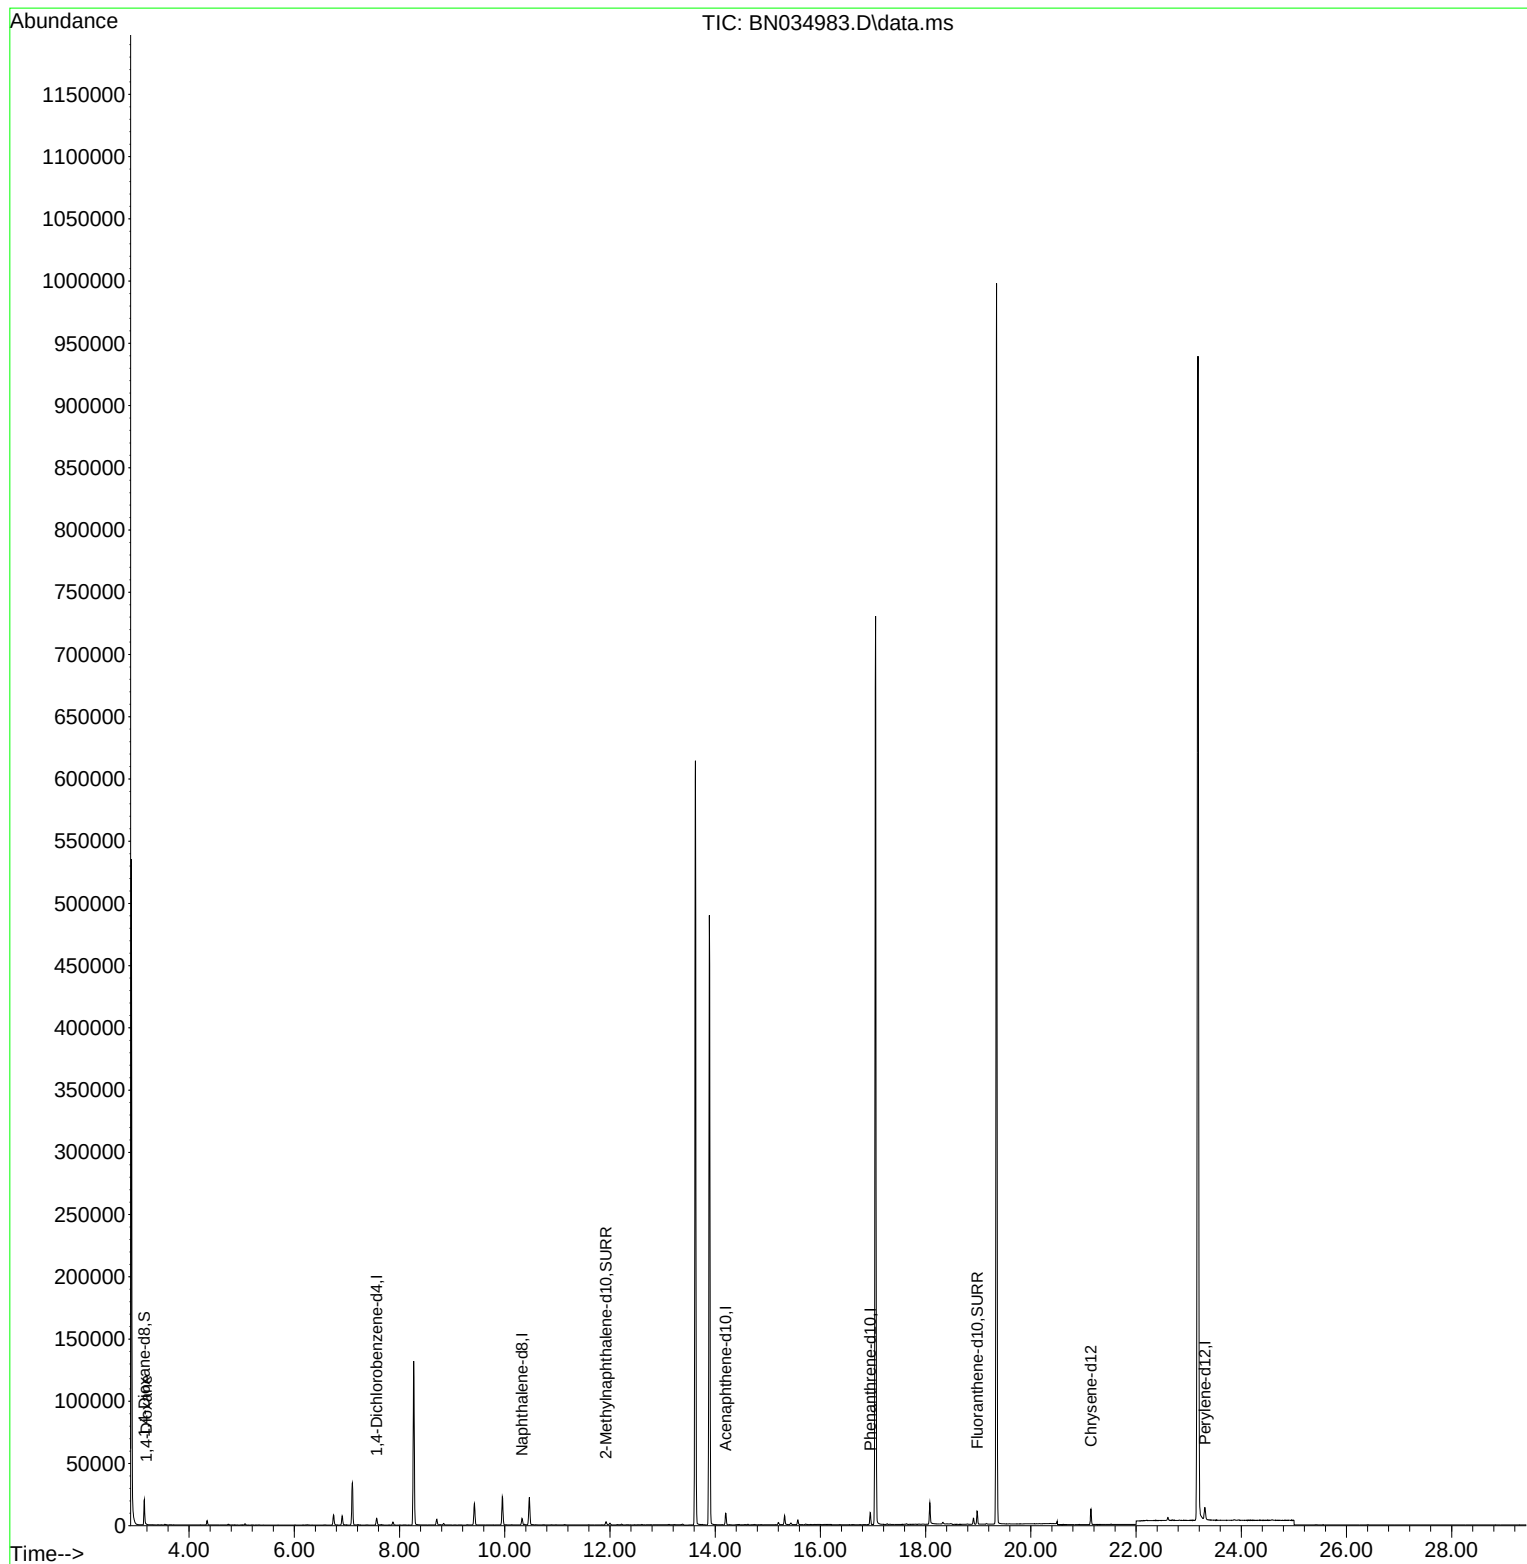

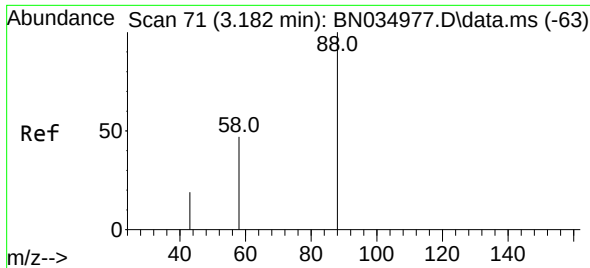

#2
 1,4-Dioxane
 Concen: 0.102 ng/ul
 RT: 3.187 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BN034983.D
 Acq: 10 Nov 2024 17:30

Instrument :
 BNA_N
 ClientSampleId :
 GCP84

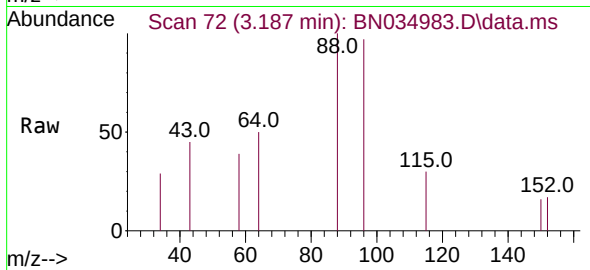

Tgt Ion: 88 Resp: 280
 Ion Ratio Lower Upper
 88 100
 43 44.7 23.3 34.9
 58 39.2 35.4 53.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

