

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
 Data File : BN034986.D
 Acq On : 10 Nov 2024 19:18
 Operator : RC/JU
 Sample : P4744-16
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCP71

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

Quant Time: Nov 10 21:53:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.566	152	3110	0.400	ng/ul	0.00
4) Naphthalene-d8	10.328	136	7657	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.199	164	5591	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.945	188	12554m	0.400	ng/ul	0.00
17) Chrysene-d12	21.142	240	11579	0.400	ng/ul	0.00
23) Perylene-d12	23.308	264	11581m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	13200	4.461	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.923	152	3920	0.334	ng/ul	-0.01
18) Fluoranthene-d10	18.981	212	13162	0.443	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.182	88	314	0.097	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110924\
Data File : BN034986.D
Acq On : 10 Nov 2024 19:18
Operator : RC/JU
Sample : P4744-16
Misc :
ALS Vial : 80 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCP71

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/12/2024


Quant Time: Nov 10 21:53:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

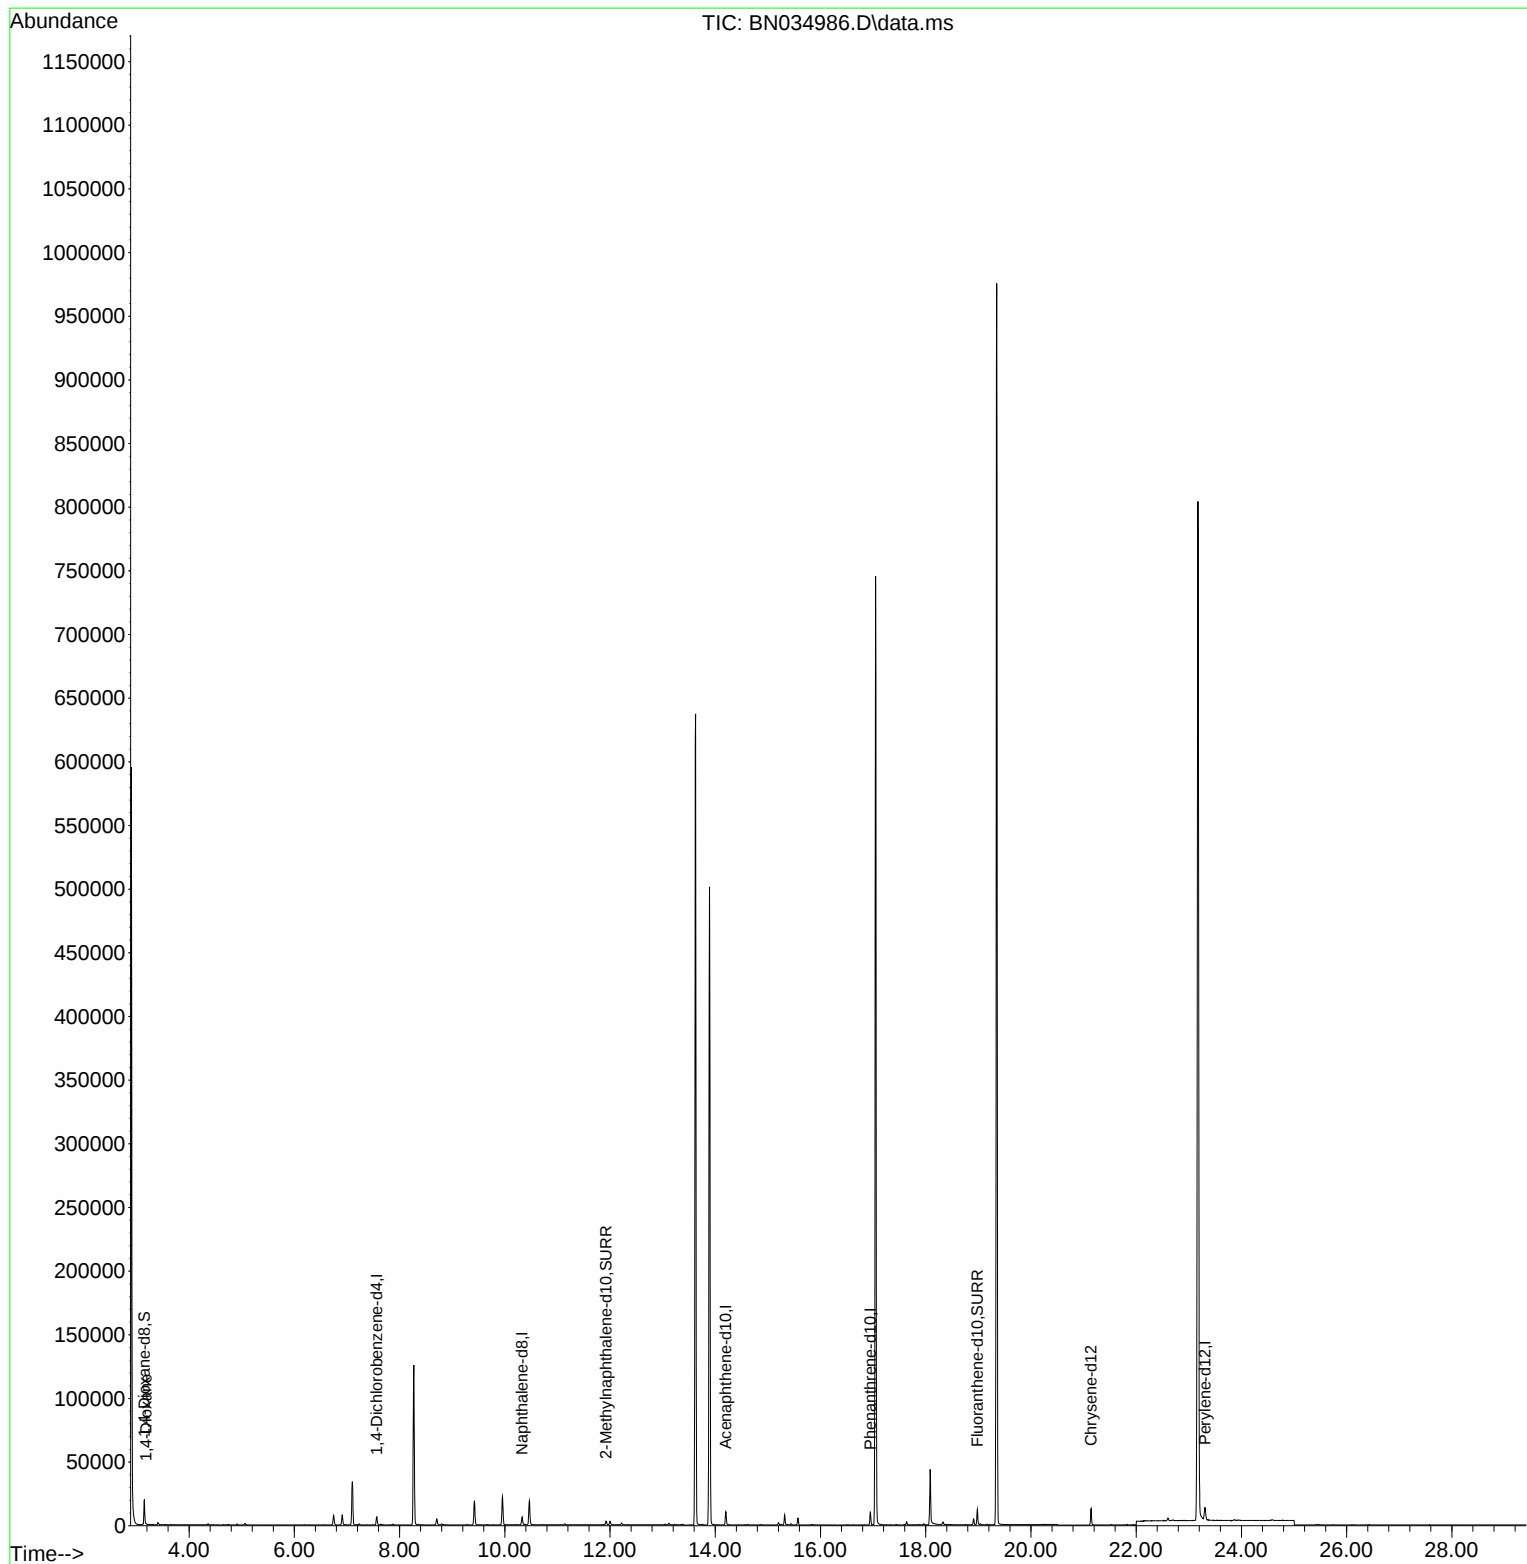

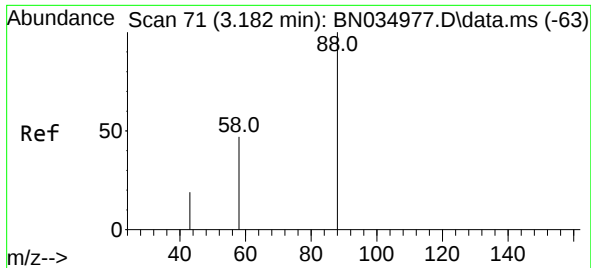

#2
 1,4-Dioxane
 Concen: 0.097 ng/ul
 RT: 3.182 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BN034986.D
 Acq: 10 Nov 2024 19:18

Instrument :
 BNA_N
 ClientSampleId :
 GCP71

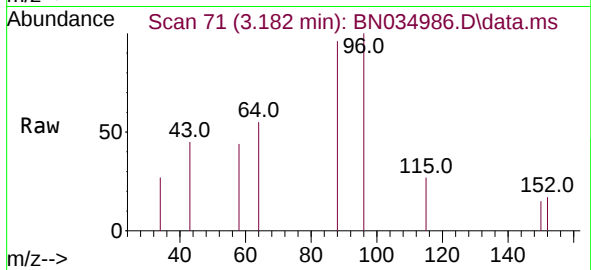

Tgt Ion: 88 Resp: 314

Ion	Ratio	Lower	Upper
88	100		
43	47.1	23.3	34.9
58	46.3	35.4	53.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/12/2024

