
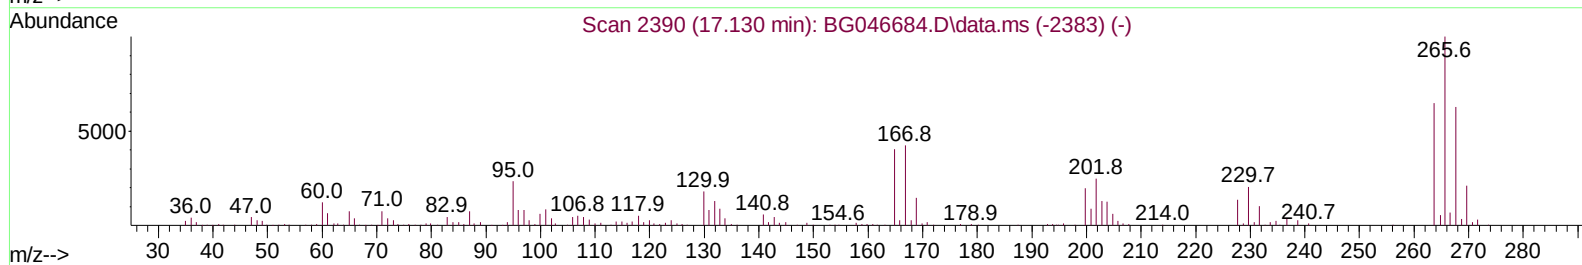
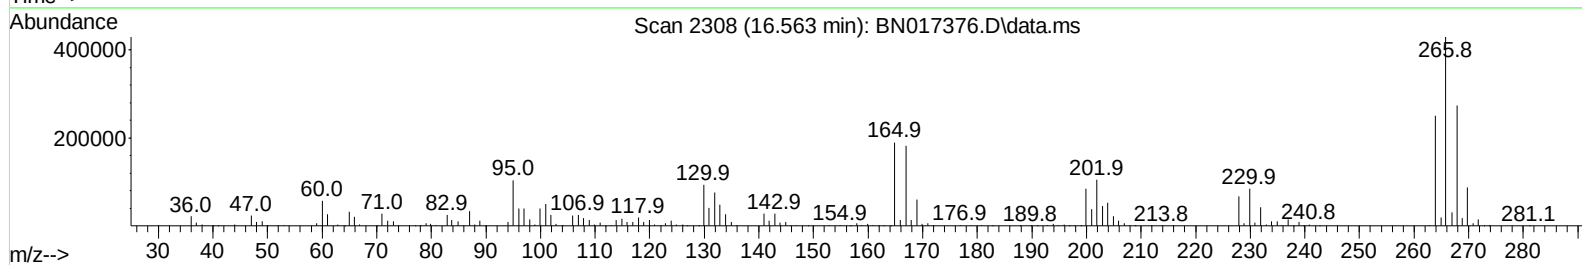


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN111021\  
Data File : BN017376.D  
Acq On : 10 Nov 2021 08:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 17:14:57 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 01 19:02:51 2021  
Response via : Initial Calibration

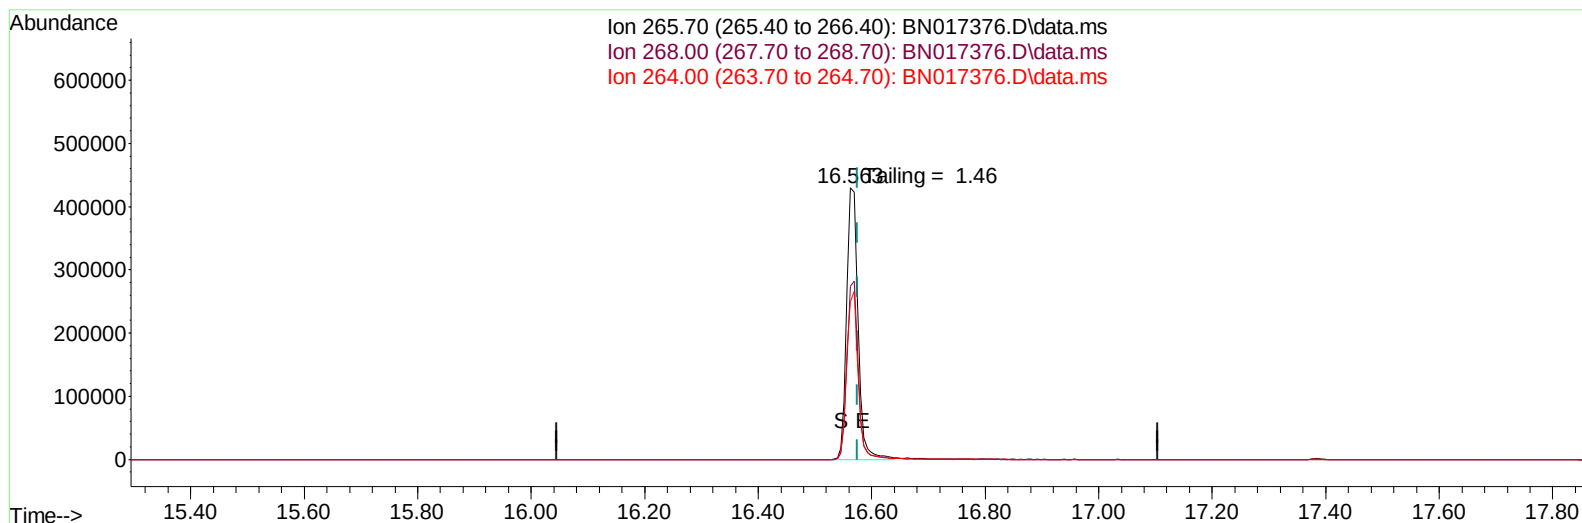




TIC: BN017376.D\data.ms

**(70) Pentachlorophenol (C)****16.563min (-0.012) 25772.96 ng****response 607386**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.78  |
| 264.00 | 61.60  | 58.21  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN111021\  
Data File : BN017376.D  
Acq On : 10 Nov 2021 08:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 17:14:57 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 01 19:02:51 2021  
Response via : Initial Calibration

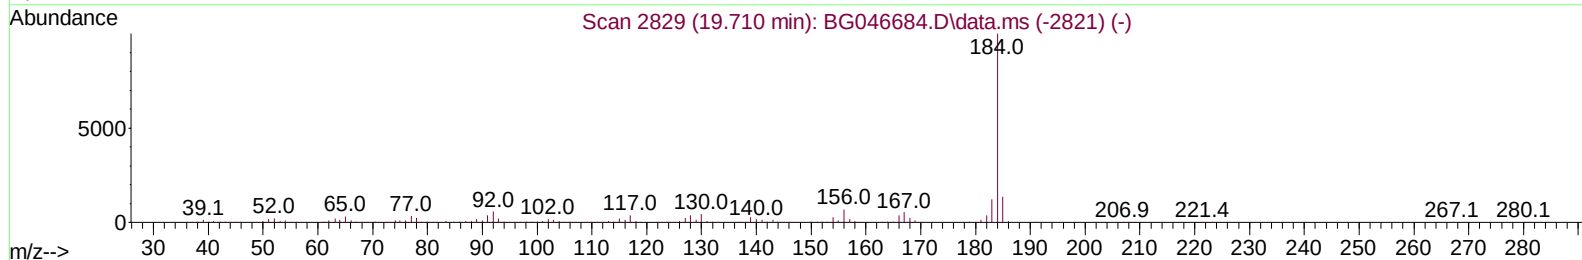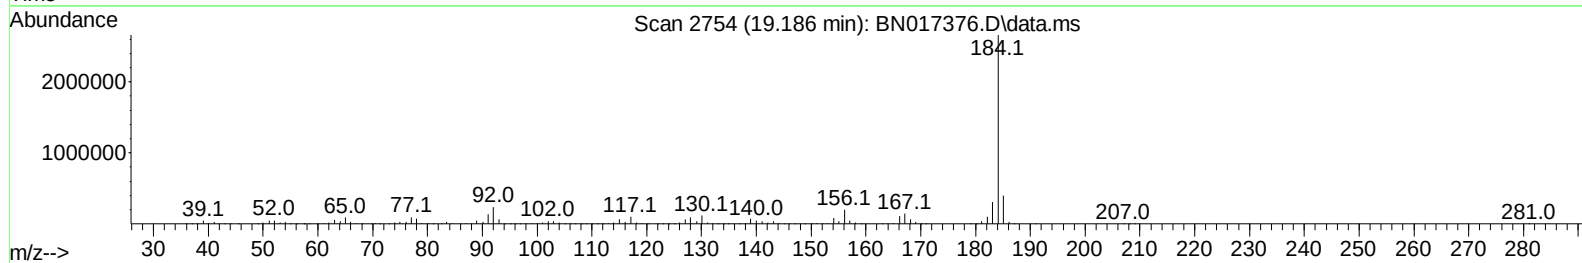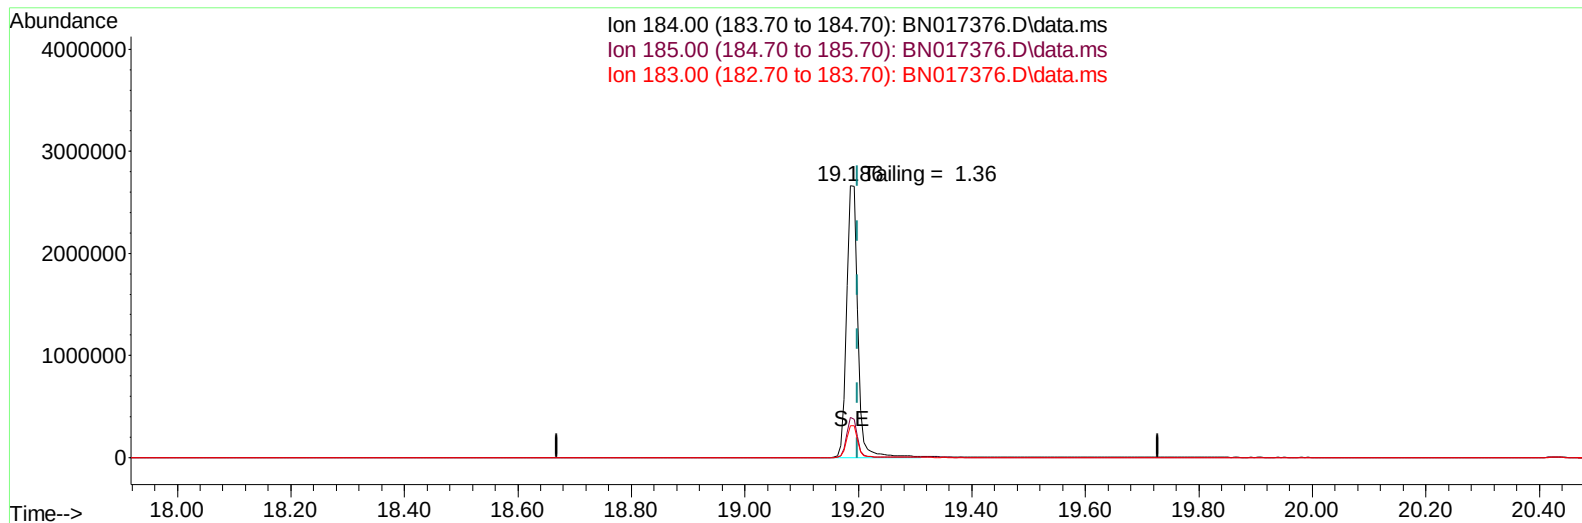

TIC: BN017376.D\data.ms

**(77) Benzidine**

19.186min (-0.012) 0.00 ng

response 3670214

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.80  |
| 183.00 | 13.20  | 11.70  |
| 0.00   | 0.00   | 0.00   |