


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111021\
 Data File : BN017376.D
 Acq On : 10 Nov 2021 08:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 10 11:00:44 2021

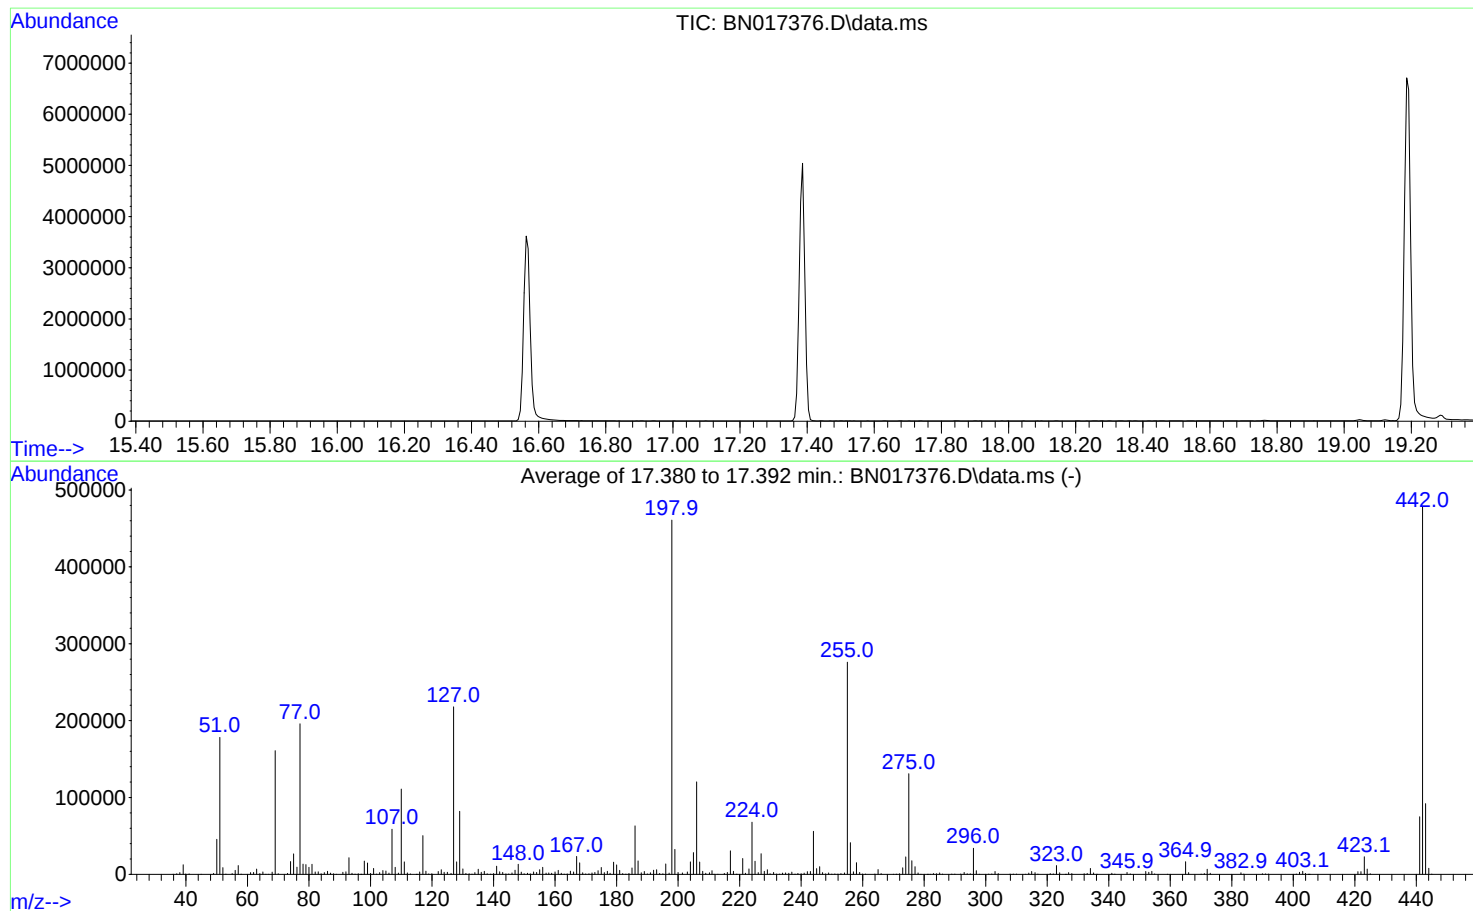




AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	178179	PASS
68	69	0.00	2	1.8	2911	PASS
69	198	0.00	100	34.9	160811	PASS
70	69	0.00	2	0.6	888	PASS
127	198	10	80	47.3	217835	PASS
197	198	0.00	2	0.4	1634	PASS
198	198	100	100	100.0	460843	PASS
199	198	5	9	7.1	32515	PASS
275	198	10	60	28.4	130912	PASS
365	198	1	100	3.5	16359	PASS
441	198	0.01	100	16.3	74965	PASS
442	442	50	100	100.0	478485	PASS
443	442	15	24	19.2	92005	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111021\
Data File : BN017376.D
Acq On : 10 Nov 2021 08:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 10 17:14:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

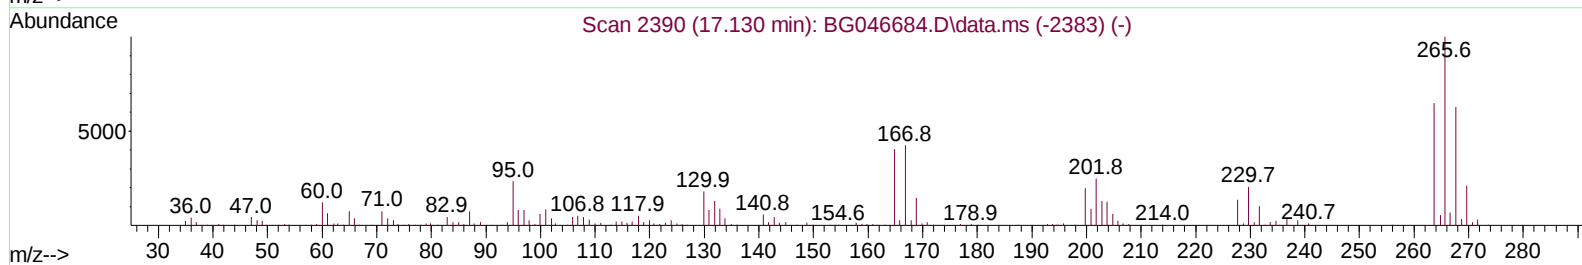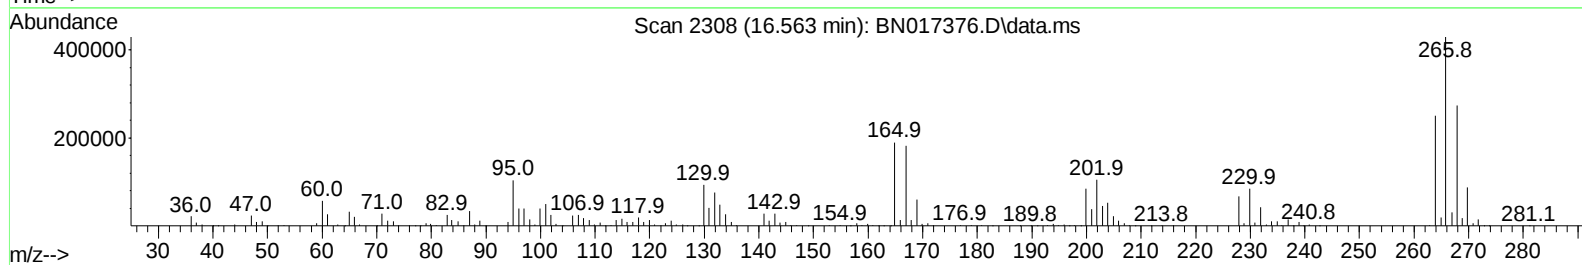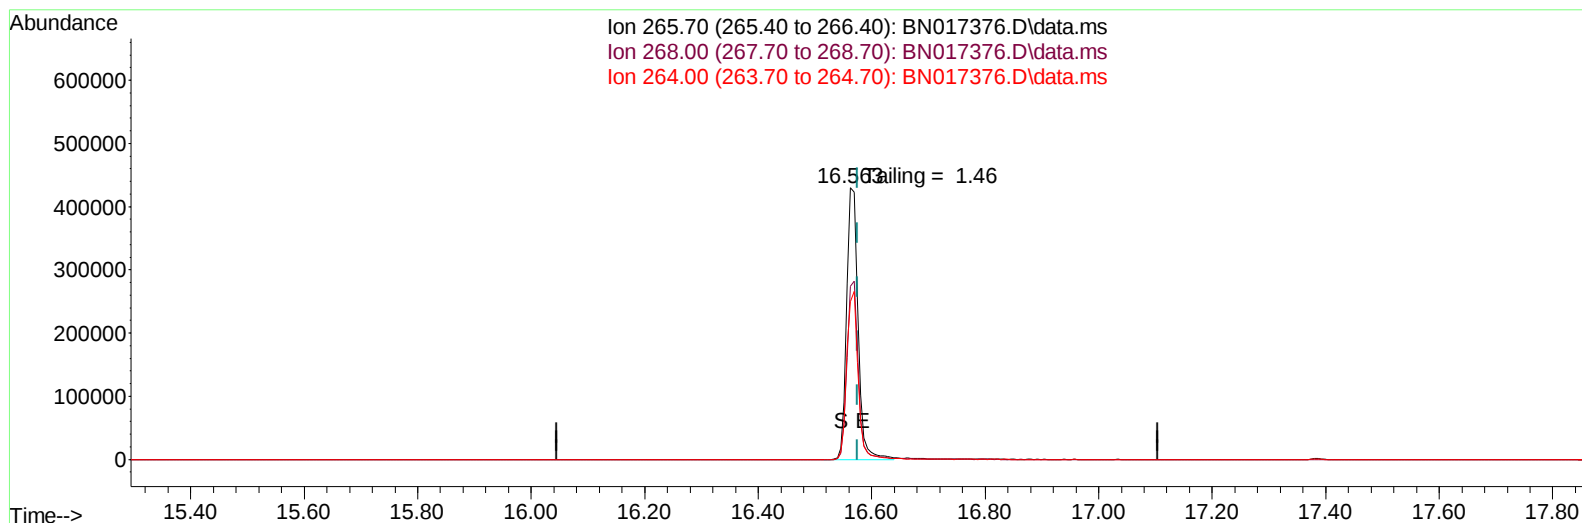

TIC: BN017376.D\data.ms

(70) Pentachloropheno1 (C)

16.563min (-0.012) 25772.96 ng

response 607386

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.78
264.00	61.60	58.21
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
11/10/2021	BNA_N	<u>BN017376.D</u>
Compound Name	Response	Retention Time
DDT	1687029	20.427
DDD	19581	19.986
DDE	246	19.474
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19827	1706856	1.16