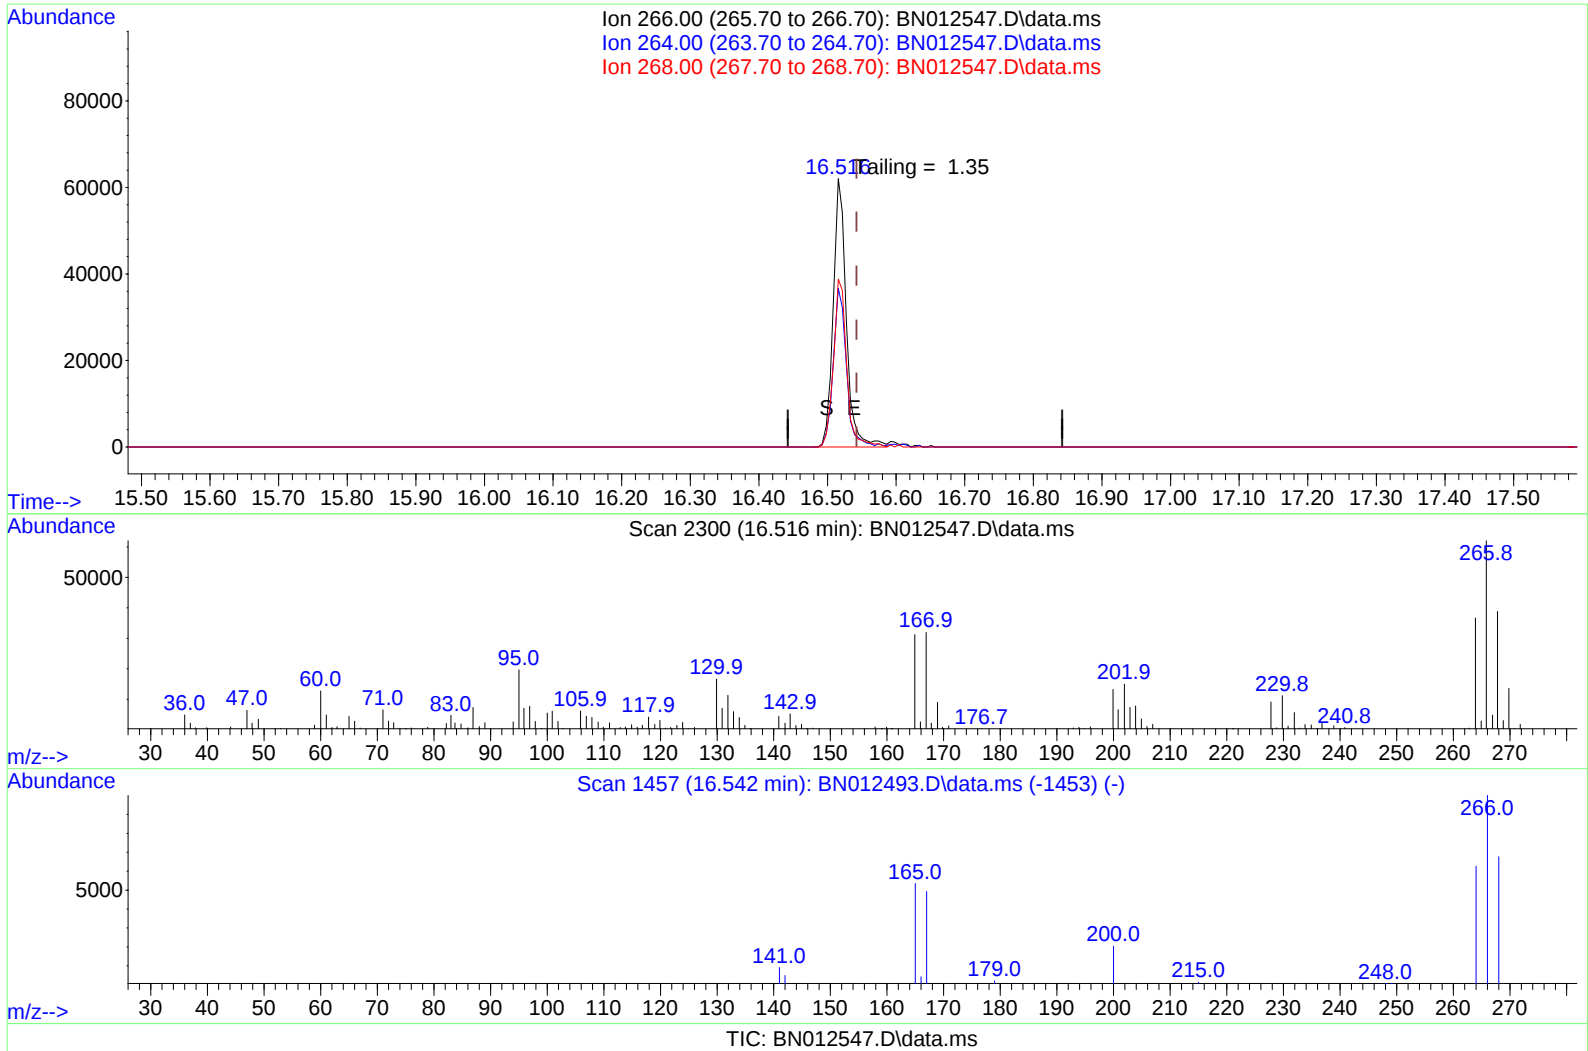


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111120\
Data File : BN012547.D
Acq On : 12 Nov 2020 01:21
Operator : CG/JU
Sample : DFTPP14
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 01:53:35 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 05 05:46:47 2020
Response via : Initial Calibration

**(24) Pentachlorophenol****16.516min (-0.026) 0.00 ng****response 80967**

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	60.69
268.00	64.40	64.30
0.00	0.00	0.00