

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111120\
 Data File : BN012556.D
 Acq On : 12 Nov 2020 09:35
 Operator : CG/JU
 Sample : L4684-11DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB178-GW-518-520DL

Manual Integrations
 APPROVED

mohammad
 11/12/2020 11:38:36 AM

Quant Time: Nov 12 10:33:35 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 05 05:46:47 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.457	152	311	0.40	ng	#-0.03
7) Naphthalene-d8	10.237	136	1176	0.40	ng	#-0.01
13) Acenaphthene-d10	14.116	164	746	0.40	ng	-0.03
19) Phenanthrene-d10	16.859	188	1595	0.40	ng	#-0.02
29) Chrysene-d12	21.078	240	1819	0.40	ng	#-0.02
36) Perylene-d12	23.193	264	2176	0.40	ng	-0.03
System Monitoring Compounds						
4) 2-Fluorophenol	5.066	112	38	0.03	ng	-0.03
5) Phenol-d6	6.652	99	19	0.01	ng	-0.02
8) Nitrobenzene-d5	8.641	82	110	0.08	ng	0.00
11) 2-Methylnaphthalene-d10	11.842	152	101	0.05	ng	-0.01
14) 2,4,6-Tribromophenol	15.626	330	48	0.09	ng	-0.01
15) 2-Fluorobiphenyl	12.733	172	232	0.08	ng	-0.03
27) Fluoranthene-d10	18.908	212	354	0.07	ng	-0.02
31) Terphenyl-d14	19.519	244	532	0.12	ng	-0.02
Target Compounds						
2) 1,4-Dioxane	3.020	88	1666m	3.43	ng	Qvalue
34) Bis(2-ethylhexyl)phtha...	21.004	149	289	0.07	ng	# 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111120\
Data File : BN012556.D
Acq On : 12 Nov 2020 09:35
Operator : CG/JU
Sample : L4684-11DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-VPB178-GW-518-520DL

Manual Integrations
APPROVED

mohammad
11/12/2020 11:38:36 AM

Quant Time: Nov 12 10:33:35 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 05 05:46:47 2020
Response via : Initial Calibration

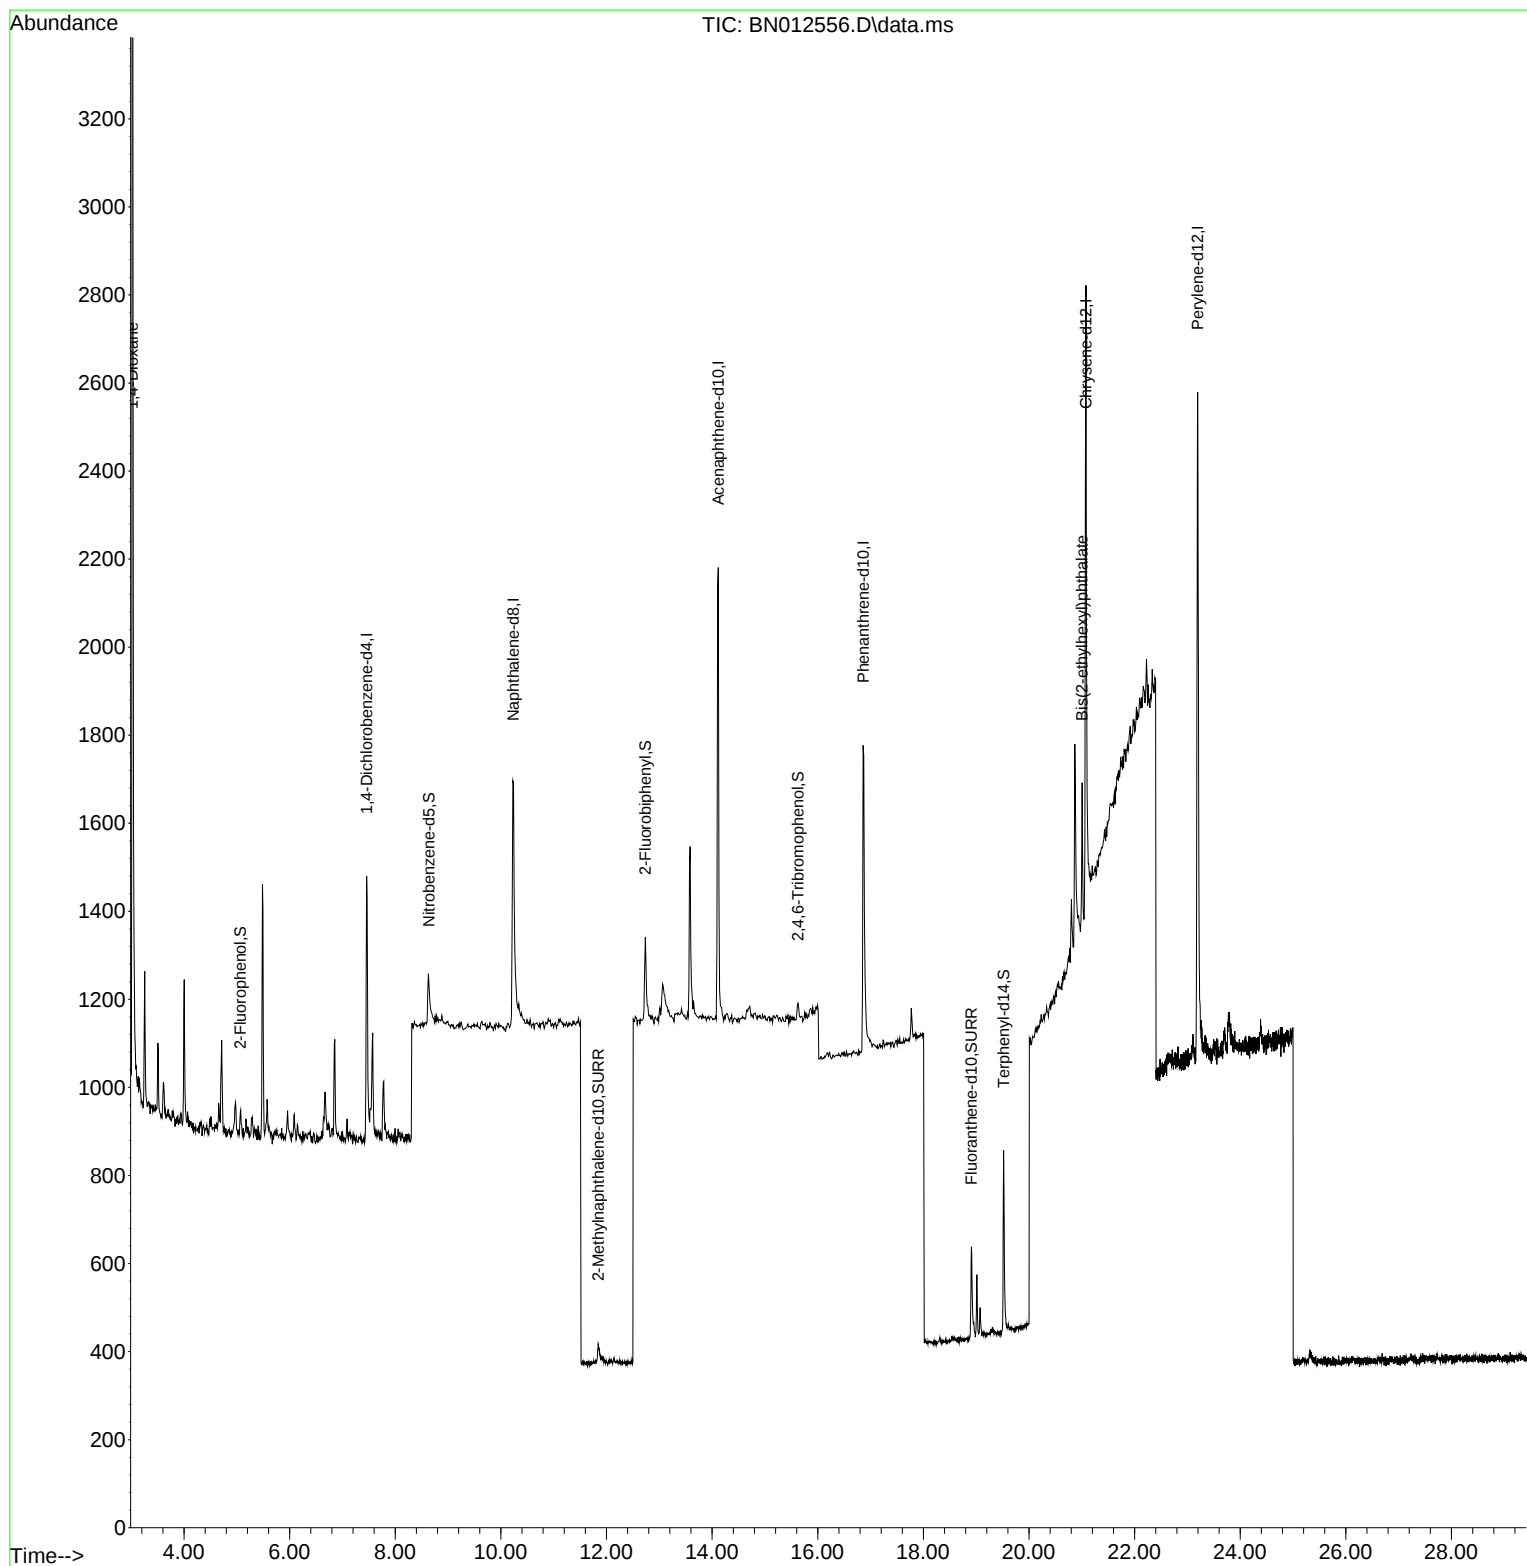







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.457 min Scan# 556
 Delta R.T. -0.032 min
 Lab File: BN012556.D
 Acq: 12 Nov 2020 09:35

Tgt Ion: 152 Resp: 311
 Ion Ratio Lower Upper
 152 100
 150 140.7 116.6 174.8
 115 88.9 52.9 79.3#

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB178-GW-518-520DL




Manual Integrations
 APPROVED


mohammad
 11/12/2020 11:38:36 AM

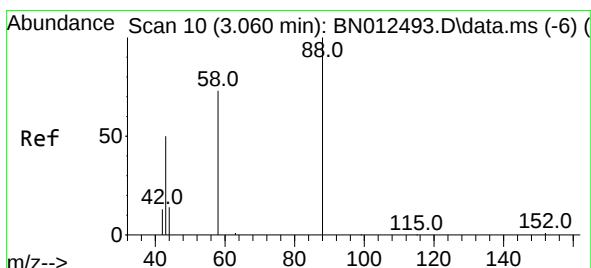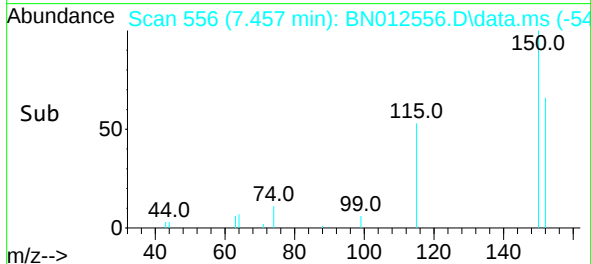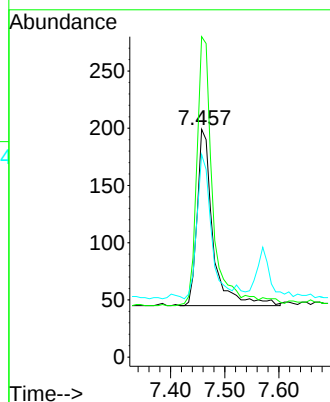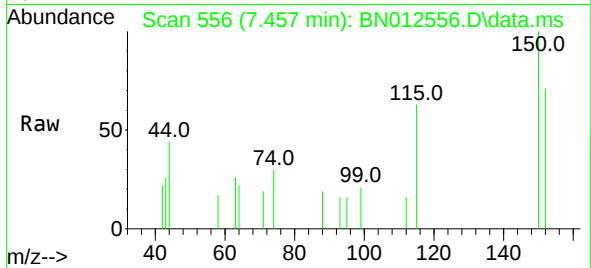

#2
 1,4-Dioxane
 Concen: 3.43 ng m
 RT: 3.020 min Scan# 5
 Delta R.T. -0.040 min
 Lab File: BN012556.D
 Acq: 12 Nov 2020 09:35

Tgt Ion: 88 Resp: 1666
 Ion Ratio Lower Upper
 88 100
 58 67.9 59.4 89.2
 43 65.0 32.3 48.5#

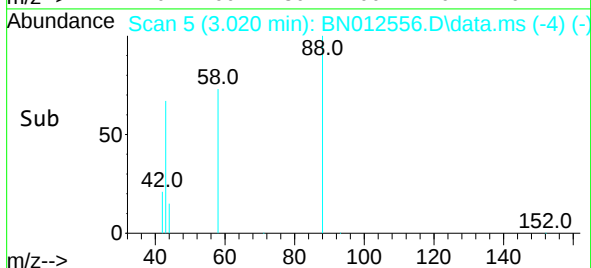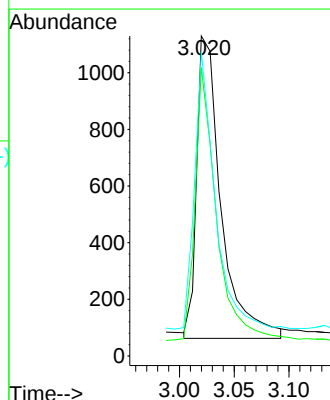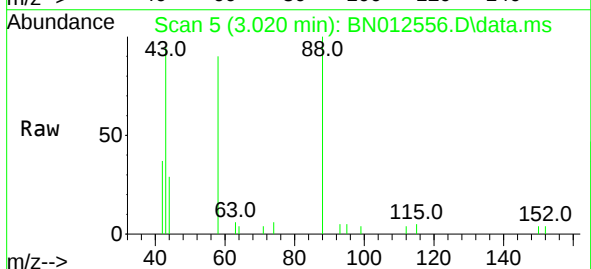

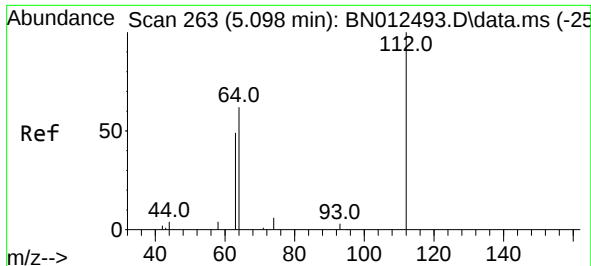





#4
2-Fluorophenol
Concen: 0.03 ng
RT: 5.066 min Scan# 259
Delta R.T. -0.032 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

Tgt Ion: 112 Resp: 38
Ion Ratio Lower Upper
112 100
64 76.3 49.5 74.3#
63 84.2 32.0 48.0#

Instrument :
BNA_N
ClientSampleId :
BP-VPB178-GW-518-520DL




Manual Integrations
APPROVED


mohammad
11/12/2020 11:38:36 AM

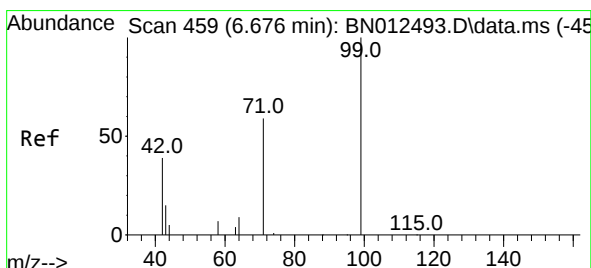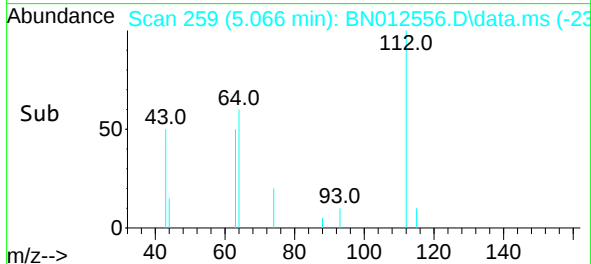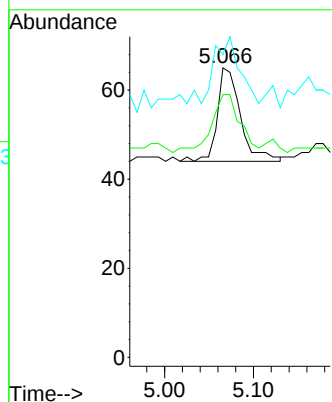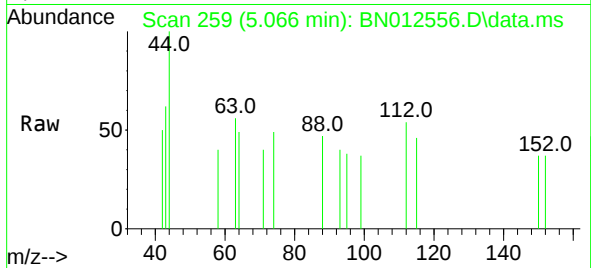

#5
Phenol-d6
Concen: 0.01 ng
RT: 6.652 min Scan# 456
Delta R.T. -0.024 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35


Tgt Ion: 99 Resp: 19
Ion Ratio Lower Upper
99 100
42 189.5 22.4 33.6#
71 100.0 37.8 56.6#

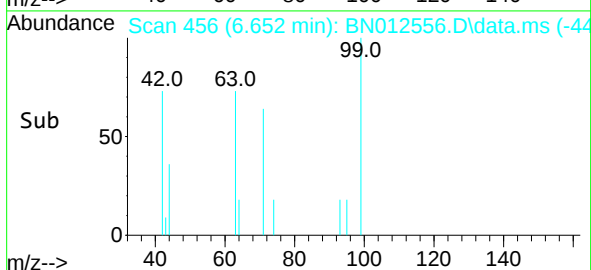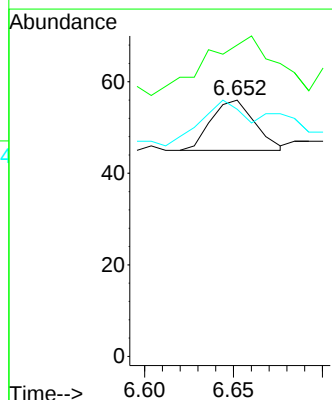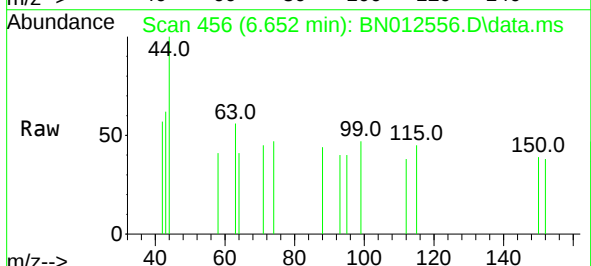

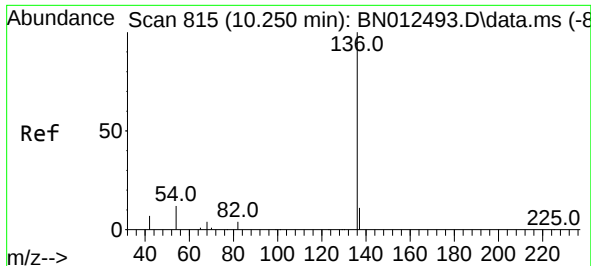

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.237 min Scan# 814
Delta R.T. -0.013 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35




Instrument :
BNA_N
ClientSampleId :
BP-VPB178-GW-518-520DL

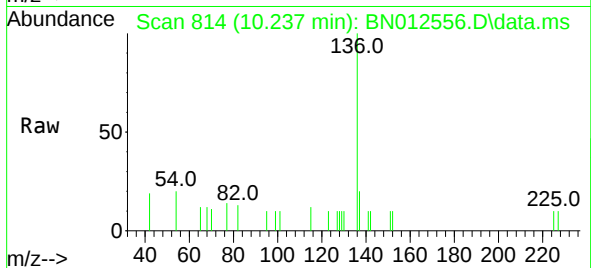


Tgt Ion: 136 Resp: 1176
Ion Ratio Lower Upper
136 100
137 20.4 10.6 15.8#
54 19.8 8.6 12.8#
68 12.4 5.7 8.5#

Manual Integrations
APPROVED



mohammad
11/12/2020 11:38:36 AM

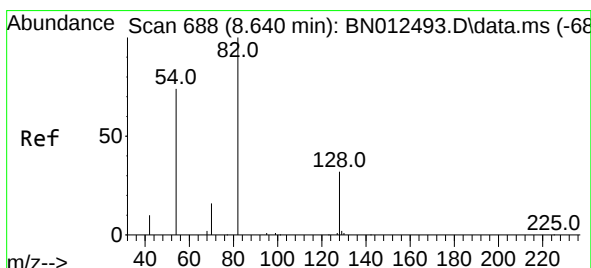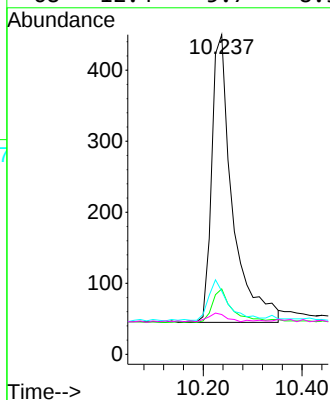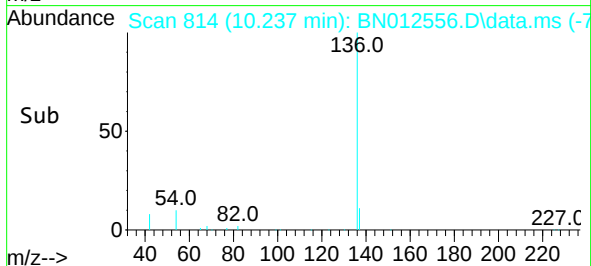


#8
Nitrobenzene-d5
Concen: 0.08 ng
RT: 8.641 min Scan# 688
Delta R.T. 0.000 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

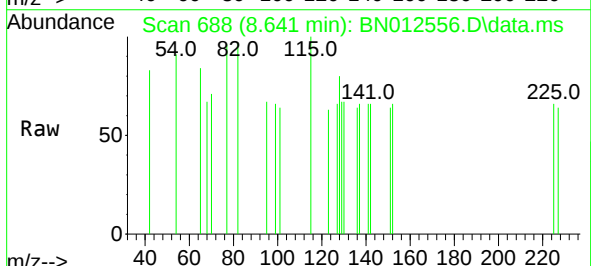

Tgt Ion: 82 Resp: 110
Ion Ratio Lower Upper
82 100
128 82.4 30.6 46.0#
54 94.1 48.3 72.5#

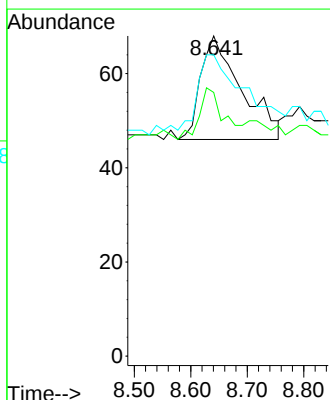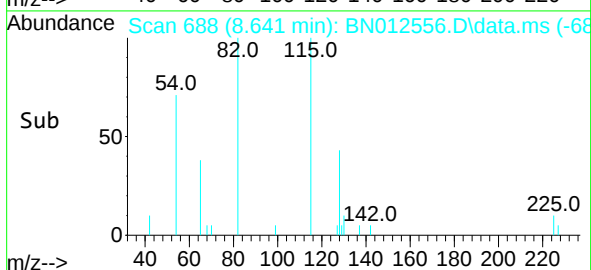

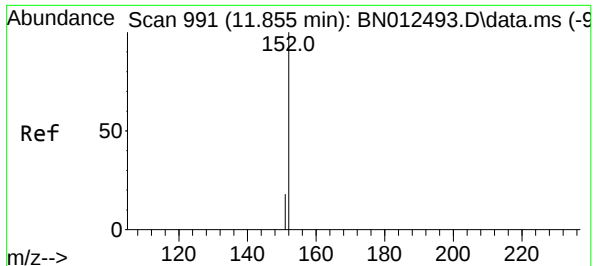





#11
2-Methylnaphthalene-d10
Concen: 0.05 ng
RT: 11.842 min Scan# 988
Delta R.T. -0.013 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

Tgt Ion:152 Resp: 101
Ion Ratio Lower Upper
152 100
151 20.8 16.7 25.1

Instrument :
BNA_N
ClientSampleId :
BP-VPB178-GW-518-520DL




Manual Integrations
APPROVED


mohammad
11/12/2020 11:38:36 AM

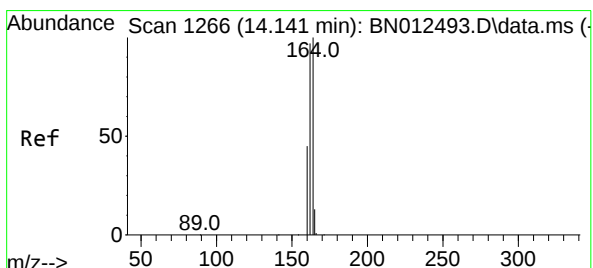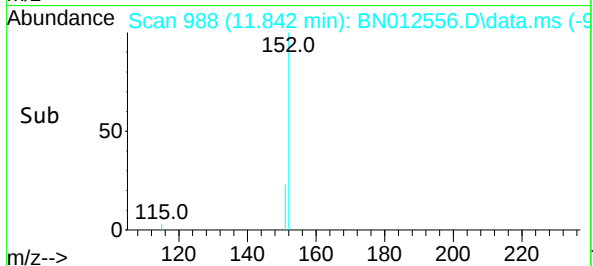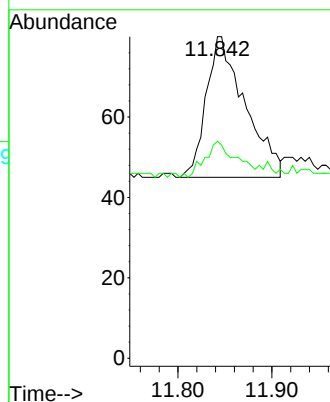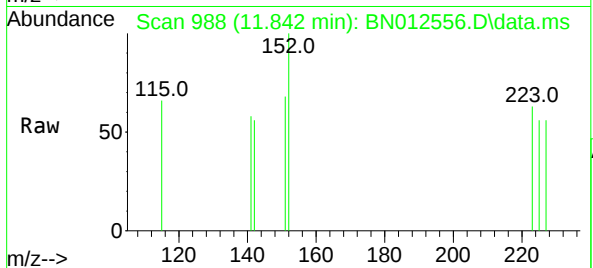

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.116 min Scan# 1264
Delta R.T. -0.025 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35


Tgt Ion:164 Resp: 746
Ion Ratio Lower Upper
164 100
162 103.5 80.6 120.8
160 52.7 39.5 59.3

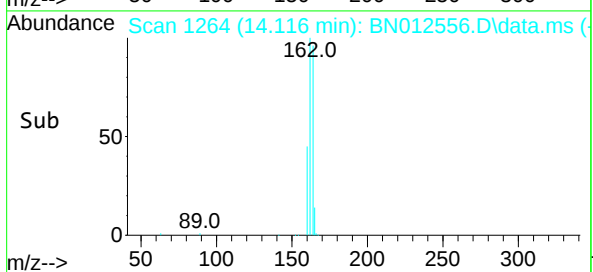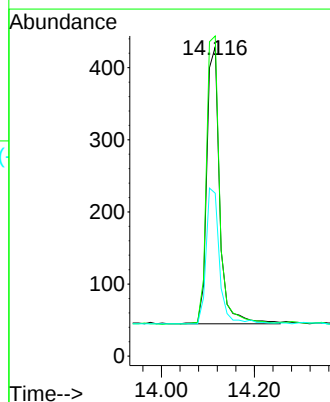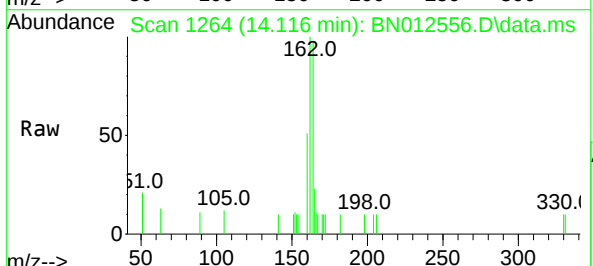

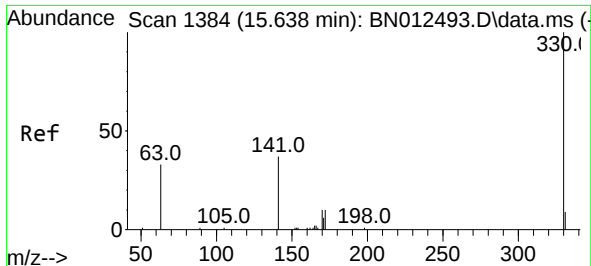

#14
2,4,6-Tribromophenol
Concen: 0.09 ng
RT: 15.626 min Scan# 1383
Delta R.T. -0.013 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35




Instrument :
BNA_N
ClientSampleId :
BP-VPB178-GW-518-520DL

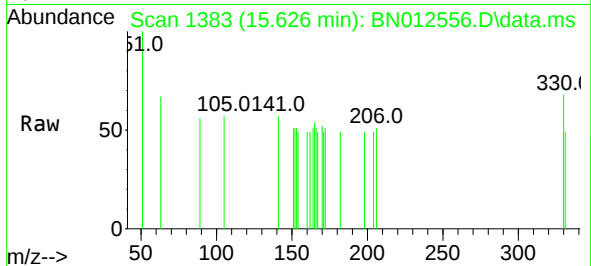

Tgt Ion:330 Resp: 48
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 37.5 34.4 51.6




Manual Integrations
APPROVED


mohammad
11/12/2020 11:38:36 AM

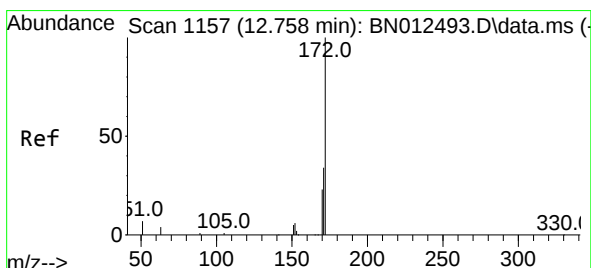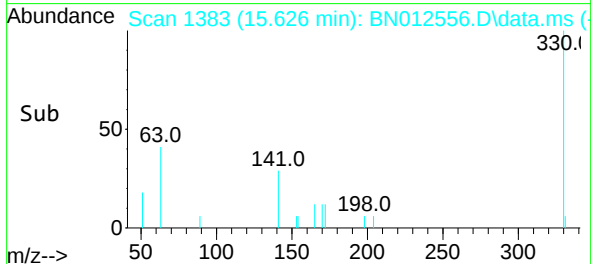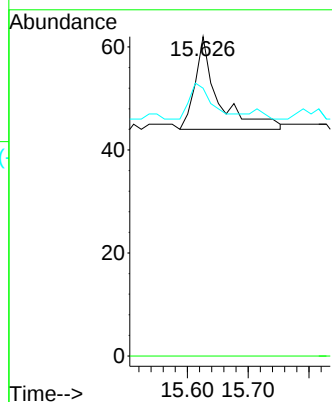


#15
2-Fluorobiphenyl
Concen: 0.08 ng
RT: 12.733 min Scan# 1155
Delta R.T. -0.025 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

Tgt Ion:172 Resp: 232
Ion Ratio Lower Upper
172 100
171 60.3 28.2 42.4#
170 49.3 20.0 30.0#

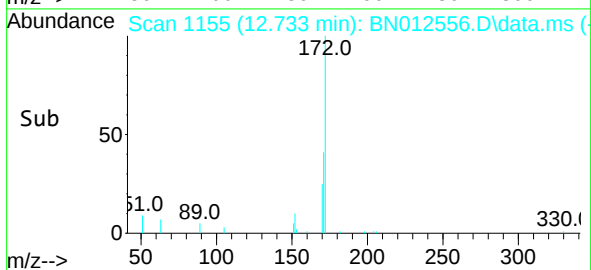
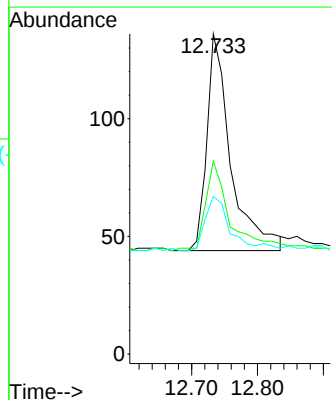
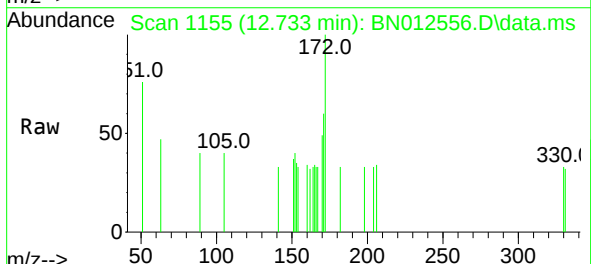


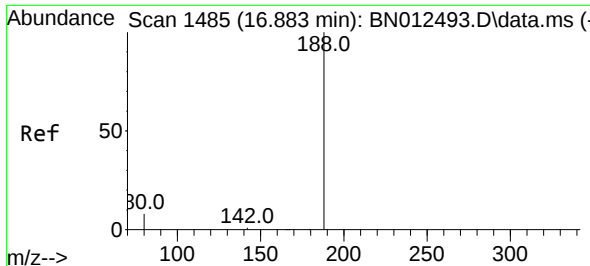


#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.859 min Scan# 1483
Delta R.T. -0.024 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

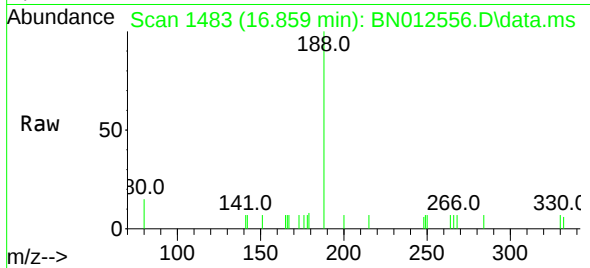



Tgt Ion:188 Resp: 1595
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 15.0 5.0 7.4#

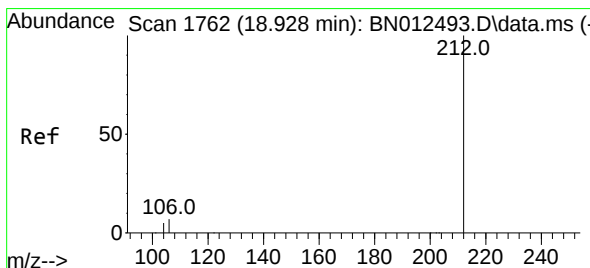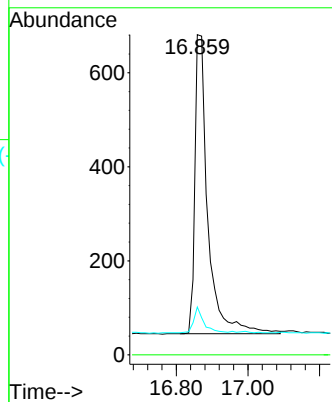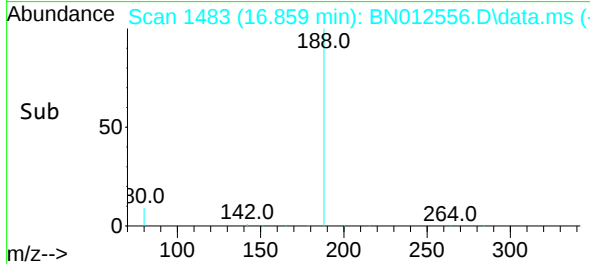

#27
Fluoranthene-d10
Concen: 0.07 ng
RT: 18.908 min Scan# 1758
Delta R.T. -0.020 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

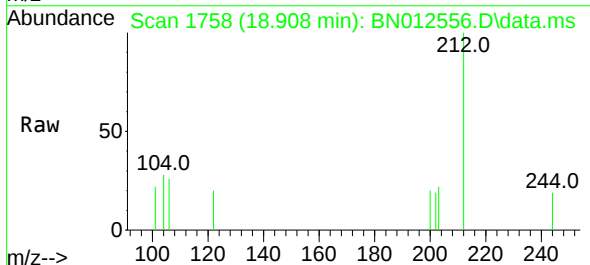


Tgt Ion:212 Resp: 354
Ion Ratio Lower Upper
212 100
106 7.1 6.8 10.2
104 3.1 4.1 6.1#

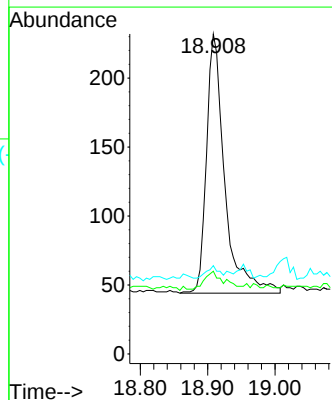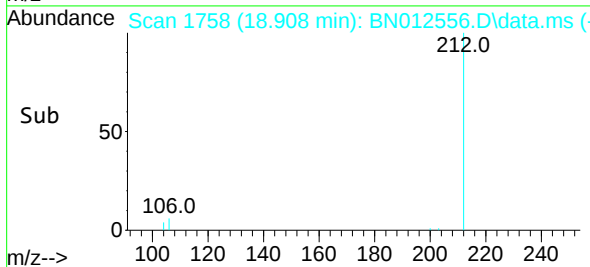

Instrument :
BNA_N
ClientSampleId :
BP-VPB178-GW-518-520DL

Manual Integrations
APPROVED

mohammad
11/12/2020 11:38:36 AM

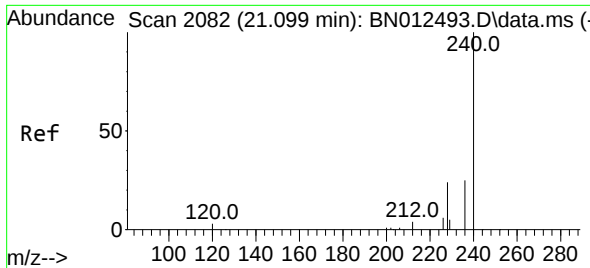





#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.078 min Scan# 2080
Delta R.T. -0.021 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

Tgt Ion:240 Resp: 1819
Ion Ratio Lower Upper
240 100
120 10.7 5.3 7.9#
236 29.7 21.8 32.8

Instrument :
BNA_N
ClientSampleId :
BP-VPB178-GW-518-520DL




Manual Integrations
APPROVED


mohammad
11/12/2020 11:38:36 AM

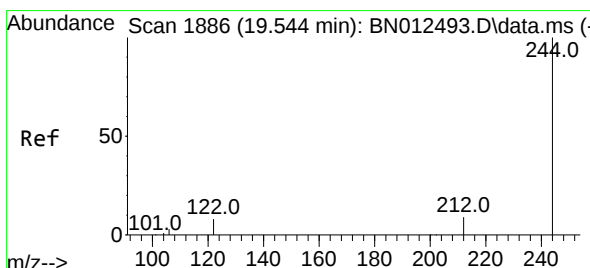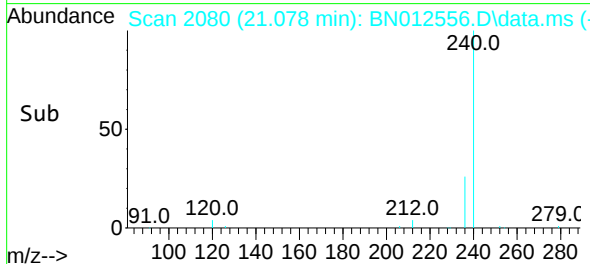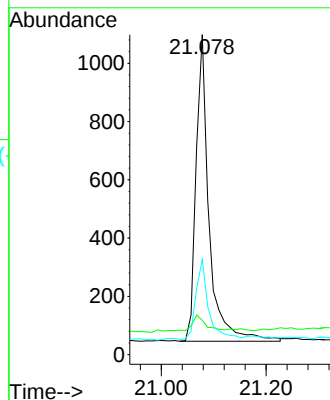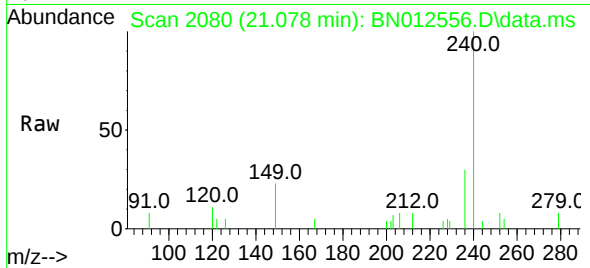

#31
Terphenyl-d14
Concen: 0.12 ng
RT: 19.519 min Scan# 1881
Delta R.T. -0.025 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

Tgt Ion:244 Resp: 532
Ion Ratio Lower Upper
244 100
212 19.7 7.3 10.9#
122 18.4 7.3 10.9#

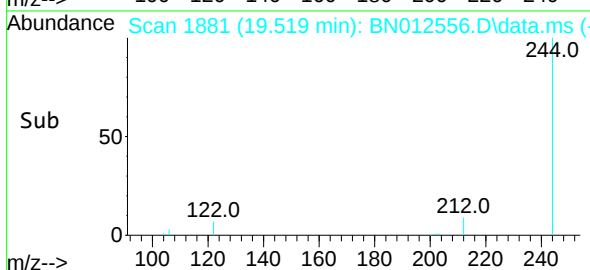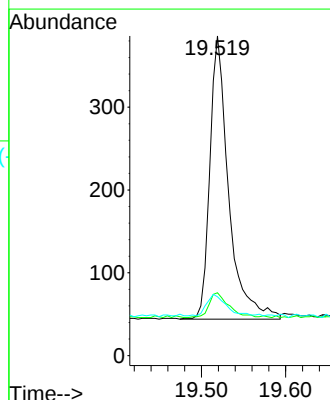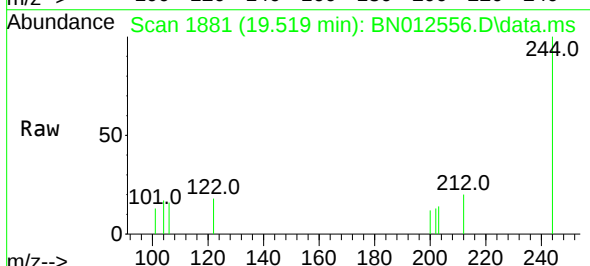

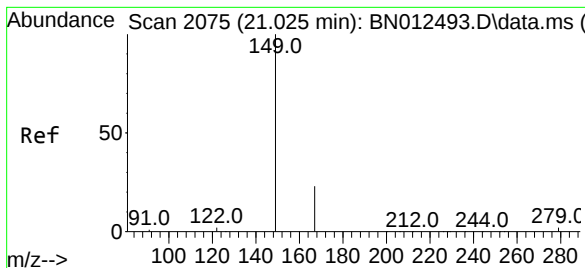





#34
Bis(2-ethylhexyl)phthalate
Concen: 0.07 ng
RT: 21.004 min Scan# 2073
Delta R.T. -0.021 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

Tgt Ion:149 Resp: 289
Ion Ratio Lower Upper
149 100
167 23.9 23.2 34.8
279 5.9 3.9 5.9#

Instrument :
BNA_N
ClientSampleId :
BP-VPB178-GW-518-520DL

Manual Integrations
APPROVED

mohammad
11/12/2020 11:38:36 AM

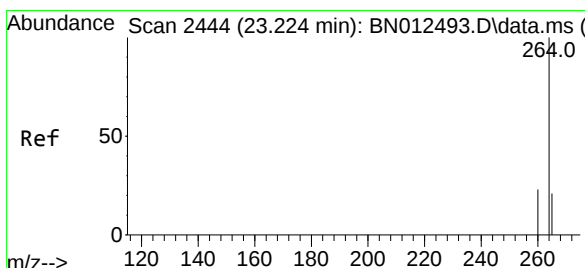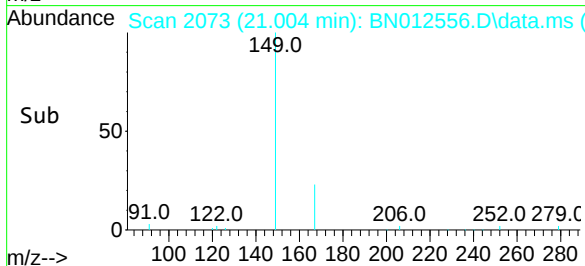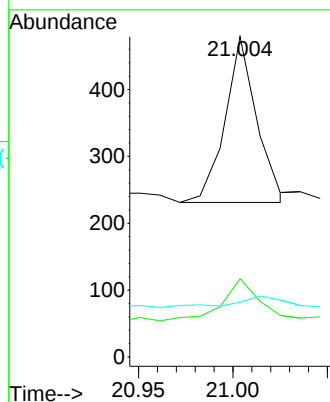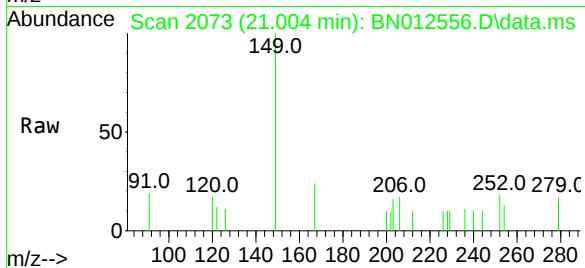

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.193 min Scan# 2435
Delta R.T. -0.031 min
Lab File: BN012556.D
Acq: 12 Nov 2020 09:35

Tgt Ion:264 Resp: 2176
Ion Ratio Lower Upper
264 100
260 25.6 19.8 29.6
265 68.0 51.4 77.0

