
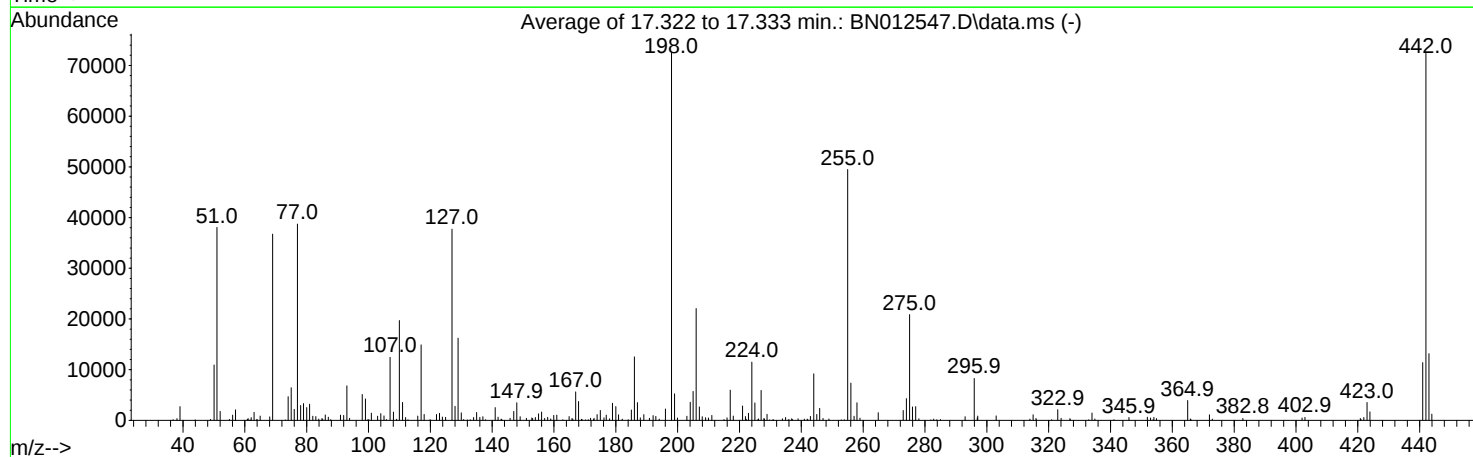


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111120\
Data File : BN012547.D
Acq On : 12 Nov 2020 01:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110420.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 05 05:46:47 2020

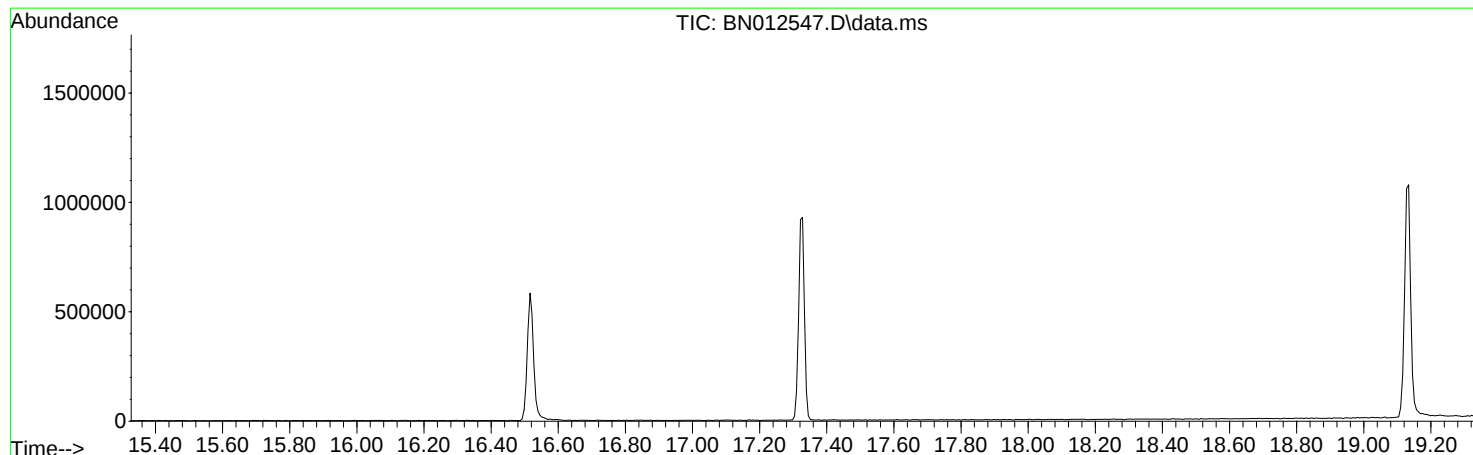

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	38056	PASS
68	69	0.00	2	1.9	691	PASS
69	198	0.00	100	50.6	36736	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	37707	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72555	PASS
199	198	5	9	7.2	5244	PASS
275	198	10	60	28.8	20865	PASS
365	198	1	100	5.4	3924	PASS
441	198	0.01	100	15.7	11393	PASS
442	198	50	100	99.8	72387	PASS
443	442	15	24	18.2	13164	PASS