
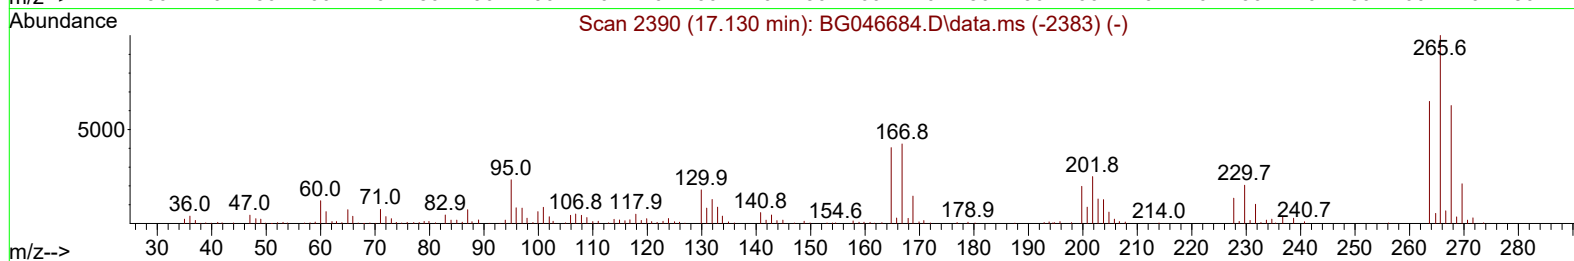
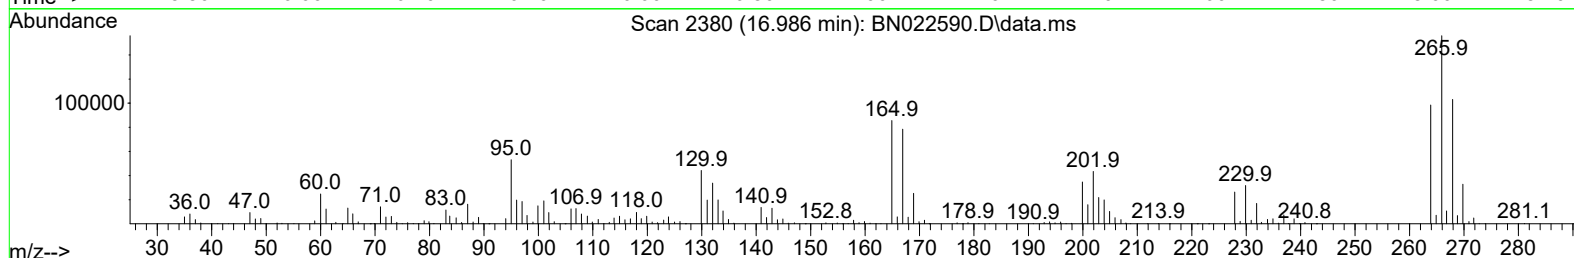


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
Data File : BN022590.D
Acq On : 10 Nov 2022 08:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 05:20:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 05:20:15 2022
Response via : Initial Calibration

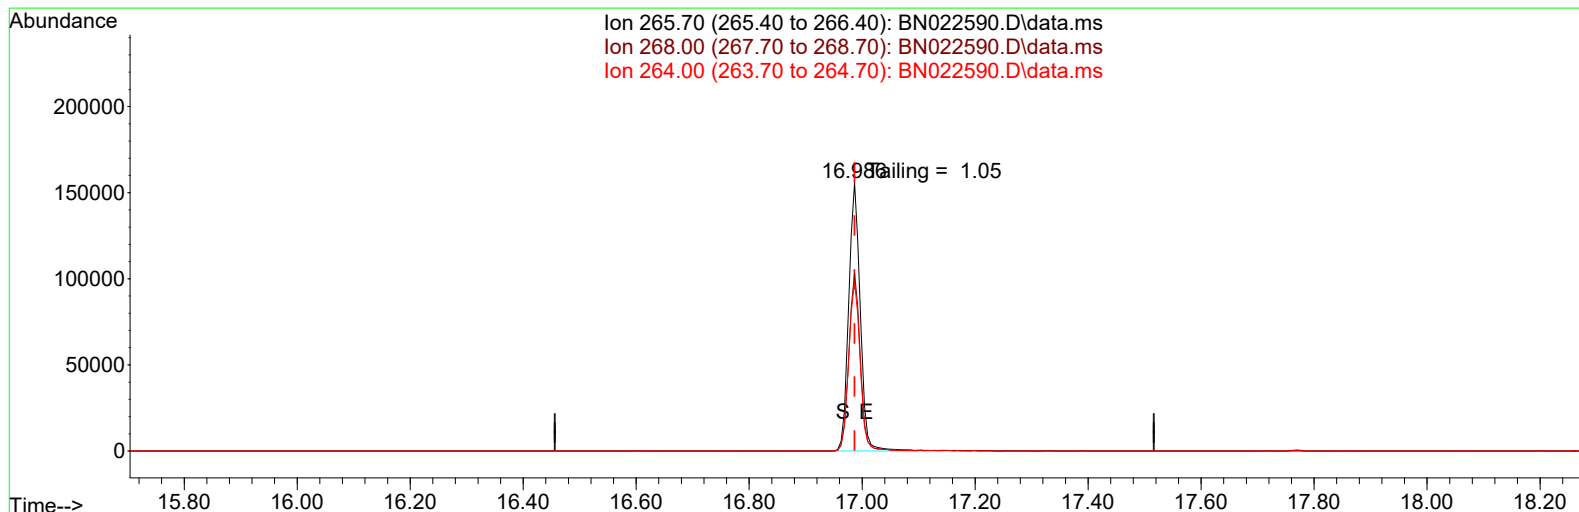

TIC: BN022590.D\data.ms

(70) Pentachlorophenol (C)




16.986min (0.000) 17653.78 ng

response 222222

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.18
264.00	61.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
Data File : BN022590.D
Acq On : 10 Nov 2022 08:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 05:20:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 05:20:15 2022
Response via : Initial Calibration

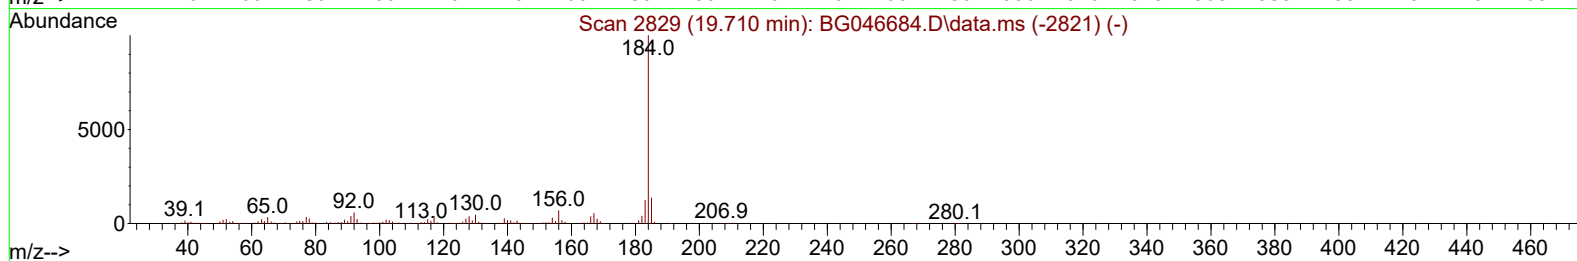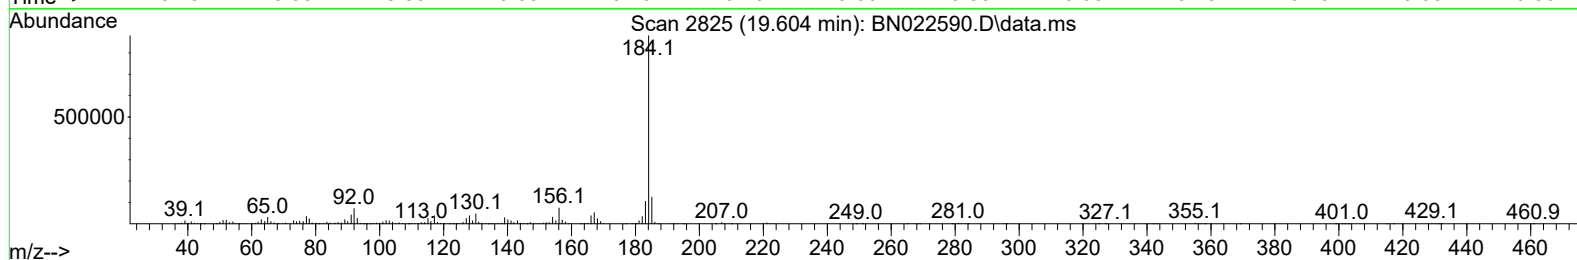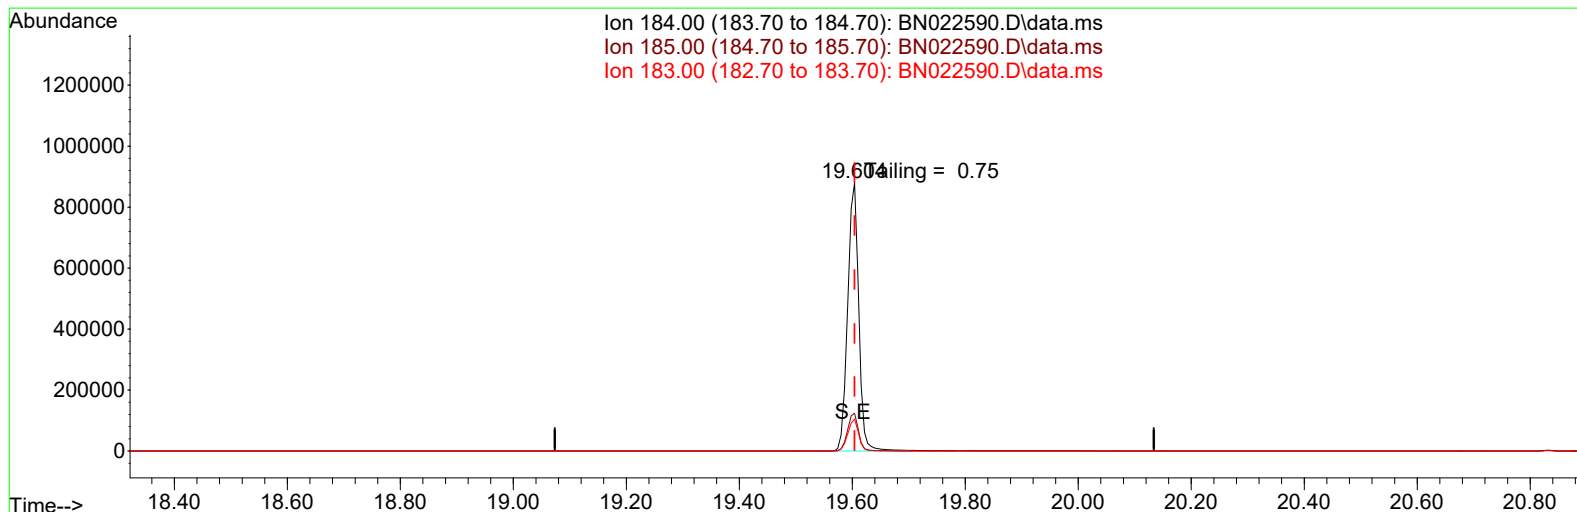

TIC: BN022590.D\data.ms

(77) Benzidine

19.604min (0.000) 0.00 ng

response 1201047

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.97
0.00	0.00	0.00